

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
 Data File : BP008881.D
 Acq On : 24 Jan 2022 11:45
 Operator : CG/JU
 Sample : PB142153BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142153BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	8	12	22	rVB	236082	303001	2.24%	0.445%
2	4.052	176	181	188	rVB	196743	263925	1.95%	0.387%
3	5.434	409	416	437	rBV	4888043	7535607	55.68%	11.060%
4	7.028	679	687	713	rBV	4342085	7263146	53.67%	10.660%
5	7.846	819	826	838	rBV	1015819	1671332	12.35%	2.453%
6	9.010	1015	1024	1049	rBV	2689916	4846815	35.81%	7.114%
7	10.646	1294	1302	1323	rBV	1142097	2145065	15.85%	3.148%
8	13.110	1711	1721	1745	rBV	7379806	11694889	86.42%	17.165%
9	14.487	1948	1955	1979	rBV	1652354	2682352	19.82%	3.937%
10	15.981	2202	2209	2240	rBV	4366549	7782245	57.50%	11.422%
11	17.245	2417	2424	2438	rBV	1892447	2861011	21.14%	4.199%
12	19.804	2854	2859	2871	rBV	10658594	13533387	100.00%	19.863%
13	21.339	3115	3120	3129	rBV	1872097	2645018	19.54%	3.882%
14	23.757	3525	3531	3544	rVB	1340872	2905437	21.47%	4.264%




Sum of corrected areas: 68133230

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008881.D
Acq On : 24 Jan 2022 11:45
Operator : CG/JU
Sample : PB142153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142153BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

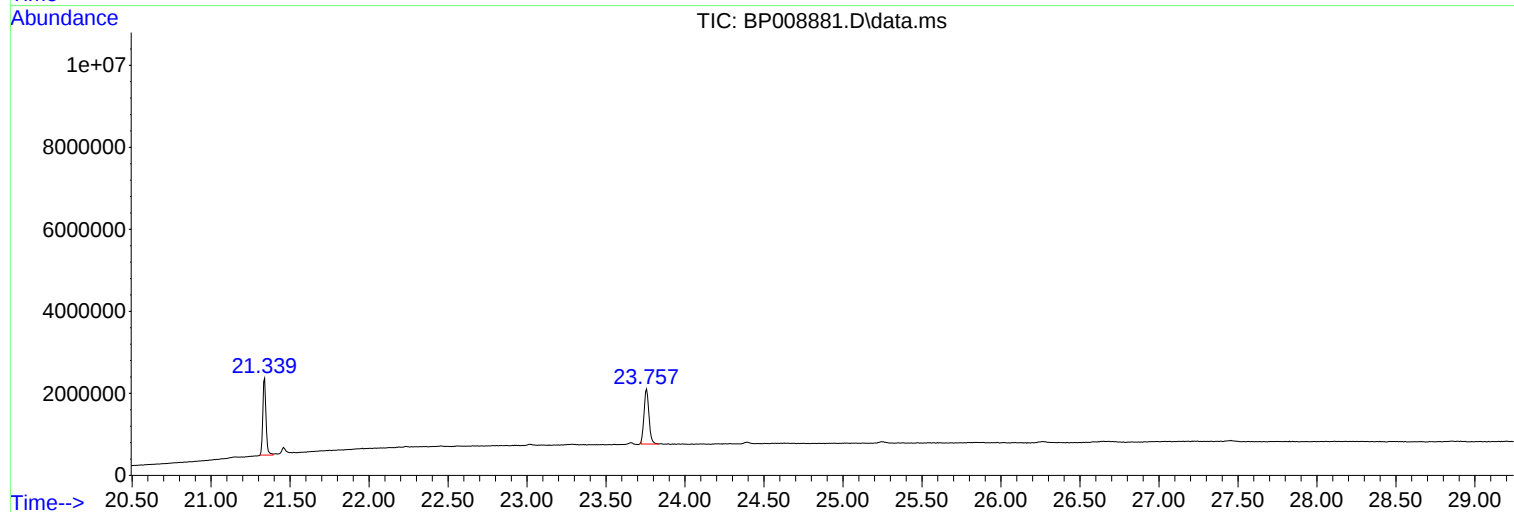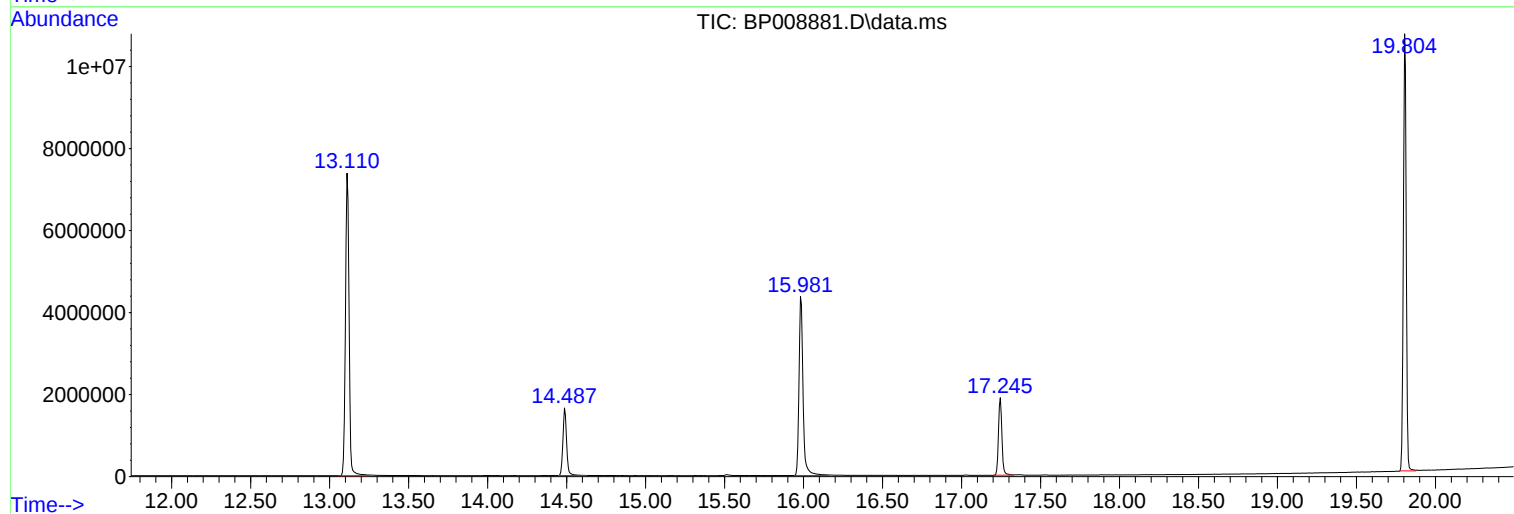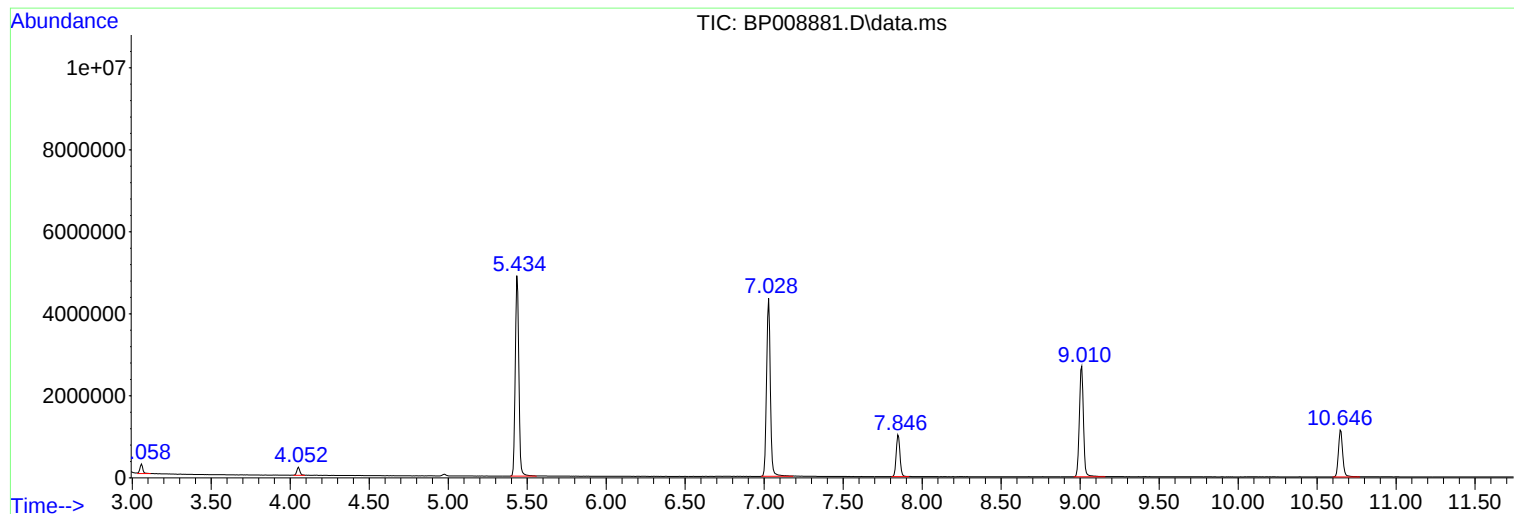

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008881.D
Acq On : 24 Jan 2022 11:45
Operator : CG/JU
Sample : PB142153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142153BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.058	3.63 ng	303001	1,4-Dichlorobenzene-d4	7.846

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

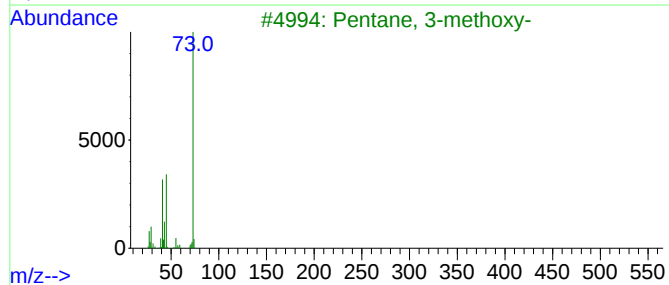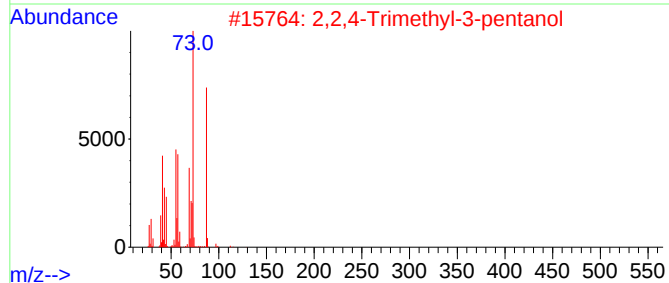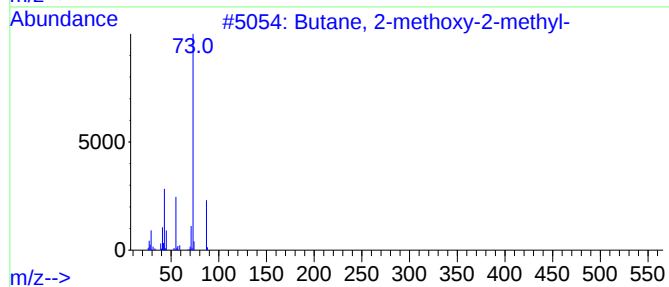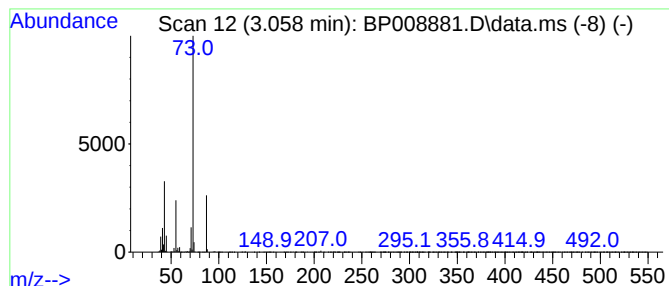

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008881.D
Acq On : 24 Jan 2022 11:45
Operator : CG/JU
Sample : PB142153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142153BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.058	3.6	ng	303001	1	7.846	1671330	20.0