

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
 Data File : BP008882.D
 Acq On : 24 Jan 2022 12:18
 Operator : CG/JU
 Sample : PB142174BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142174BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	8	12	21	rVB	242410	294437	1.59%	0.356%
2	4.052	176	181	191	rVB	196068	270620	1.46%	0.327%
3	5.434	409	416	433	rBV	5398285	8193680	44.16%	9.912%
4	7.028	678	687	709	rBV	4671730	8125621	43.79%	9.829%
5	7.846	819	826	841	rBV	1126872	1821303	9.82%	2.203%
6	9.005	1015	1023	1045	rBV	3105410	5442760	29.33%	6.584%
7	10.646	1292	1302	1321	rBV	1345022	2439465	13.15%	2.951%
8	13.110	1713	1721	1745	rBV	8969009	13816741	74.46%	16.714%
9	14.487	1947	1955	1978	rBV	2076853	3278284	17.67%	3.966%
10	15.981	2201	2209	2238	rBV	6105968	10039824	54.11%	12.145%
11	17.239	2417	2423	2437	rBV	2427010	3739476	20.15%	4.524%
12	19.804	2853	2859	2874	rBV	14580941	18555047	100.00%	22.446%
13	21.333	3114	3119	3128	rBV	2519266	3413581	18.40%	4.129%
14	23.751	3524	3530	3549	rVB2	1480889	3236013	17.44%	3.915%




Sum of corrected areas: 82666852

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008882.D
Acq On : 24 Jan 2022 12:18
Operator : CG/JU
Sample : PB142174BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

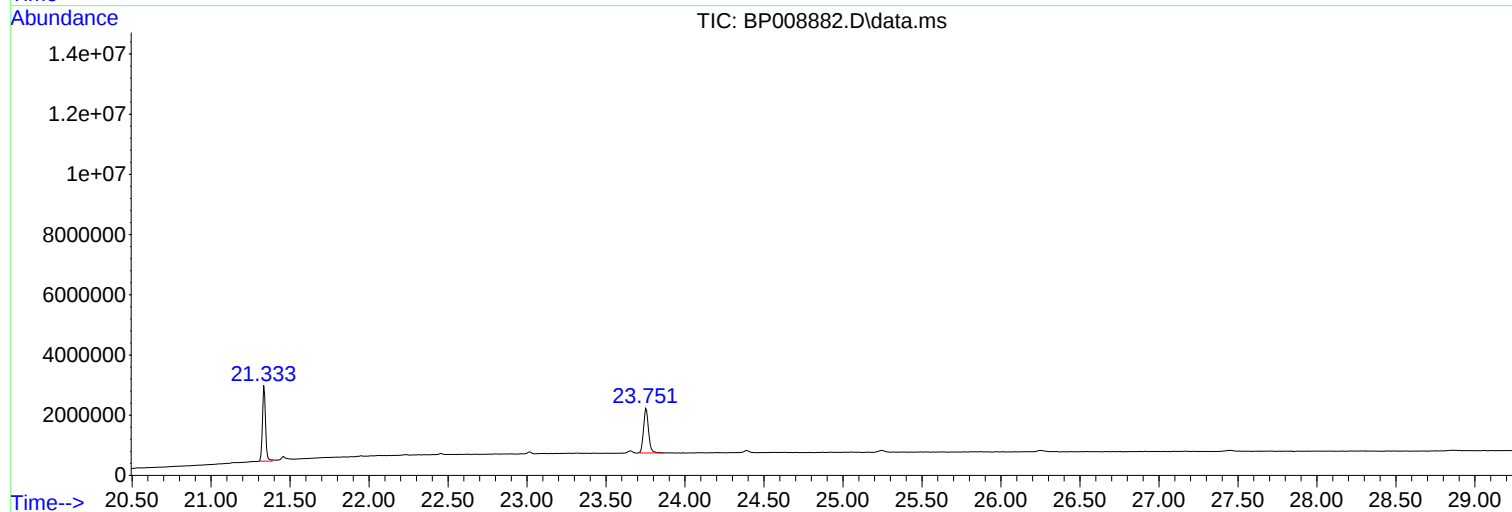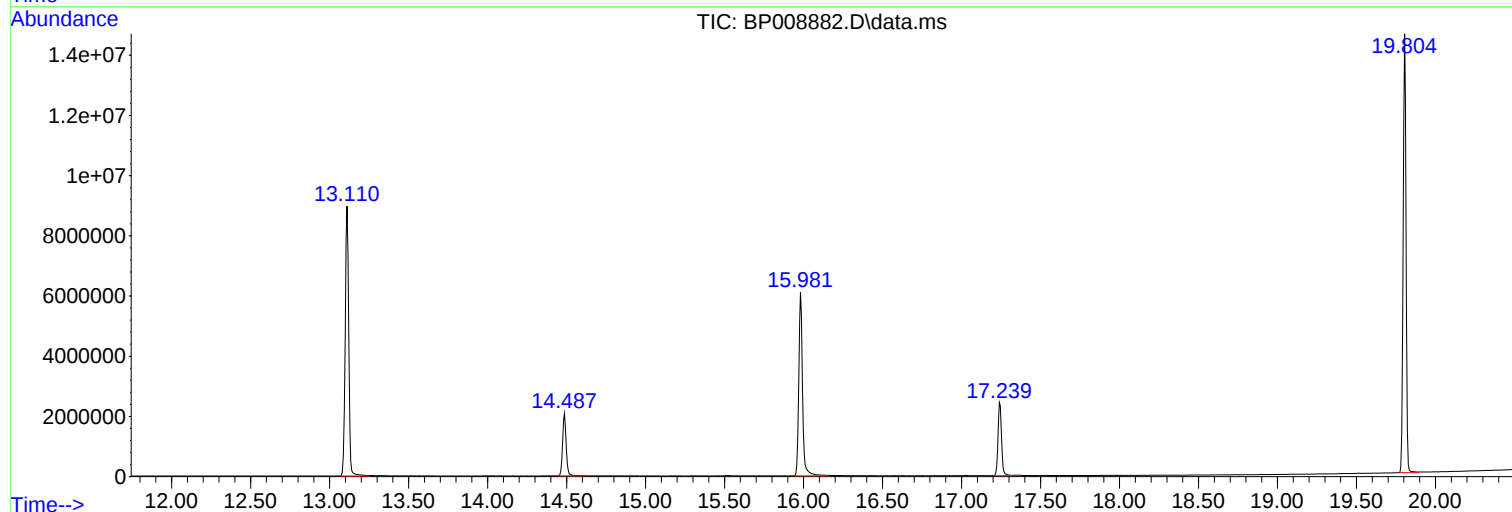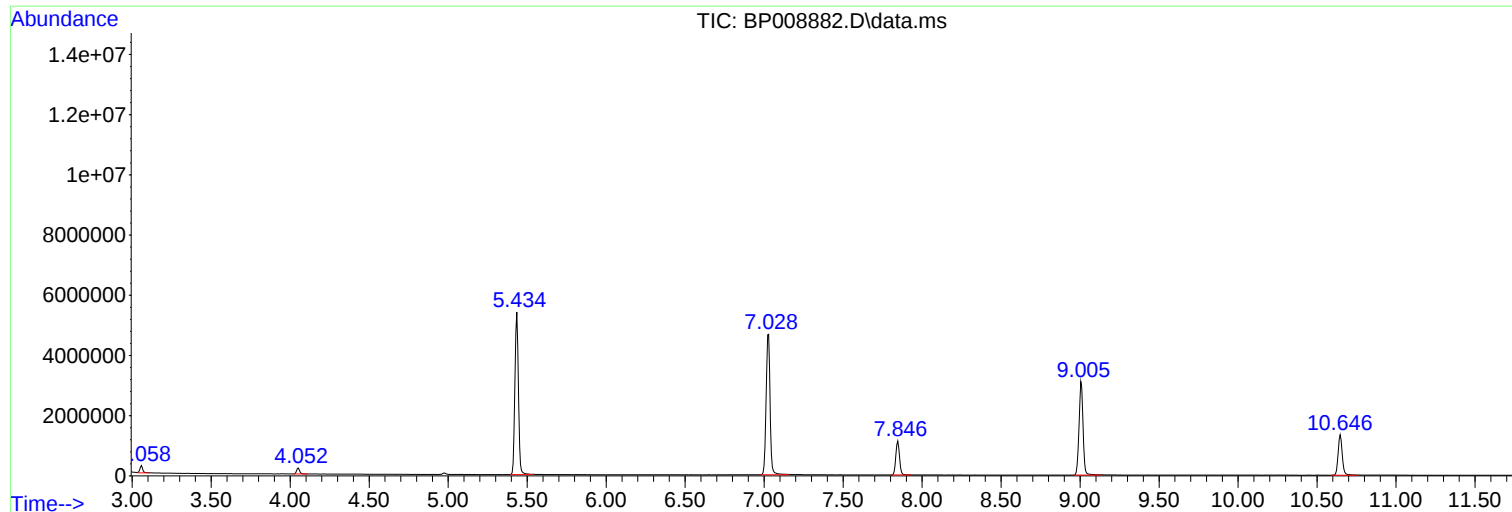

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008882.D
Acq On : 24 Jan 2022 12:18
Operator : CG/JU
Sample : PB142174BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142174BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.058	3.23 ng	294437	1,4-Dichlorobenzene-d4	7.846

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
3			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	22
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

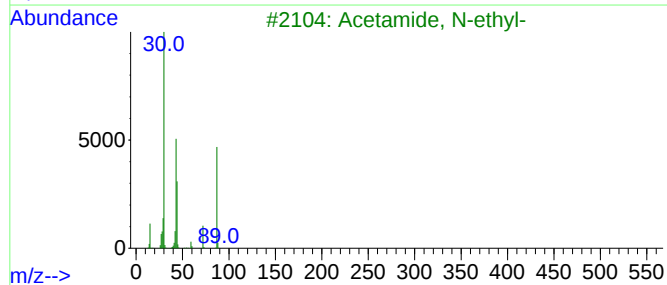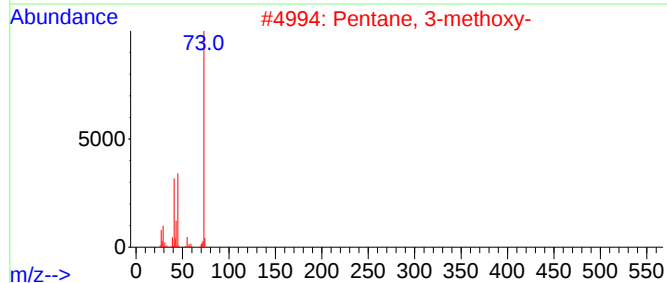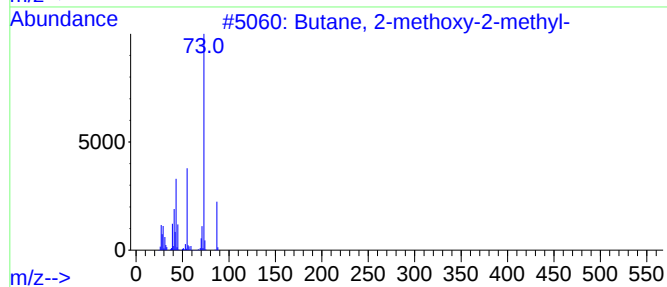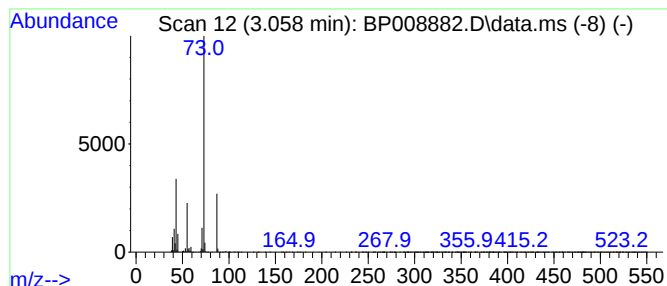

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008882.D
Acq On : 24 Jan 2022 12:18
Operator : CG/JU
Sample : PB142174BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.058	3.2	ng	294437	1	7.846	1821300	20.0