

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
 Data File : BP008896.D
 Acq On : 24 Jan 2022 20:20
 Operator : CG/JU
 Sample : N1243-09 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 AMI-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008896.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	7	11	24	rVB	144386	255881	4.07%	0.701%
2	5.434	410	416	433	rBV	836816	1406310	22.38%	3.851%
3	7.028	680	687	701	rBV	771162	1432322	22.80%	3.922%
4	7.852	818	827	836	rBV	1409758	2343806	37.31%	6.418%
5	9.010	1017	1024	1047	rBV	500588	932123	14.84%	2.552%
6	10.651	1295	1303	1319	rBV	1804874	3239791	51.57%	8.871%
7	13.110	1715	1721	1734	rBV	1650938	2601500	41.41%	7.123%
8	14.216	1903	1909	1915	rBV	35773	73996	1.18%	0.203%
9	14.492	1949	1956	1976	rBV	2828418	4350687	69.25%	11.913%
10	15.987	2204	2210	2227	rBV	1026694	1710488	27.23%	4.683%
11	16.216	2245	2249	2251	rBV2	51563	73189	1.16%	0.200%
12	17.063	2391	2393	2402	rVB5	40374	65945	1.05%	0.181%
13	17.251	2419	2425	2435	rBV	2935278	4470753	71.16%	12.241%
14	18.145	2573	2577	2584	rBV3	128922	229463	3.65%	0.628%
15	19.810	2855	2860	2865	rBV	2322801	2828629	45.02%	7.745%
16	21.339	3117	3120	3136	rVB	3626901	6282582	100.00%	17.202%
17	23.768	3528	3533	3540	rVB2	2074452	4224236	67.24%	11.566%




Sum of corrected areas: 36521701

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008896.D
Acq On : 24 Jan 2022 20:20
Operator : CG/JU
Sample : N1243-09 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
AMI-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

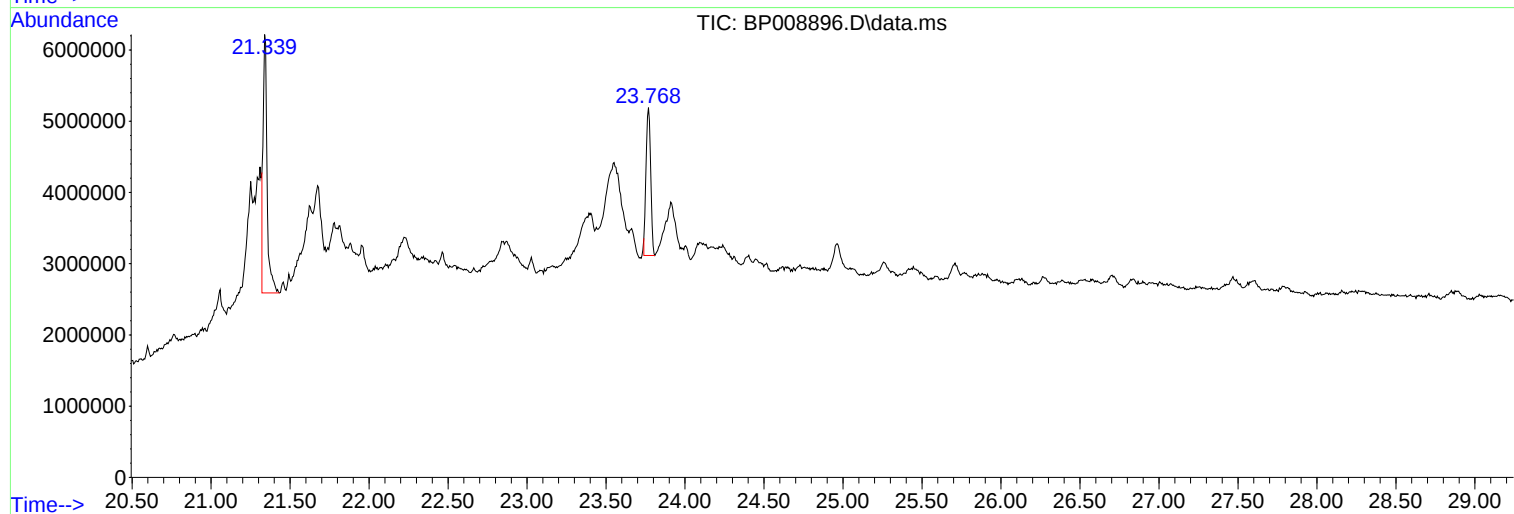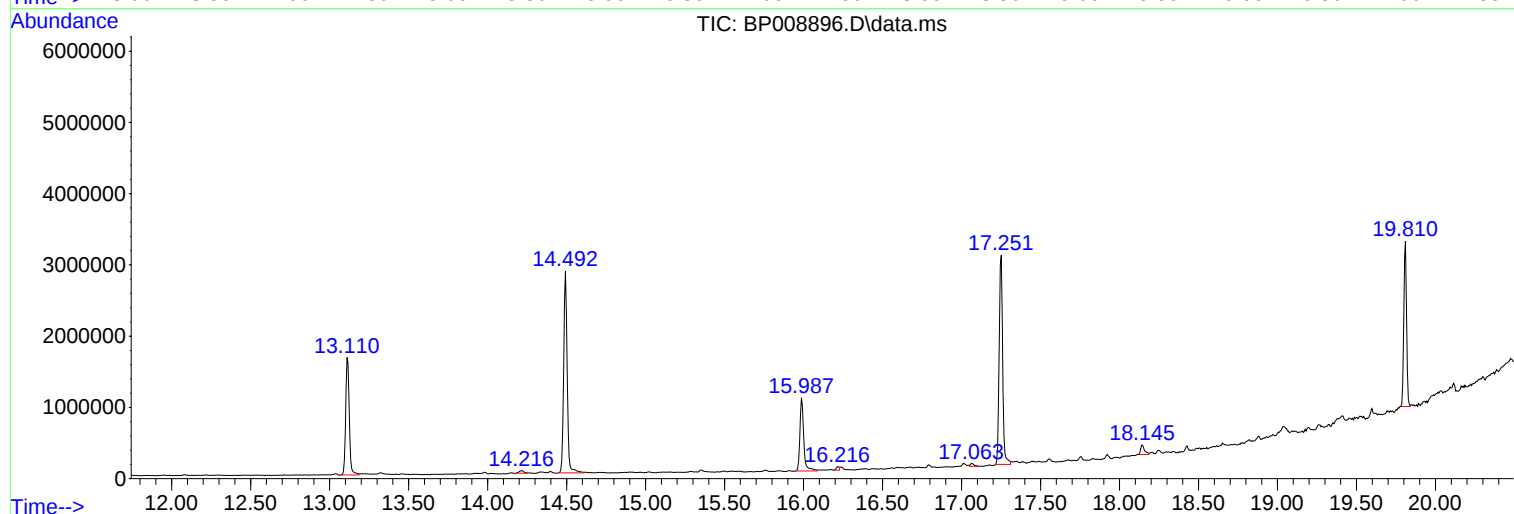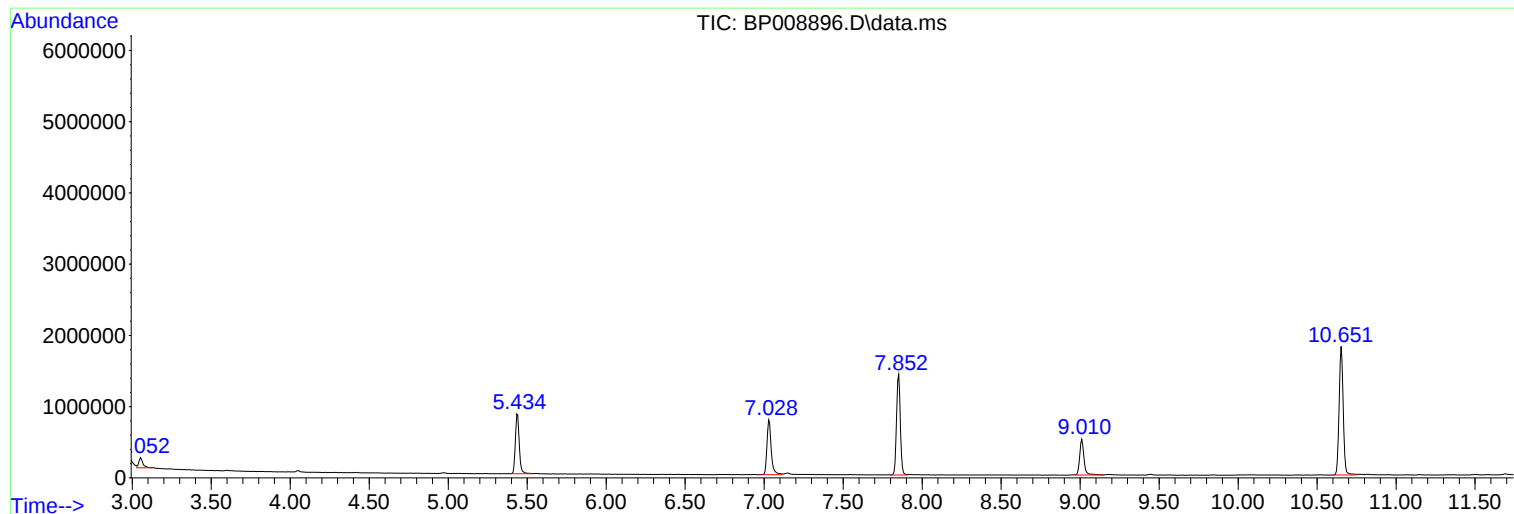

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008896.D
Acq On : 24 Jan 2022 20:20
Operator : CG/JU
Sample : N1243-09 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
AMI-3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.052	2.18 ng	255881	1,4-Dichlorobenzene-d4	7.852

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	53
2			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

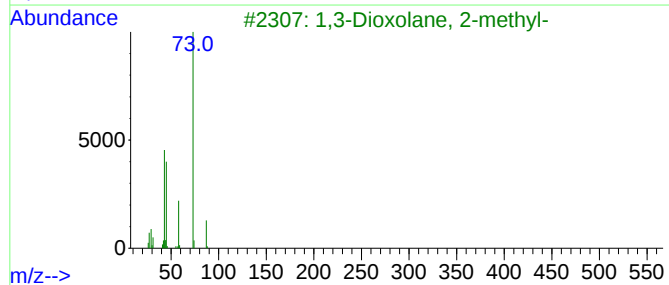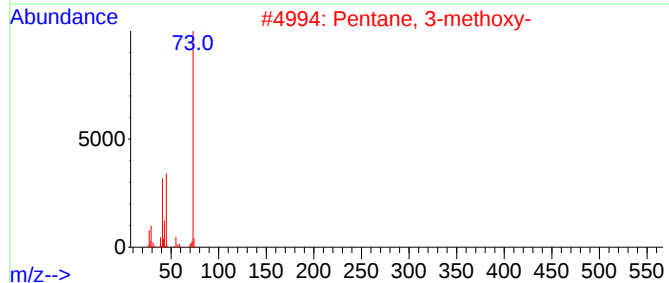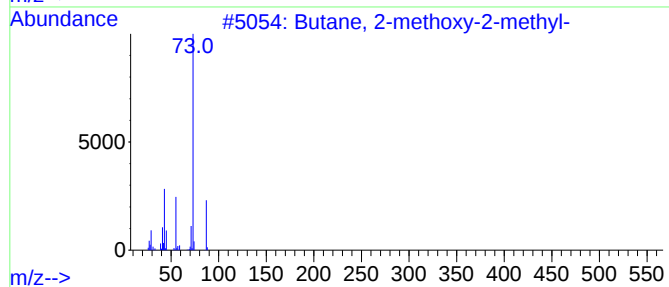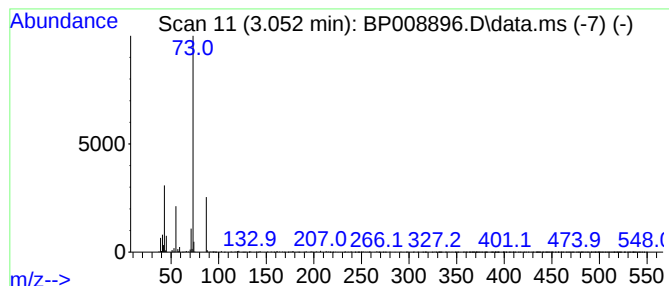

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008896.D
Acq On : 24 Jan 2022 20:20
Operator : CG/JU
Sample : N1243-09 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
AMI-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.052	2.2	ng	255881	1	7.852	2343810	20.0