
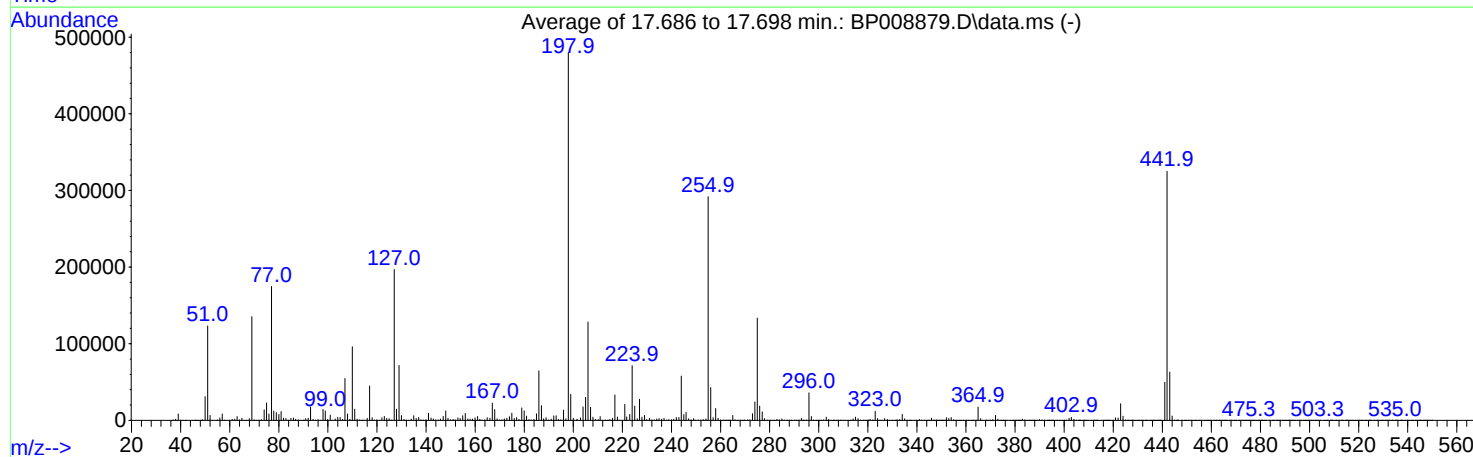


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
 Data File : BP008879.D
 Acq On : 24 Jan 2022 10:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 26 01:52:51 2022

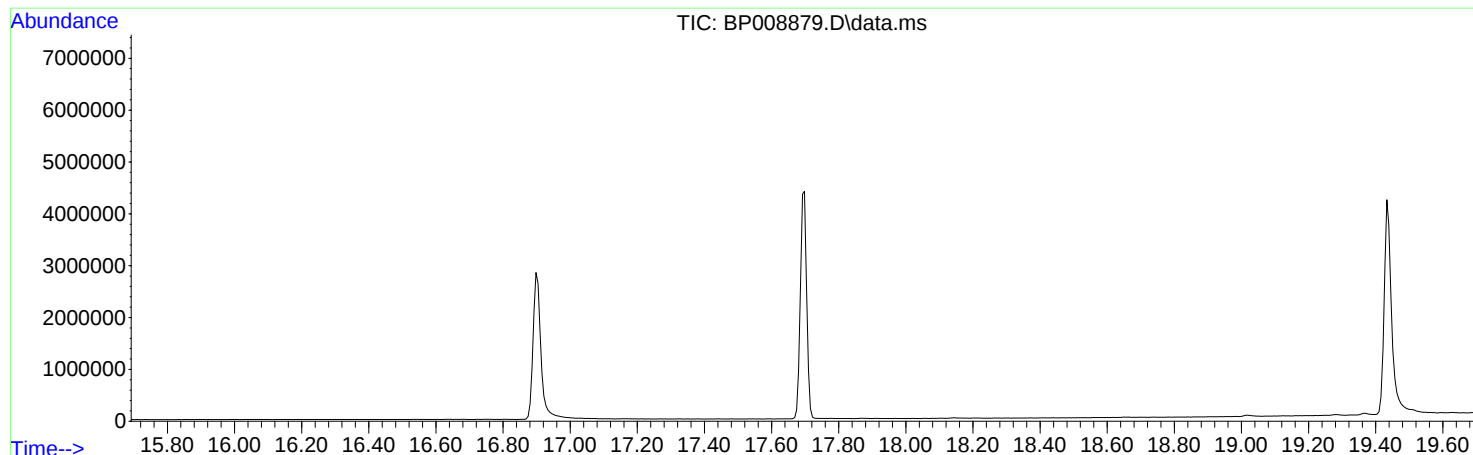


AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	123142	PASS
68	69	0.00	2	1.7	2249	PASS
69	198	0.00	100	28.2	135386	PASS
70	69	0.00	2	0.5	709	PASS
127	198	10	80	41.0	196821	PASS
197	198	0.00	2	0.5	2166	PASS
198	198	100	100	100.0	480010	PASS
199	198	5	9	7.0	33737	PASS
275	198	10	60	27.8	133343	PASS
365	198	1	100	3.6	17400	PASS
441	198	0.01	100	10.4	49789	PASS
442	442	100	100	100.0	325131	PASS
443	442	15	24	19.4	63024	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008879.D
Acq On : 24 Jan 2022 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 24 17:10:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

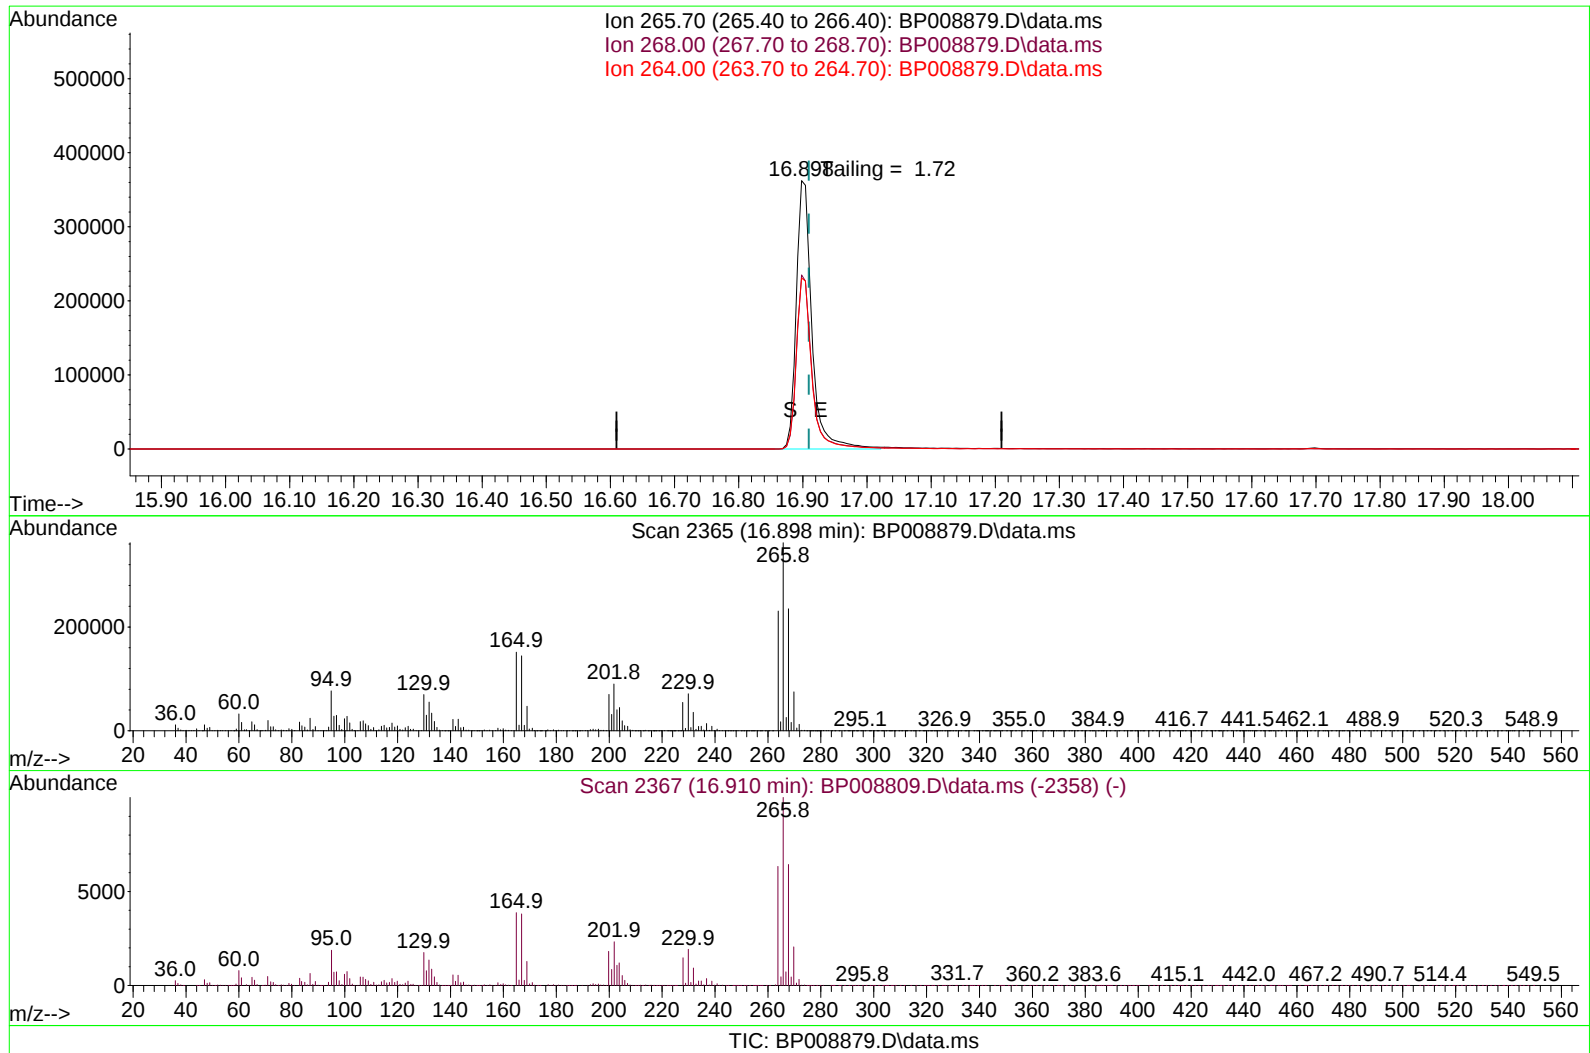

(70) Pentachlorophenol (C)

16.898min (-0.012) 272033.44 ng




response 617874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.89
264.00	62.90	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
 Data File : BP008879.D
 Acq On : 24 Jan 2022 10:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 24 17:10:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 14 18:05:00 2022
 Response via : Initial Calibration

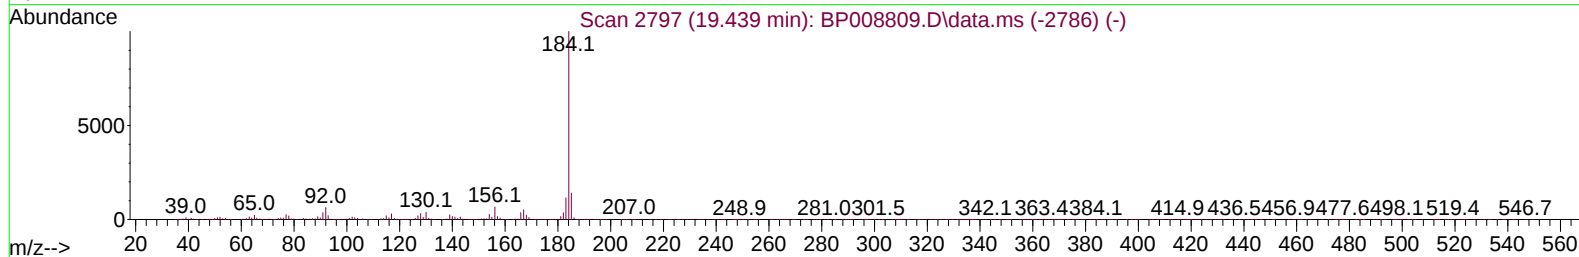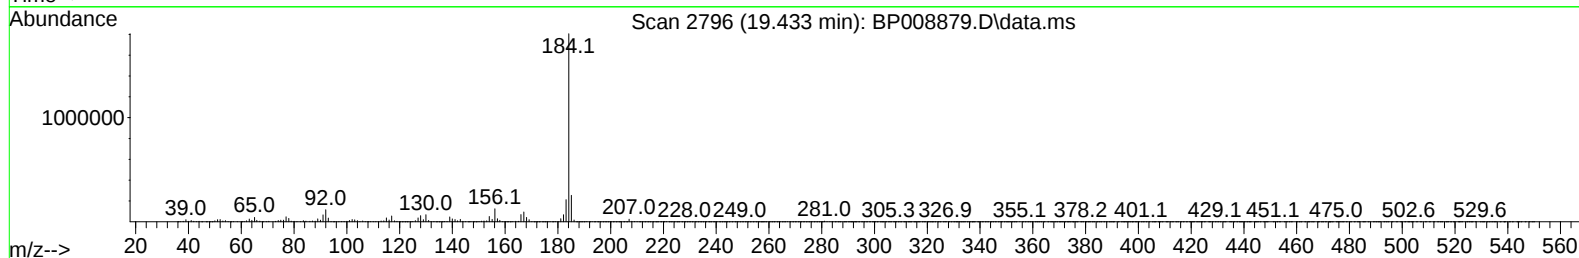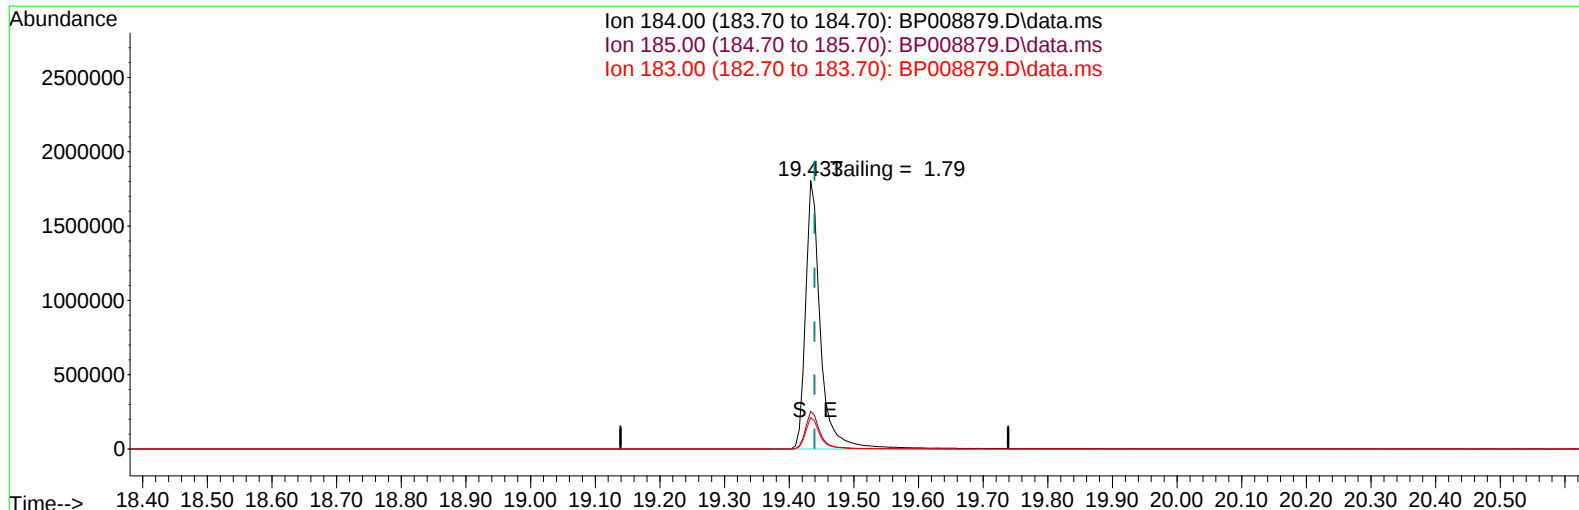

TIC: BP008879.D\data.ms

(77) Benzidine

19.433min (-0.006) 60654.00 ng

response 2890599

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.03
183.00	11.90	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2022	BNA_P	<u>BP008879.D</u>
Compound Name	Response	Retention Time
DDT	1726015	20.63
DDD	79392	20.21
DDE	5469	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
84861	1810876	4.69

Instrument :
BNA_P
ClientSampleId :
DFTPP