
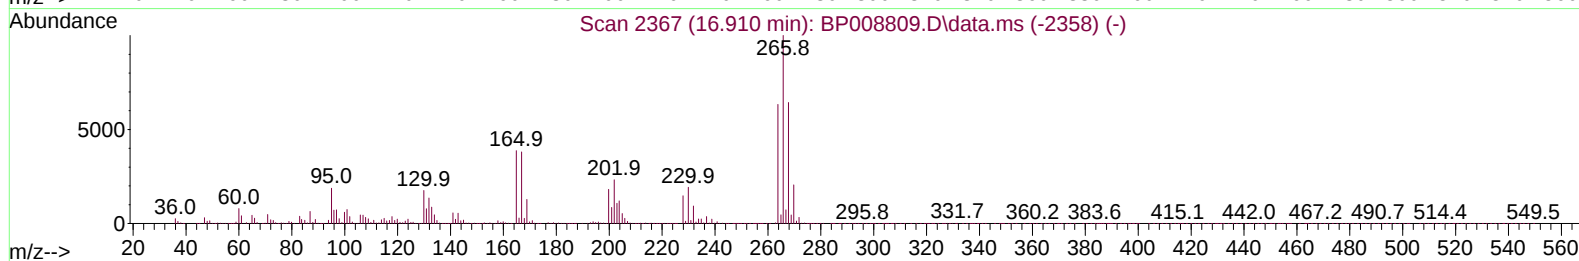
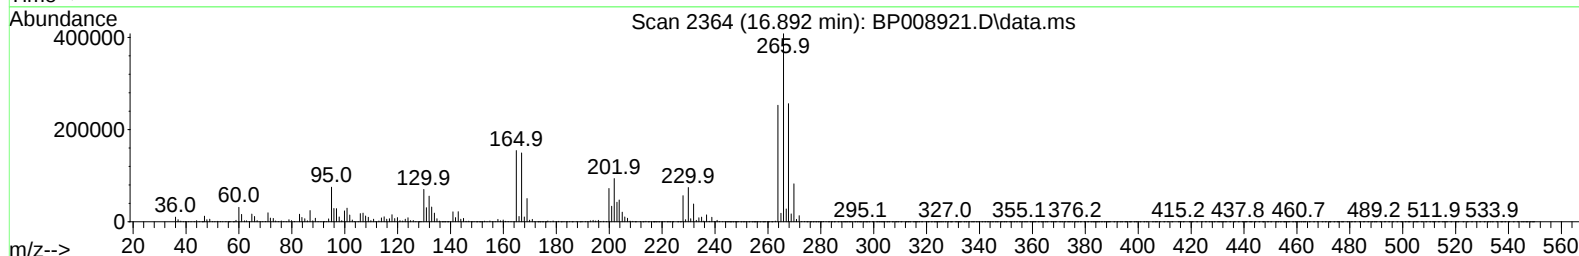


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008921.D
Acq On : 26 Jan 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:32:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration

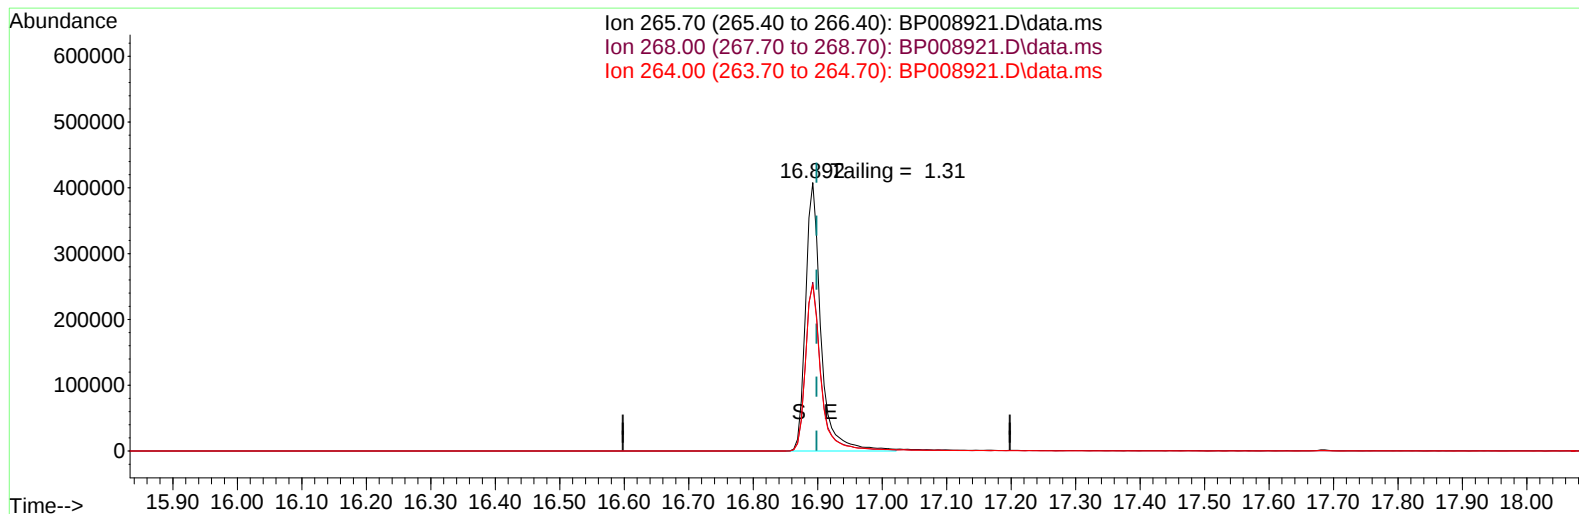

TIC: BP008921.D\data.ms

(70) Pentachlorophenol (C)




16.892min (-0.006) 218943.47 ng

response 682522

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.85
264.00	62.90	62.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008921.D
Acq On : 26 Jan 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:32:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration

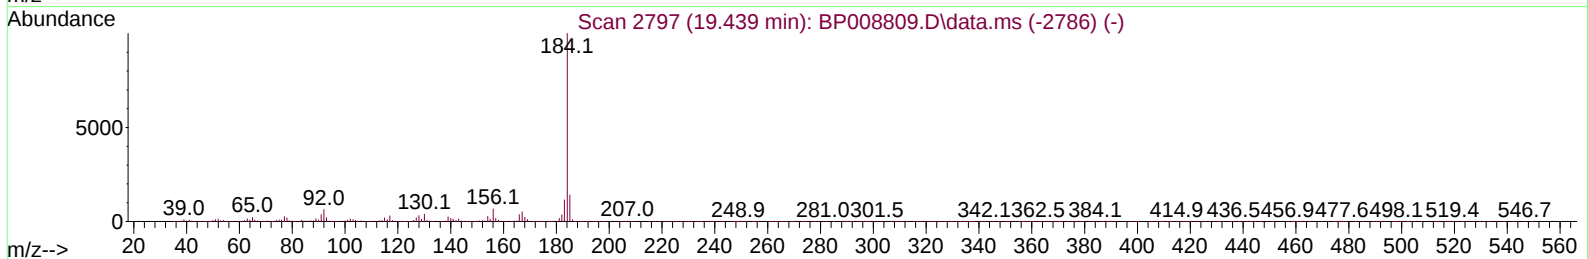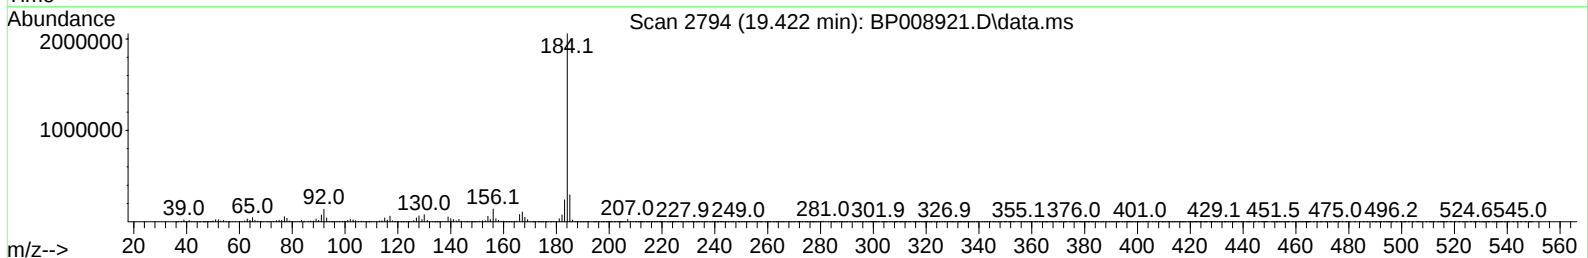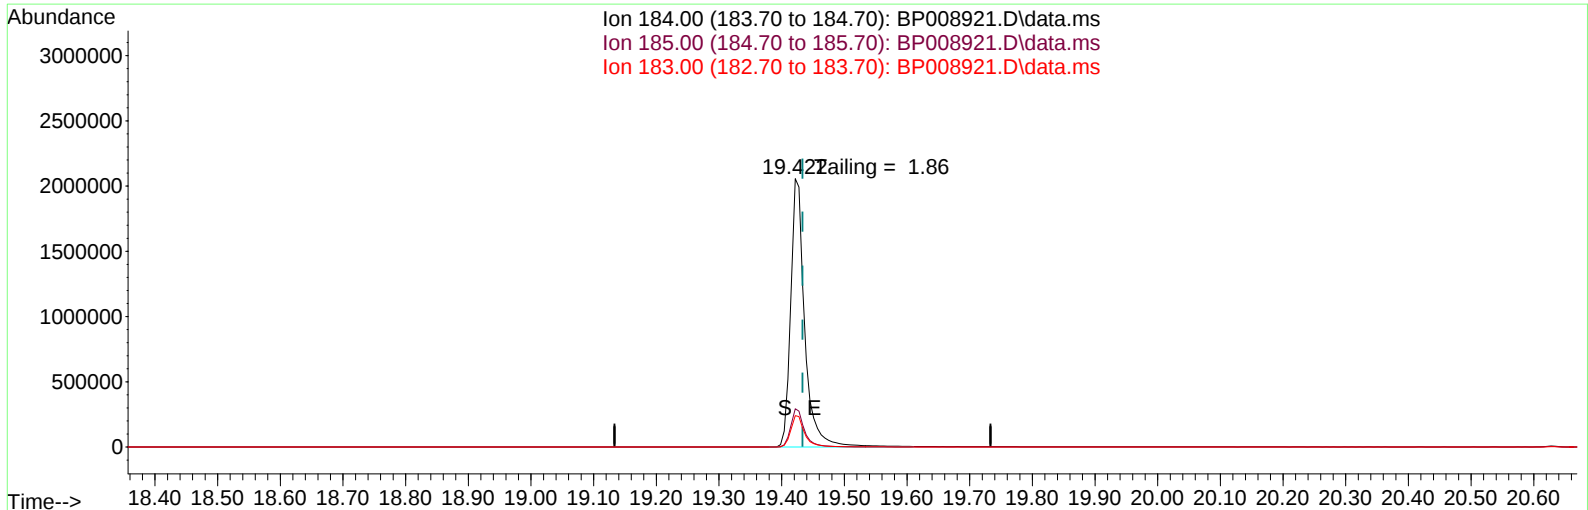

TIC: BP008921.D\data.ms

(77) Benzidine**19.422min (-0.012) 34236.17 ng****response 3236590**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.28
183.00	11.90	11.70
0.00	0.00	0.00