

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
 Data File : BP008937.D
 Acq On : 26 Jan 2022 19:26
 Operator : CG/JU
 Sample : N1267-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RED-EXT-WALL

Quant Time: Jan 27 05:23:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 01:52:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	214672	20.000	ng	0.00
21) Naphthalene-d8	10.634	136	832324	20.000	ng	0.00
39) Acenaphthene-d10	14.475	164	529185	20.000	ng	0.00
64) Phenanthrene-d10	17.228	188	1130706	20.000	ng	-0.01
76) Chrysene-d12	21.322	240	1226525	20.000	ng	-0.01
86) Perylene-d12	23.727	264	1286689	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	1386485	99.877	ng	0.00
7) Phenol-d6	7.011	99	1713948	101.959	ng	-0.01
23) Nitrobenzene-d5	8.993	82	1050440	71.651	ng	0.00
42) 2,4,6-Tribromophenol	15.969	330	821852	106.695	ng	-0.01
45) 2-Fluorobiphenyl	13.098	172	2762178	68.834	ng	0.00
79) Terphenyl-d14	19.792	244	4651274	64.011	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008937.D
Acq On : 26 Jan 2022 19:26
Operator : CG/JU
Sample : N1267-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RED-EXT-WALL

Quant Time: Jan 27 05:23:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration




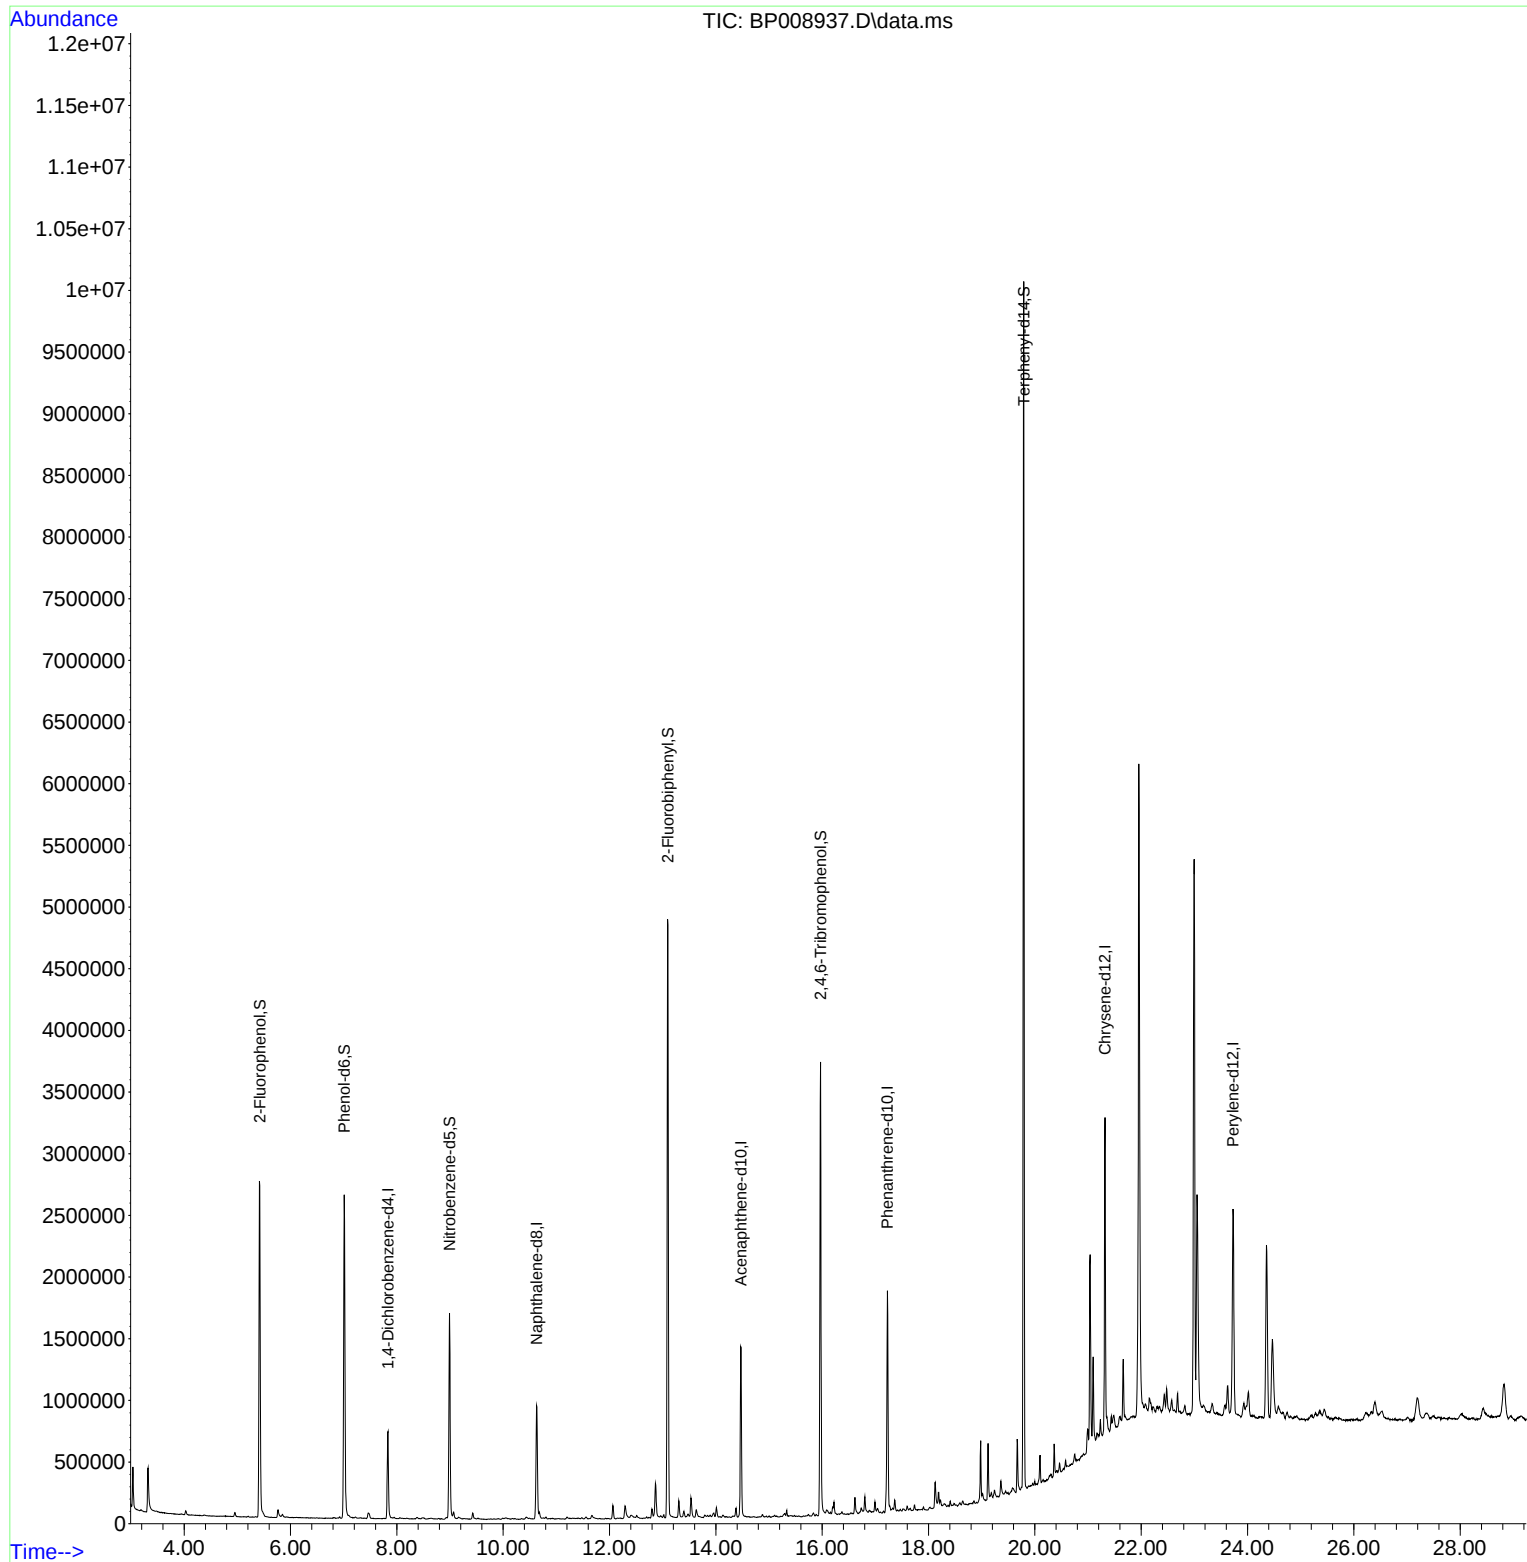




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.834 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26




Instrument :
BNA_P
ClientSampleId :
RED-EXT-WALL


Tgt Ion:152 Resp: 214672
Ion Ratio Lower Upper
152 100
150 154.5 127.0 190.6
115 53.7 43.7 65.5

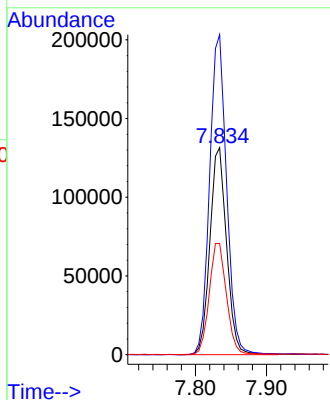

#5
2-Fluorophenol
Concen: 99.877 ng
RT: 5.422 min Scan# 414
Delta R.T. -0.006 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26

Tgt Ion:112 Resp: 1386485
Ion Ratio Lower Upper
112 100
64 49.5 39.7 59.5
63 26.4 20.0 30.0

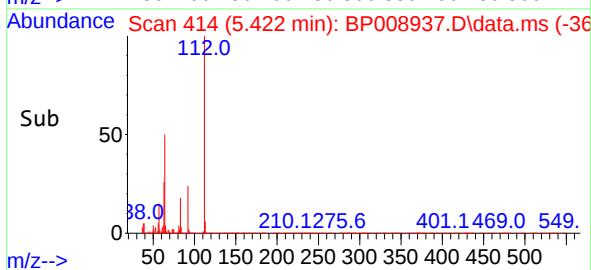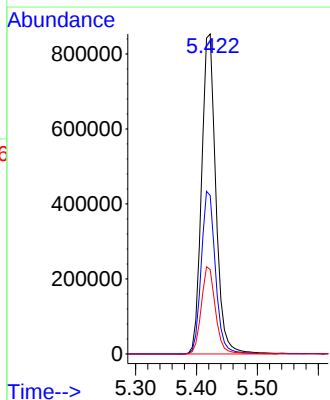







#7
Phenol-d6
Concen: 101.959 ng
RT: 7.011 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26

Instrument :
BNA_P
ClientSampleId :
RED-EXT-WALL

Tgt Ion: 99 Resp: 1713948




Ion	Ratio	Lower	Upper
99	100		
42	15.5	10.8	16.2
71	31.1	23.8	35.6

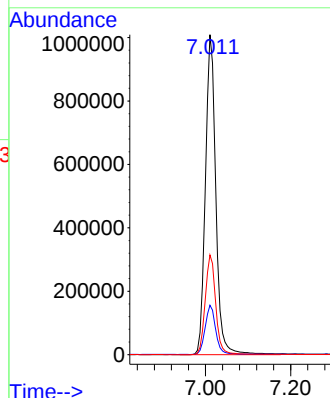


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.634 min Scan# 1300
Delta R.T. -0.006 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26

Tgt Ion:136 Resp: 832324

Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.0	13.4
54	6.2	4.9	7.3
68	5.3	4.3	6.5


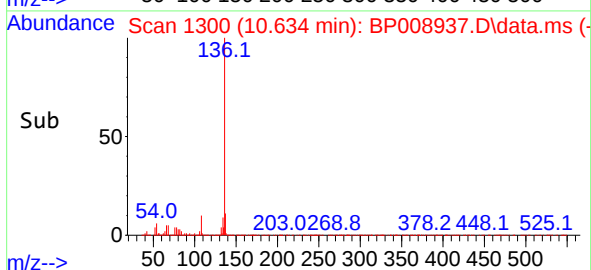
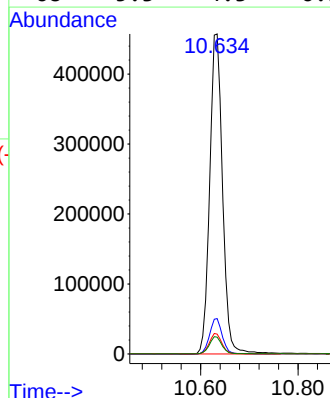





#23
Nitrobenzene-d5
Concen: 71.651 ng
RT: 8.993 min Scan# 1021
Delta R.T. -0.006 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26




Instrument :
BNA_P
ClientSampleId :
RED-EXT-WALL


Tgt Ion: 82 Resp: 1050440
Ion Ratio Lower Upper
82 100
128 46.9 39.4 59.2
54 43.1 32.6 48.8

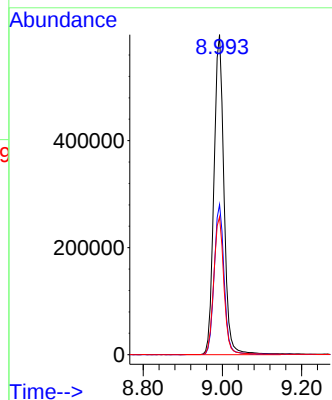

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.475 min Scan# 1953
Delta R.T. -0.006 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26

Tgt Ion:164 Resp: 529185
Ion Ratio Lower Upper
164 100
162 99.9 79.9 119.9
160 44.8 35.5 53.3


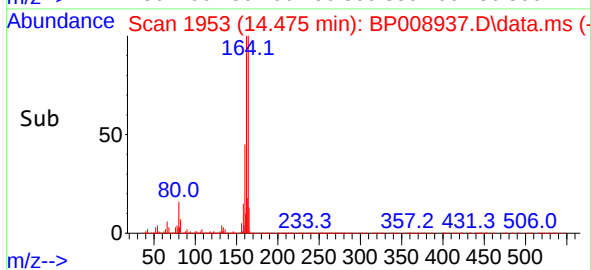
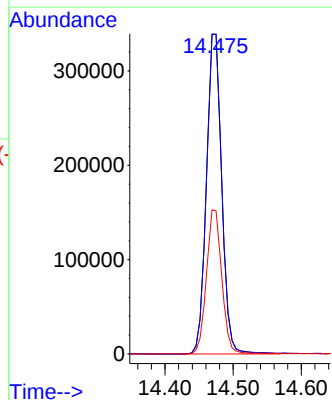





#42
2,4,6-Tribromophenol
Concen: 106.695 ng
RT: 15.969 min Scan# 21
Delta R.T. -0.012 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26




Instrument :
BNA_P
ClientSampleId :
RED-EXT-WALL


Tgt Ion:330 Resp: 821852
Ion Ratio Lower Upper
330 100
332 95.8 77.0 115.4
141 29.8 21.3 31.9

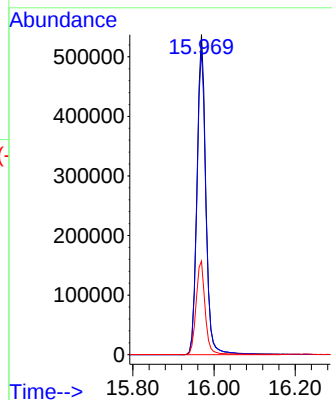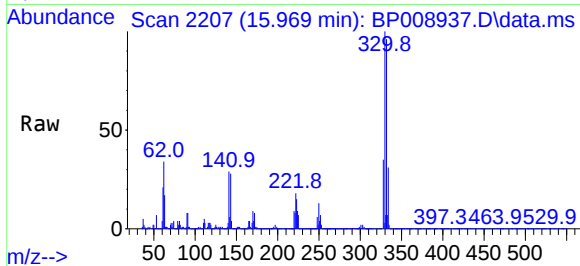

#45
2-Fluorobiphenyl
Concen: 68.834 ng
RT: 13.098 min Scan# 1719
Delta R.T. -0.006 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26

Tgt Ion:172 Resp: 2762178
Ion Ratio Lower Upper
172 100
171 35.0 29.3 43.9
170 23.4 19.5 29.3


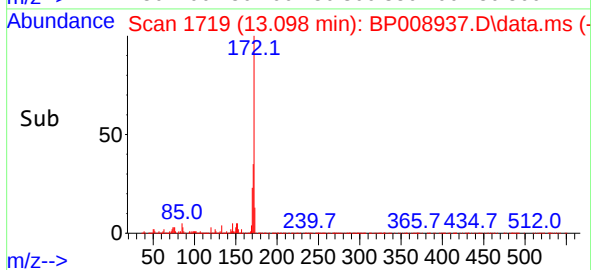
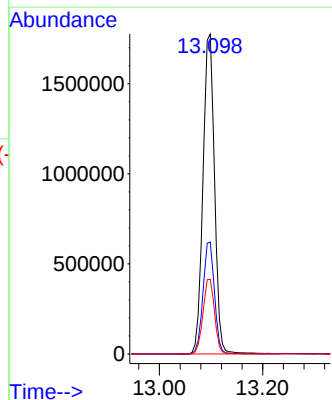
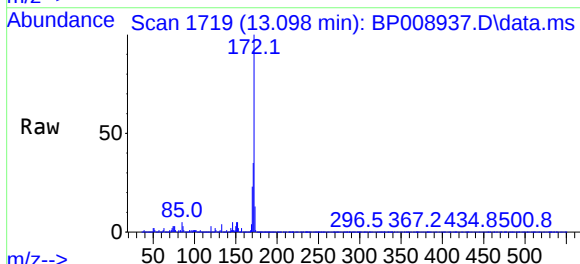




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.228 min Scan# 2425
Delta R.T. -0.012 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26




Instrument :
BNA_P
ClientSampleId :
RED-EXT-WALL


Tgt Ion:188 Resp: 1130706
Ion Ratio Lower Upper
188 100
94 7.8 6.8 10.2
80 8.1 7.2 10.8

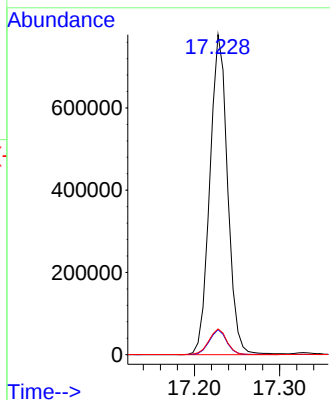

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.322 min Scan# 3117
Delta R.T. -0.012 min
Lab File: BP008937.D
Acq: 26 Jan 2022 19:26

Tgt Ion:240 Resp: 1226525
Ion Ratio Lower Upper
240 100
120 8.5 7.7 11.5
236 26.7 21.2 31.8


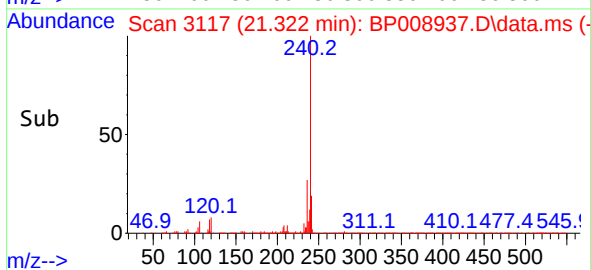
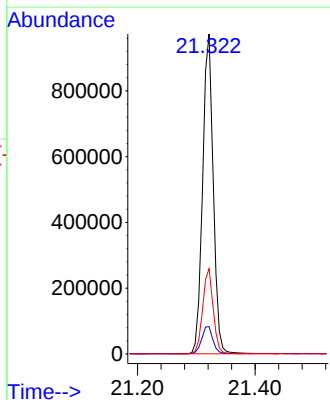





#79
 Terphenyl-d14
 Concen: 64.011 ng
 RT: 19.792 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP008937.D
 Acq: 26 Jan 2022 19:26

Instrument :
 BNA_P
 ClientSampleId :
 RED-EXT-WALL

Tgt Ion:244 Resp: 4651274
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.5 9.7
 122 8.7 9.2 13.8#

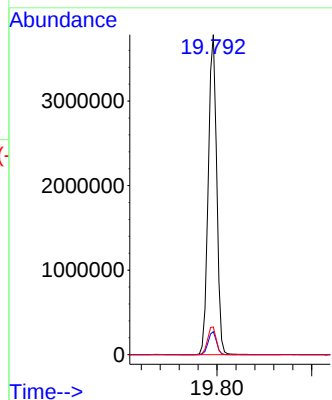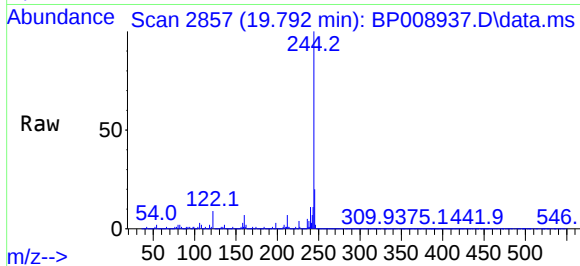

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.727 min Scan# 3526
 Delta R.T. -0.024 min
 Lab File: BP008937.D
 Acq: 26 Jan 2022 19:26

Tgt Ion:264 Resp: 1286689
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.1 28.7
 265 21.9 17.1 25.7

