

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
 Data File : BP008923.D
 Acq On : 26 Jan 2022 11:18
 Operator : CG/JU
 Sample : PB142251BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142251BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	6	10	22	rVB	258821	334052	1.81%	0.390%
2	5.422	407	414	434	rBV	5575807	8750490	47.41%	10.226%
3	7.016	677	685	712	rBV	4991199	8662669	46.93%	10.123%
4	7.834	817	824	835	rBV	1187438	1925701	10.43%	2.250%
5	8.999	1012	1022	1044	rBV	3361999	5850052	31.69%	6.836%
6	10.634	1293	1300	1320	rBV	1471537	2636093	14.28%	3.081%
7	13.098	1709	1719	1746	rBV	9486953	14752587	79.92%	17.240%
8	14.475	1946	1953	1970	rBV	2259772	3510107	19.02%	4.102%
9	15.975	2200	2208	2240	rBV	6629222	10635252	57.62%	12.428%
10	17.233	2415	2422	2436	rBV	2493579	3919660	21.23%	4.580%
11	19.798	2852	2858	2868	rBV	14709826	18458803	100.00%	21.571%
12	21.321	3113	3117	3125	rBV	2417517	3199481	17.33%	3.739%
13	23.733	3521	3527	3538	rVB2	1376544	2937808	15.92%	3.433%




Sum of corrected areas: 85572755

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008923.D
Acq On : 26 Jan 2022 11:18
Operator : CG/JU
Sample : PB142251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142251BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

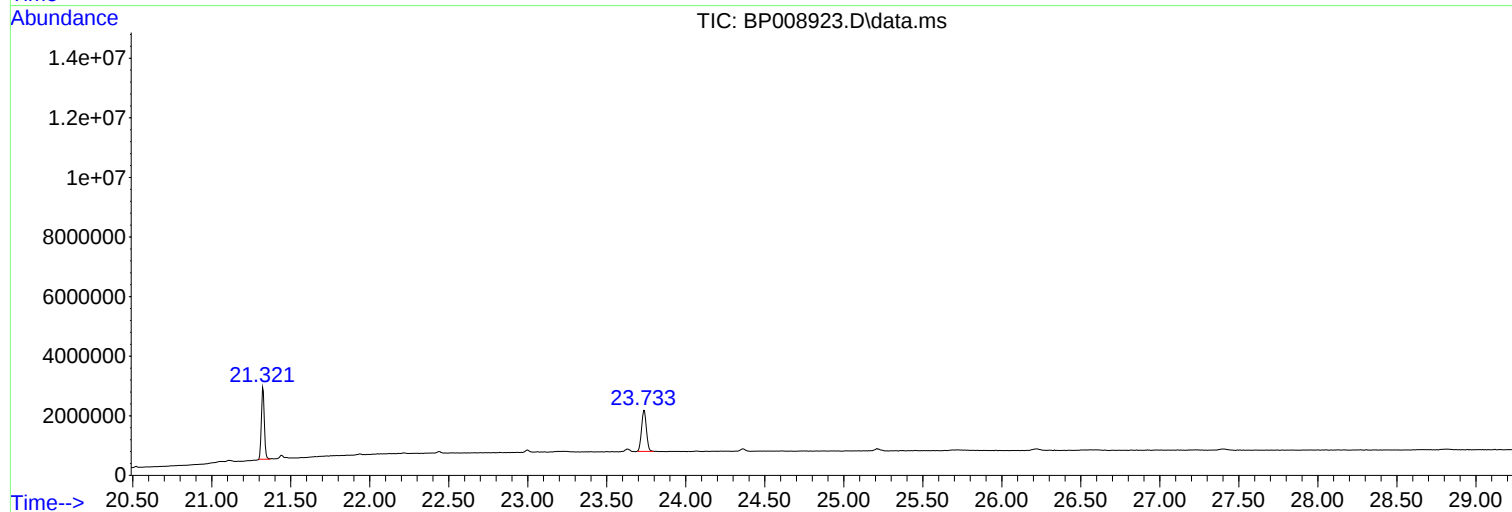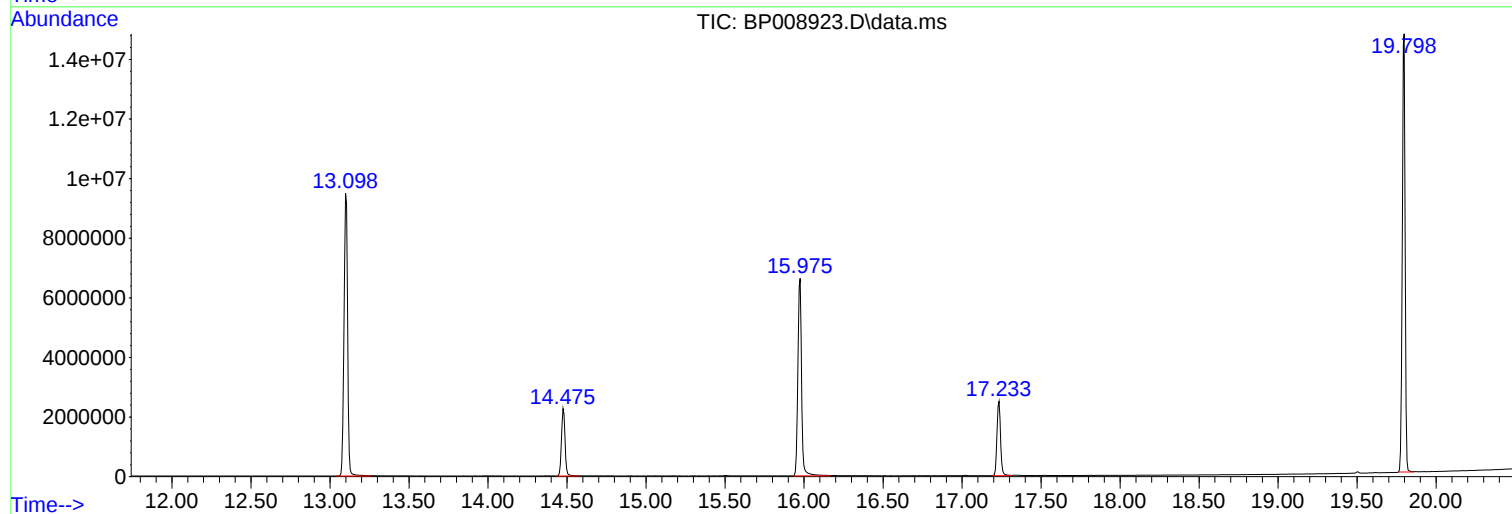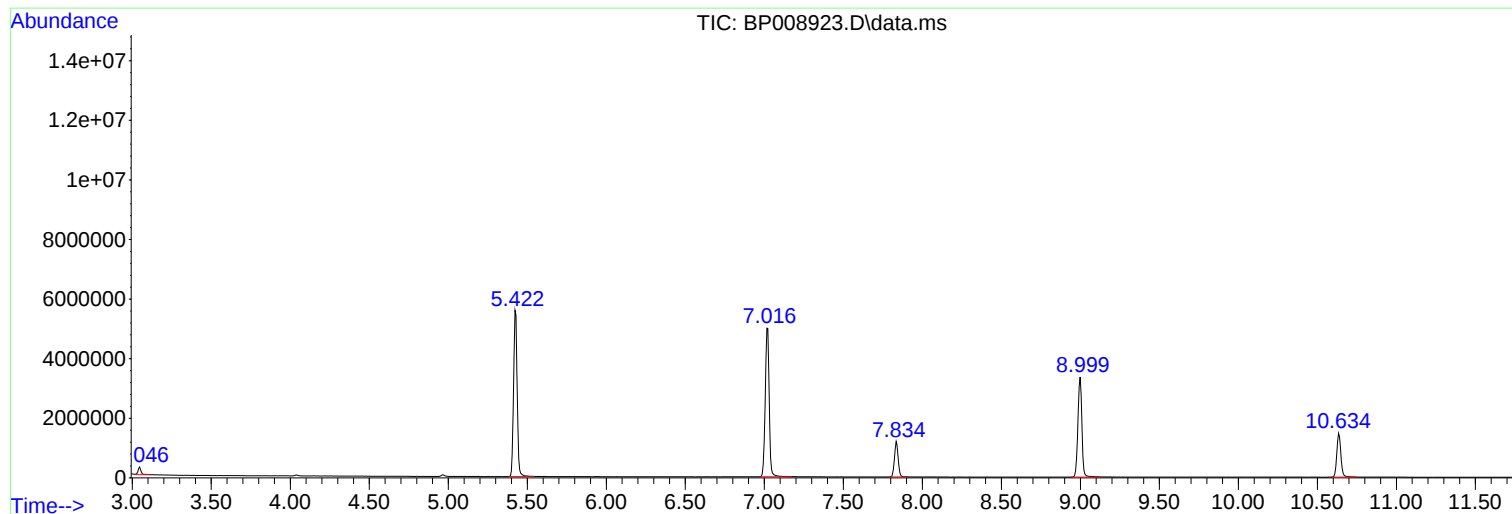

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008923.D
Acq On : 26 Jan 2022 11:18
Operator : CG/JU
Sample : PB142251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142251BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.046	3.47 ng	334052	1,4-Dichlorobenzene-d4	7.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9

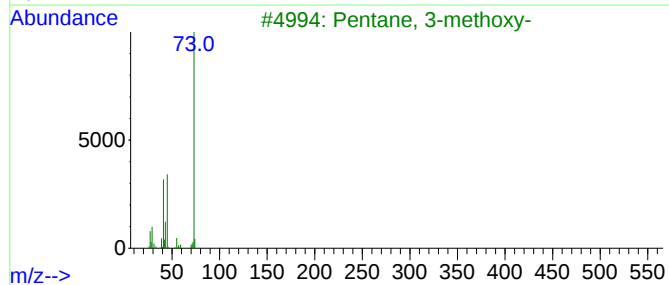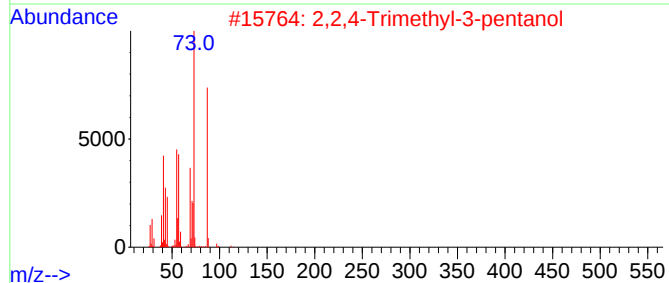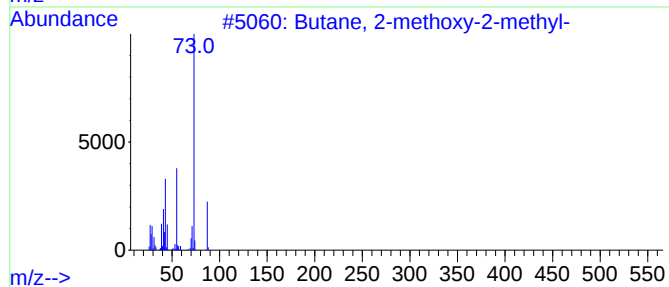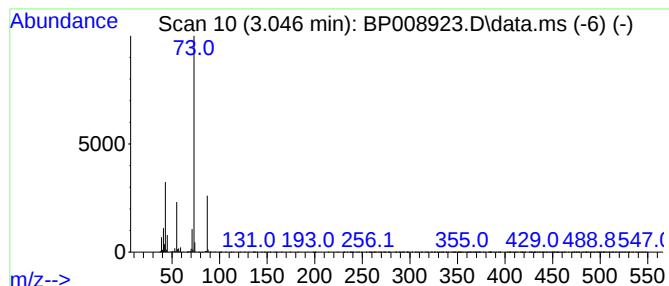

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008923.D
Acq On : 26 Jan 2022 11:18
Operator : CG/JU
Sample : PB142251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142251BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
Butane, 2-metho...	3.046	3.5	ng	334052	1	7.834	1925700	20.0