

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
 Data File : BP008941.D
 Acq On : 26 Jan 2022 21:39
 Operator : CG/JU
 Sample : N1263-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 D2-E2B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	5	9	19	rVB	76517	132926	2.57%	0.424%
2	5.422	408	414	420	rBV	204935	338920	6.55%	1.081%
3	5.475	420	423	435	rVB	24641	52103	1.01%	0.166%
4	7.016	680	685	700	rVB	153538	339644	6.56%	1.084%
5	7.481	756	764	770	rBV3	28687	70009	1.35%	0.223%
6	7.834	815	824	833	rBV	941474	1588798	30.70%	5.069%
7	8.999	1016	1022	1030	rBV	98999	192761	3.72%	0.615%
8	10.634	1290	1300	1307	rBV	1174625	2147370	41.49%	6.852%
9	13.093	1710	1718	1730	rBV	381585	636226	12.29%	2.030%
10	14.469	1946	1952	1960	rBV	1870520	2888961	55.82%	9.218%
11	15.969	2202	2207	2215	rBV	260196	414235	8.00%	1.322%
12	17.228	2413	2421	2426	rBV	2319587	3494255	67.52%	11.149%
13	17.269	2426	2428	2434	rVB	372035	462207	8.93%	1.475%
14	17.363	2440	2444	2451	rVB	93233	136687	2.64%	0.436%
15	17.639	2488	2491	2499	rVB	32153	52406	1.01%	0.167%
16	18.098	2565	2569	2571	rBV	60534	82014	1.58%	0.262%
17	18.145	2571	2577	2581	rVB2	88559	197968	3.83%	0.632%
18	18.286	2596	2601	2605	rBV3	97624	166919	3.23%	0.533%
19	18.633	2656	2660	2665	rVB4	49979	85125	1.64%	0.272%
20	18.816	2689	2691	2696	rVB3	49405	57476	1.11%	0.183%
21	18.980	2716	2719	2724	rBV3	103037	162567	3.14%	0.519%
22	19.122	2739	2743	2748	rBV3	124732	173267	3.35%	0.553%
23	19.239	2758	2763	2769	rBV	1156944	1563191	30.20%	4.988%
24	19.298	2770	2773	2777	rVB2	78437	94982	1.84%	0.303%
25	19.357	2781	2783	2786	rBV3	45165	58349	1.13%	0.186%
26	19.592	2819	2823	2831	rVB	951610	1306000	25.24%	4.167%
27	19.669	2833	2836	2841	rVB2	112577	142410	2.75%	0.454%
28	19.786	2852	2856	2861	rVB	721350	904984	17.49%	2.888%
29	21.045	3067	3070	3075	rBV3	301264	479837	9.27%	1.531%
30	21.098	3075	3079	3087	rVB2	654104	982209	18.98%	3.134%
31	21.233	3098	3102	3107	rVB	836831	918095	17.74%	2.929%
32	21.322	3110	3117	3121	rBV2	3264005	5175324	100.00%	16.513%
33	21.357	3121	3123	3128	rVB	685099	753965	14.57%	2.406%
34	22.998	3398	3402	3407	rBV	582065	1101766	21.29%	3.515%
35	23.733	3521	3527	3533	rVB2	1926079	3986577	77.03%	12.720%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008941.D
Acq On : 26 Jan 2022 21:39
Operator : CG/JU
Sample : N1263-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
D2-E2B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 31340533

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008941.D
Acq On : 26 Jan 2022 21:39
Operator : CG/JU
Sample : N1263-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
D2-E2B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

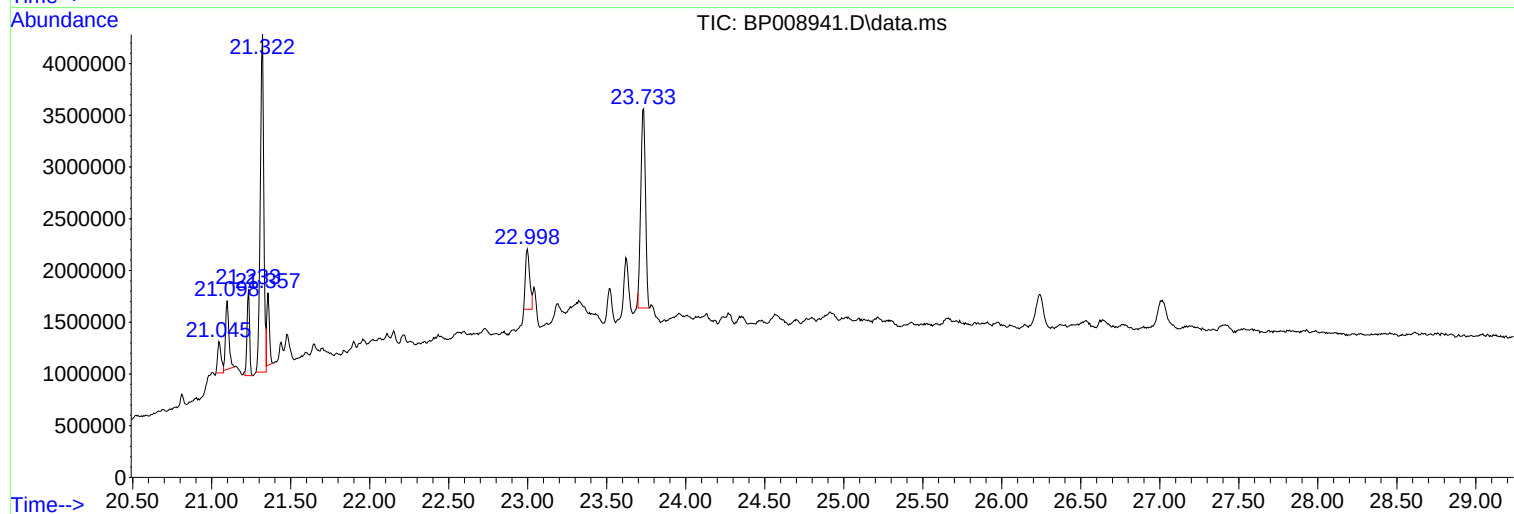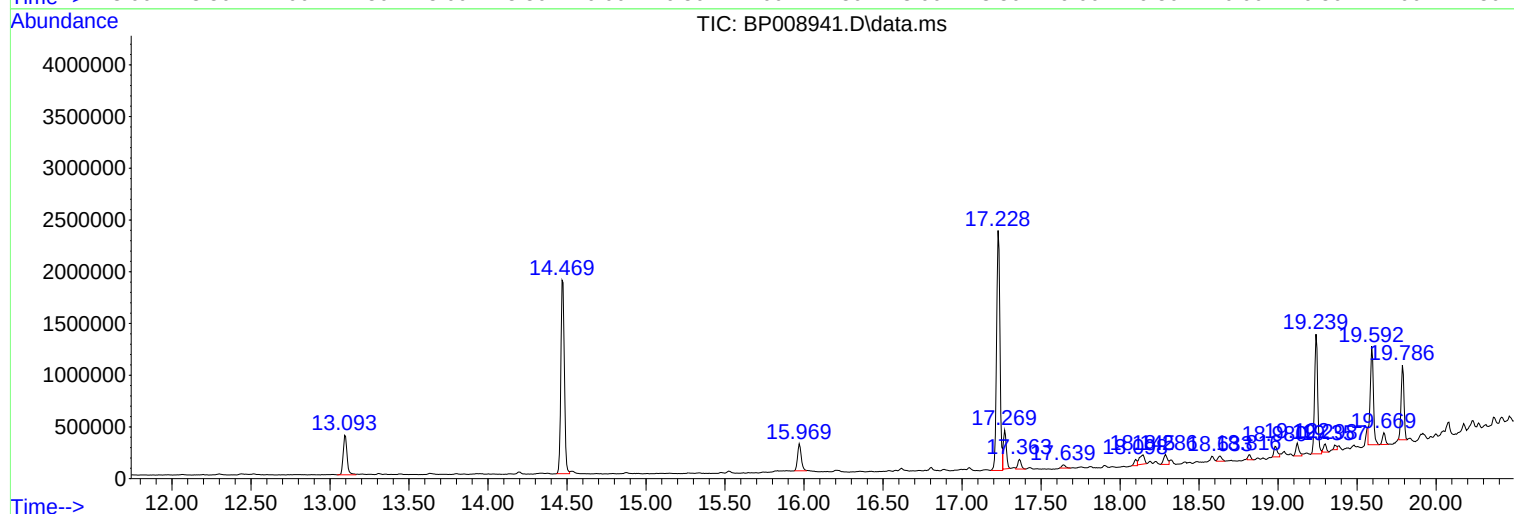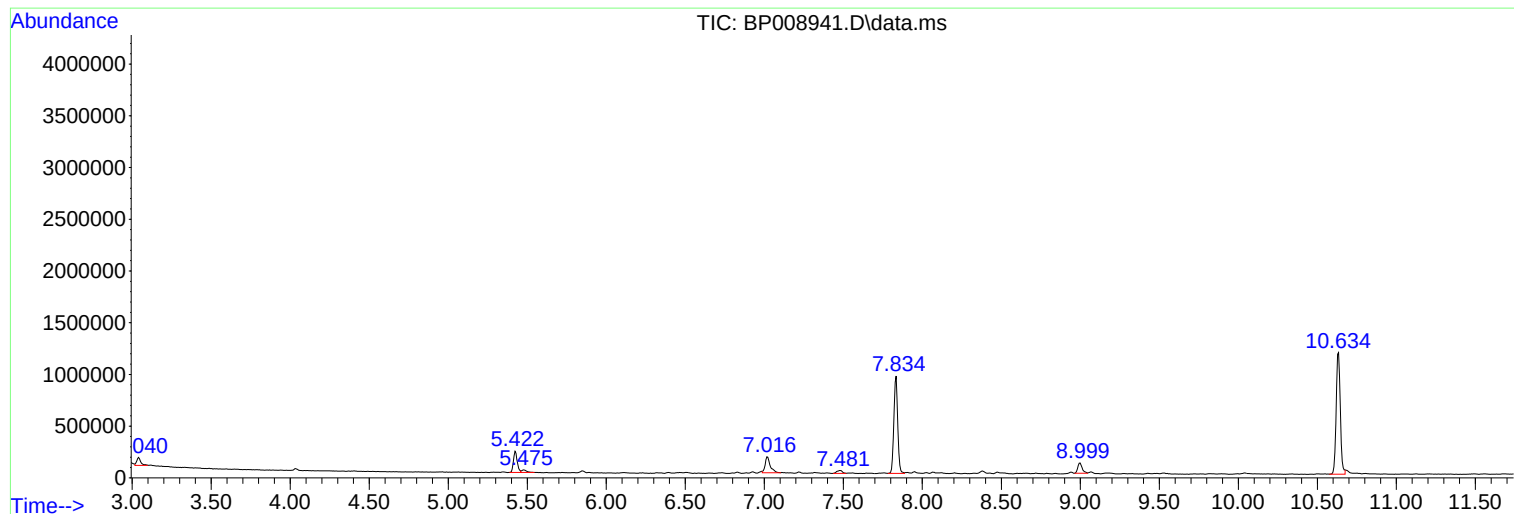

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008941.D
Acq On : 26 Jan 2022 21:39
Operator : CG/JU
Sample : N1263-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
D2-E2B










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.098	3.80 ng	982209	Chrysene-d12	21.322

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	72
2			Phenyl(2-phenyl-1,3-dioxolan-2-y...	298	C18H18O4	006963-16-2	72
3			Phenyl(2-phenyl-1,3-dioxolan-2-y...	256	C16H16O3	005694-69-9	72
4			Benzoic acid, 2-(4-nitrophenoxy)...	287	C15H13NO5	1000368-92-7	56
5			1,3-Dioxolane, 2-(methoxymethyl)...	194	C11H14O3	1000156-71-2	56

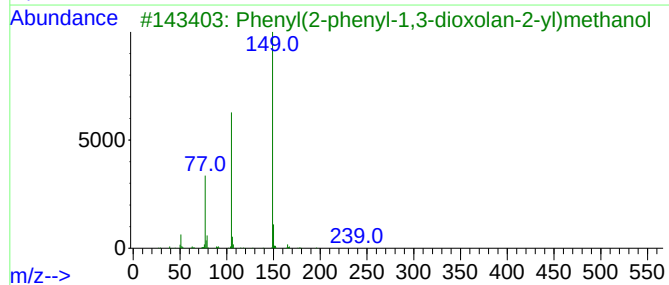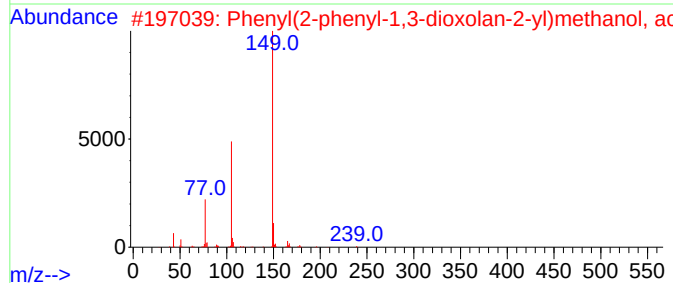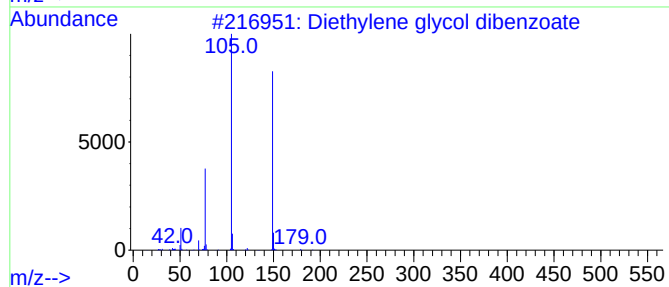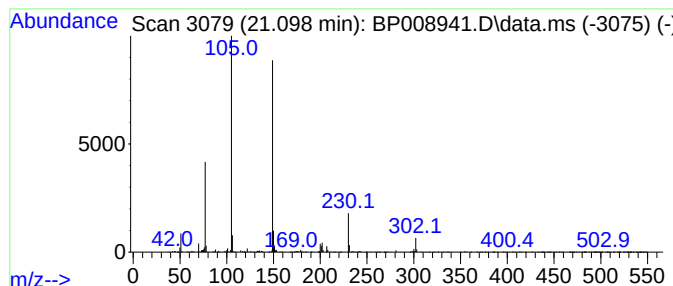

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008941.D
Acq On : 26 Jan 2022 21:39
Operator : CG/JU
Sample : N1263-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
D2-E2B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glyc...	21.098	3.8	ng	982209	5	21.322	5175320	20.0