
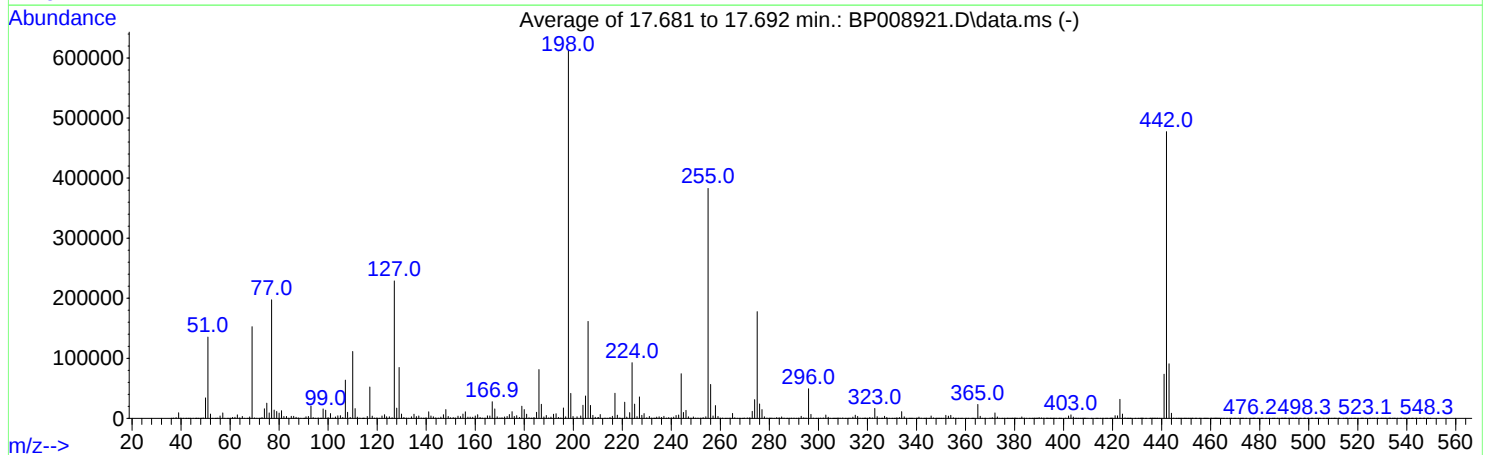


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
 Data File : BP008921.D
 Acq On : 26 Jan 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 26 01:52:51 2022

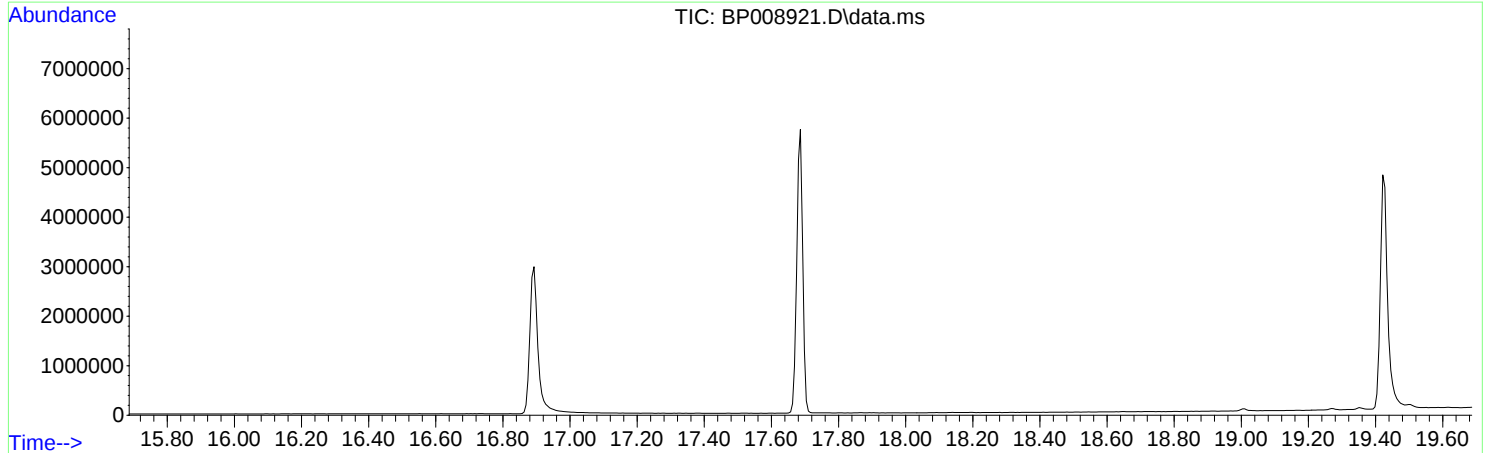


AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.1	135257	PASS
68	69	0.00	2	1.6	2501	PASS
69	198	0.00	100	24.9	152783	PASS
70	69	0.00	2	0.5	798	PASS
127	198	10	80	37.4	228863	PASS
197	198	0.00	2	0.4	2663	PASS
198	198	100	100	100.0	612465	PASS
199	198	5	9	6.8	41472	PASS
275	198	10	60	29.0	177813	PASS
365	198	1	100	3.8	23195	PASS
441	198	0.01	100	12.0	73565	PASS
442	442	100	100	100.0	477380	PASS
443	442	15	24	19.1	90981	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008921.D
Acq On : 26 Jan 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 27 06:32:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration

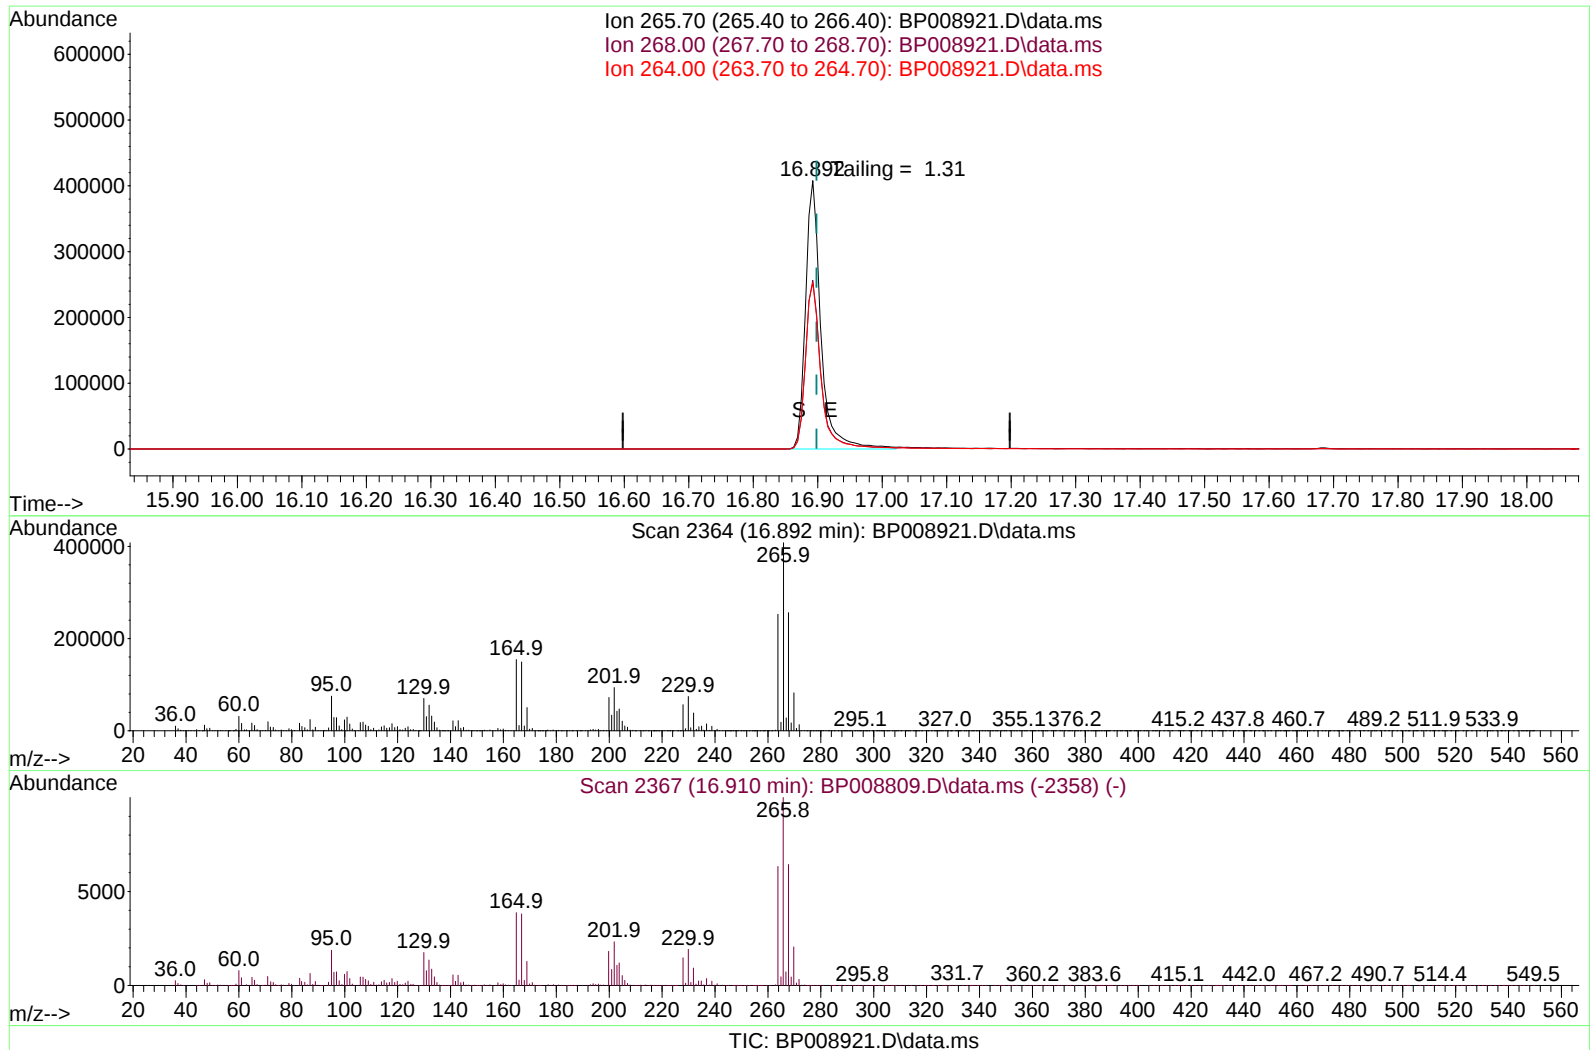

(70) Pentachlorophenol (C)

16.892min (-0.006) 218943.47 ng




response 682522

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.85
264.00	62.90	62.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012622\
Data File : BP008921.D
Acq On : 26 Jan 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 27 06:32:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration

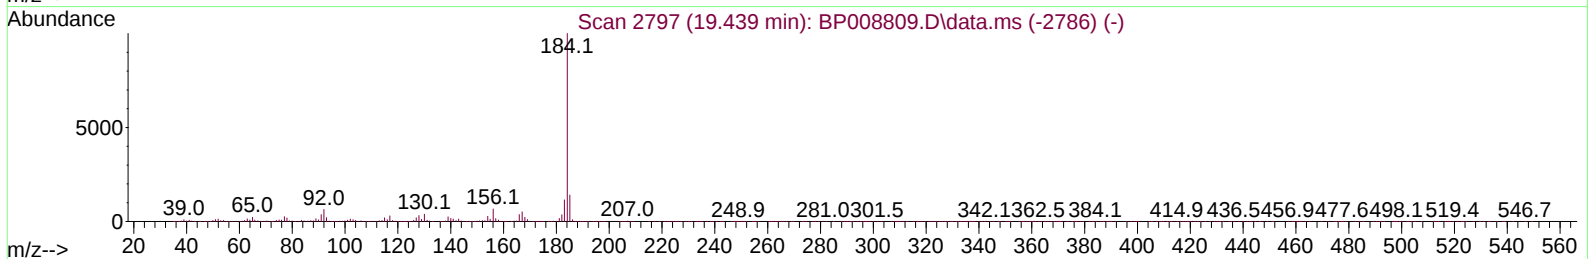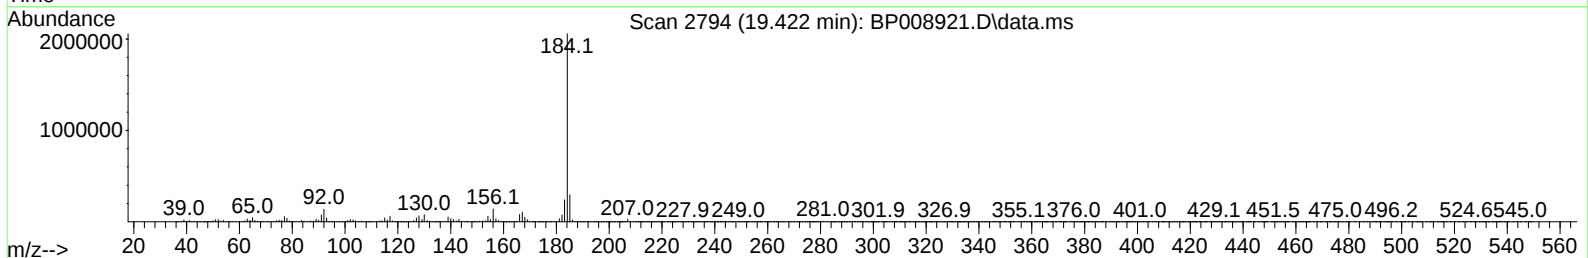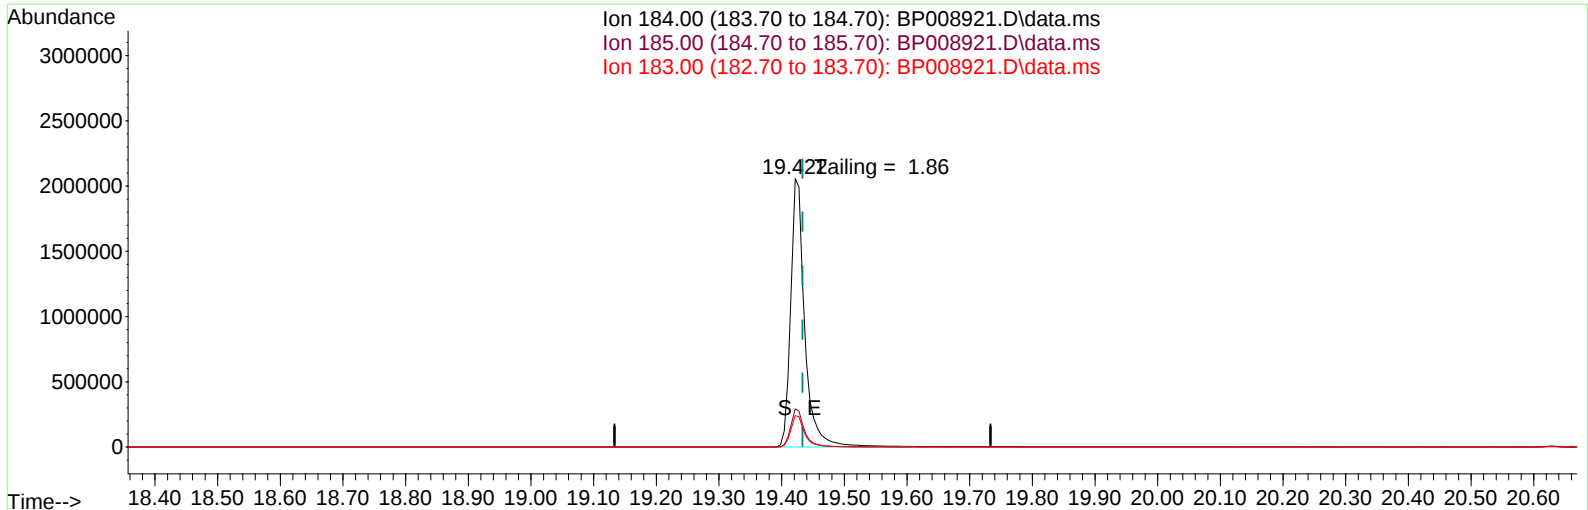

TIC: BP008921.D\data.ms

(77) Benzidine

19.422min (-0.012) 34236.17 ng

response 3236590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.28
183.00	11.90	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/26/2022	BNA_P	<u>BP008921.D</u>
Compound Name	Response	Retention Time
DDT	1917784	20.628
DDD	44286	20.204
DDE	3858	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48144	1965928	2.45

Instrument :
BNA_P
ClientSampleId :
DFTPP