
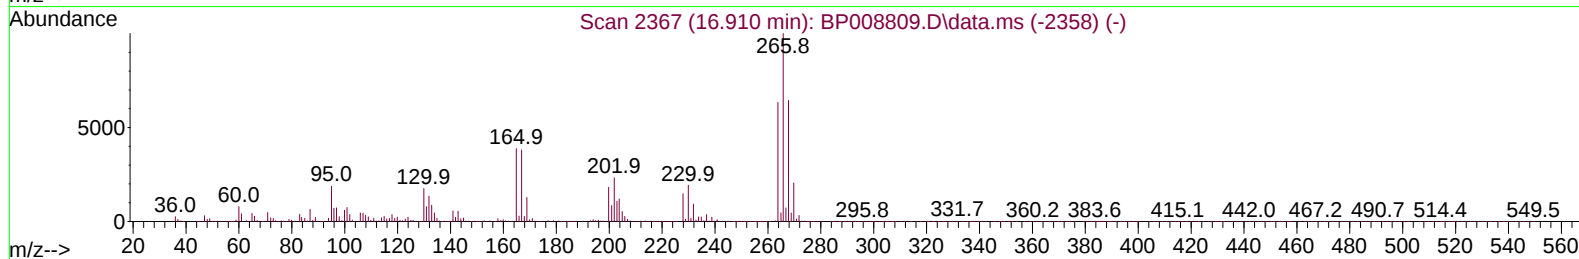
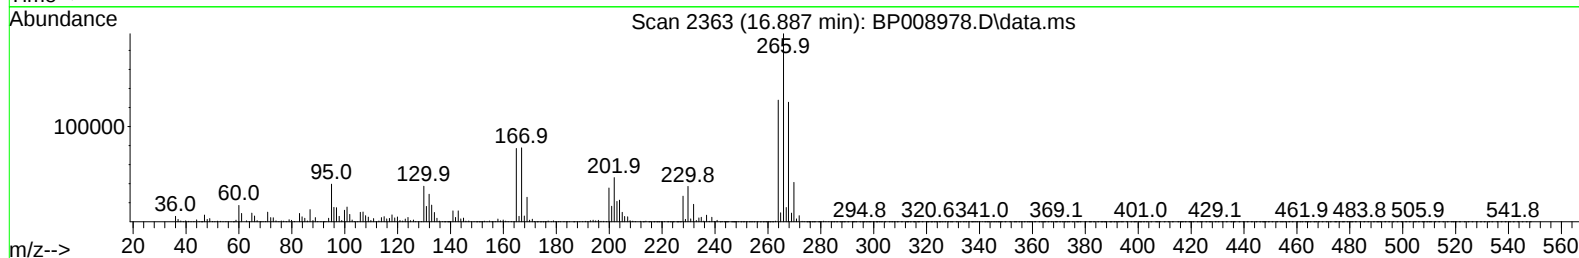


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020122\
Data File : BP008978.D
Acq On : 01 Feb 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 14:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 04:16:03 2022
Response via : Initial Calibration

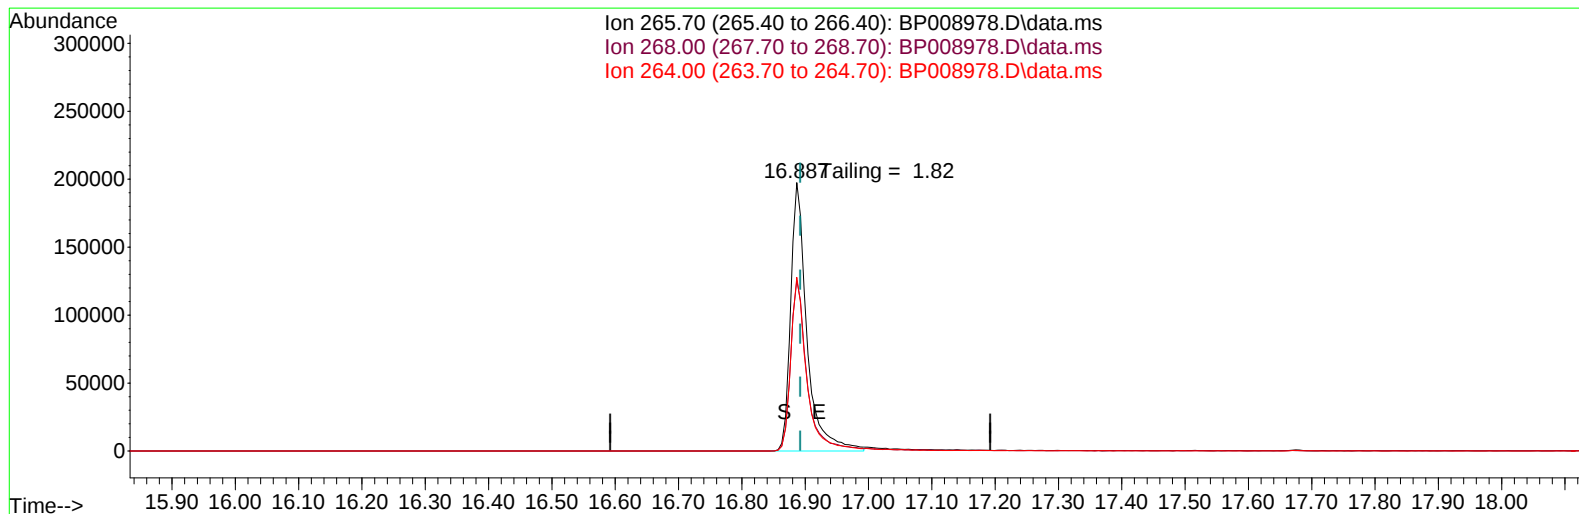

TIC: BP008978.D\data.ms

(70) Pentachlorophenol (C)




16.887min (-0.006) 206563.91 ng

response 363687

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.56
264.00	62.90	64.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020122\
Data File : BP008978.D
Acq On : 01 Feb 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 14:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 04:16:03 2022
Response via : Initial Calibration

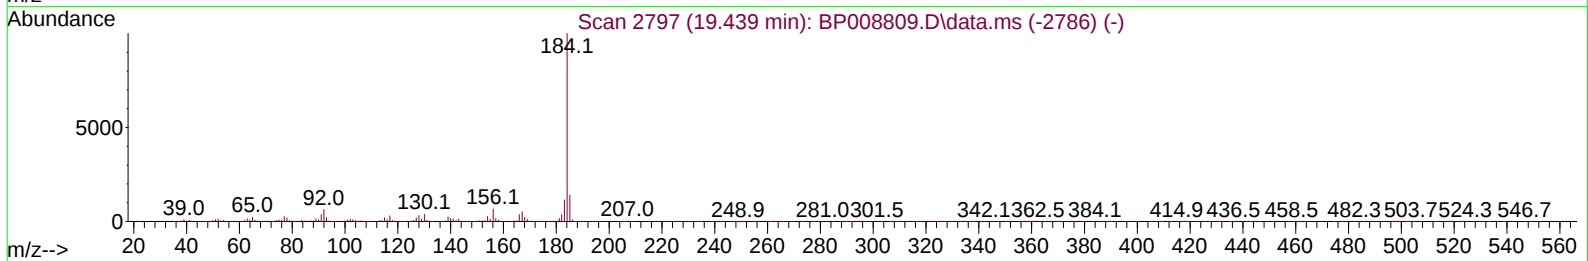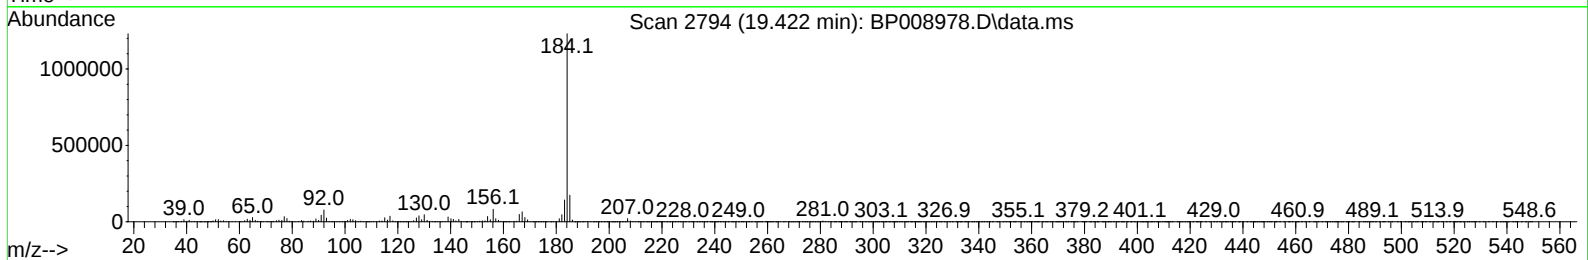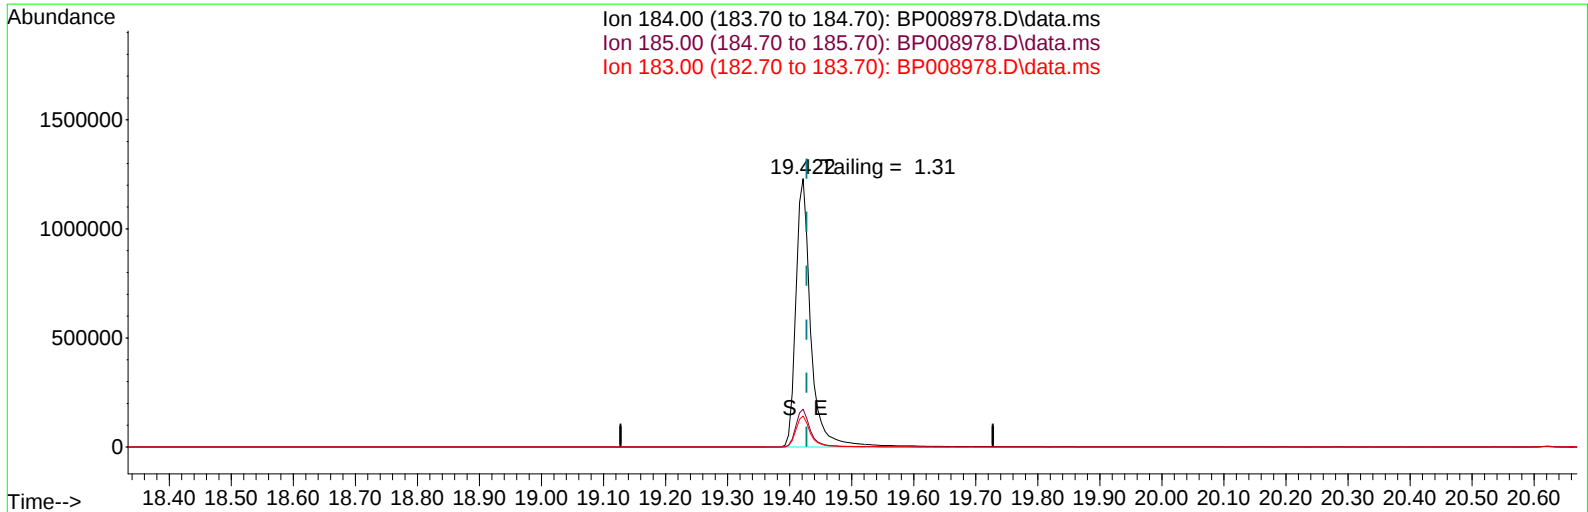

TIC: BP008978.D\data.ms

(77) Benzidine**19.422min (-0.006) 32626.91 ng****response 2078204**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.10
183.00	11.90	11.61
0.00	0.00	0.00