
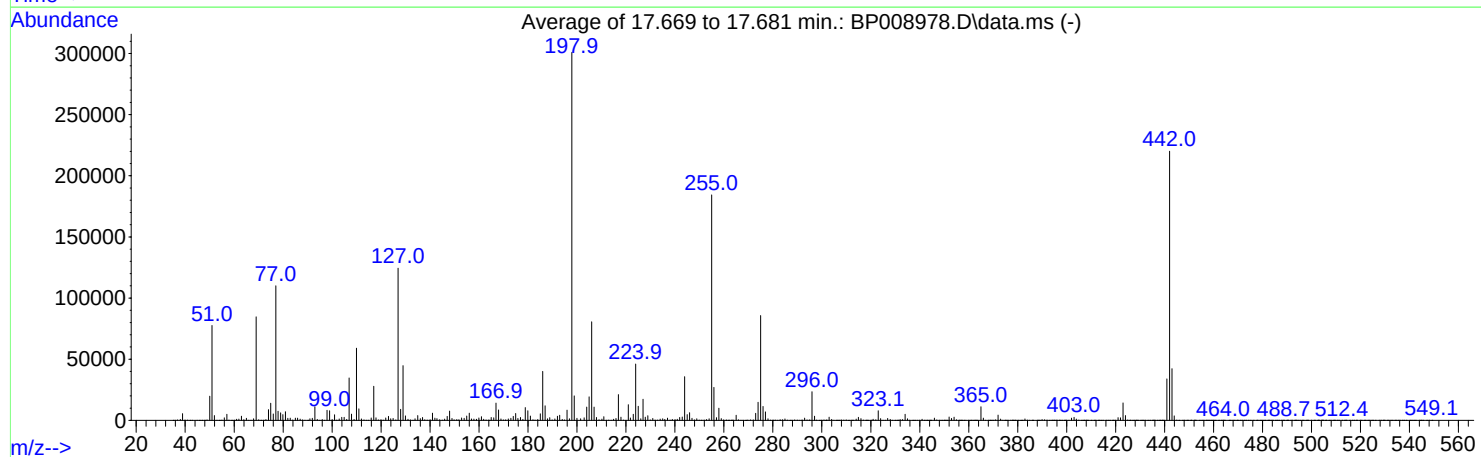


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020122\
 Data File : BP008978.D
 Acq On : 01 Feb 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 01 04:16:03 2022

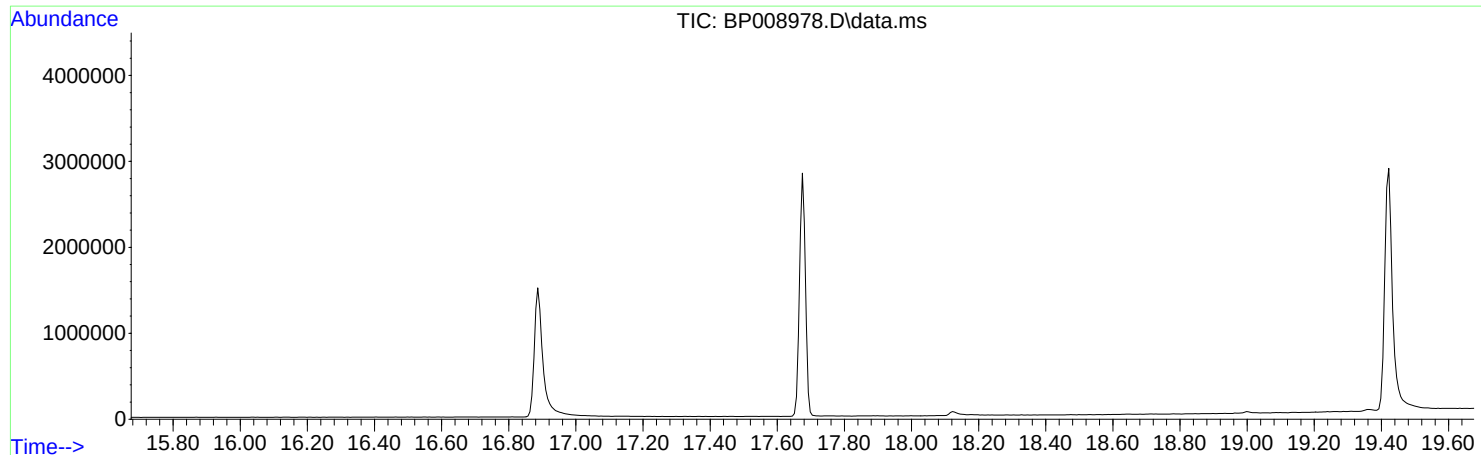




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	77539	PASS
68	69	0.00	2	1.6	1328	PASS
69	198	0.00	100	28.2	84731	PASS
70	69	0.00	2	0.6	486	PASS
127	198	10	80	41.3	124382	PASS
197	198	0.00	2	0.4	1325	PASS
198	198	100	100	100.0	300812	PASS
199	198	5	9	6.7	20046	PASS
275	198	10	60	28.5	85683	PASS
365	198	1	100	3.7	11118	PASS
441	198	0.01	100	11.3	33941	PASS
442	442	100	100	100.0	220117	PASS
443	442	15	24	19.2	42216	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020122\
Data File : BP008978.D
Acq On : 01 Feb 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 01 14:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 04:16:03 2022
Response via : Initial Calibration

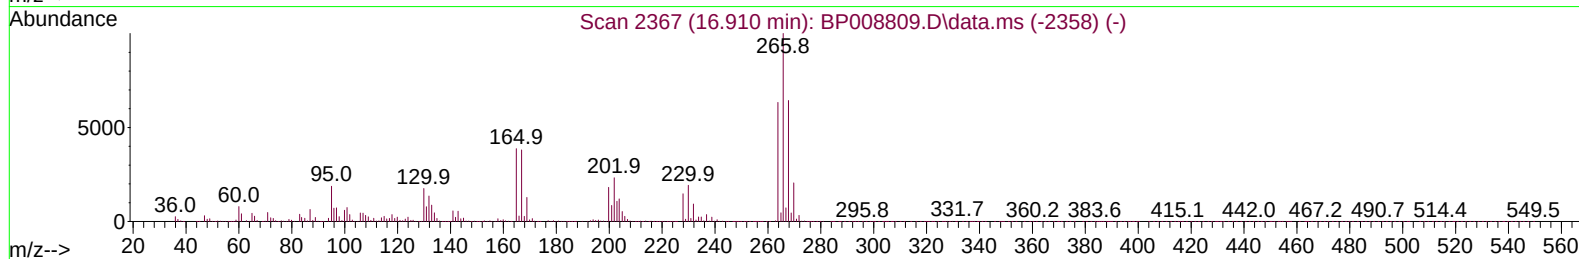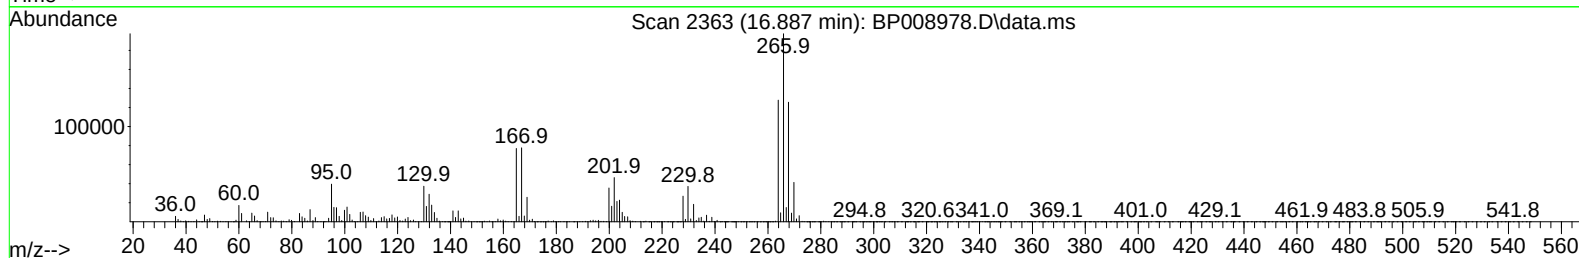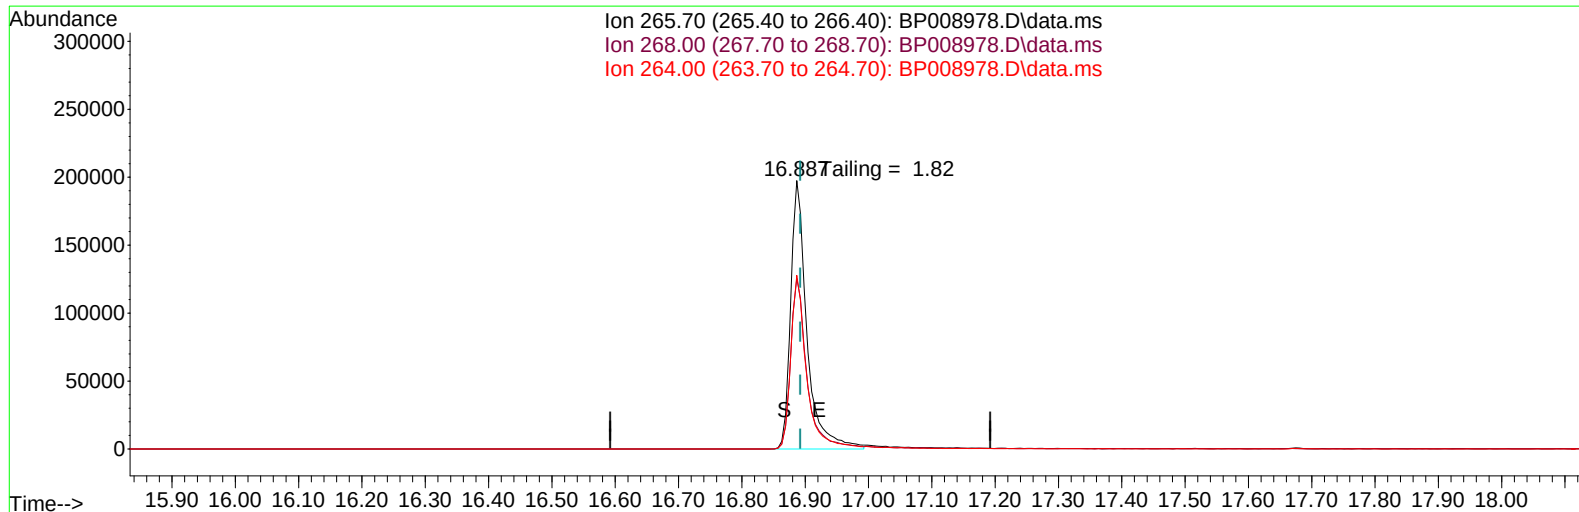

TIC: BP008978.D\data.ms

(70) Pentachlorophenol (C)

16.887min (-0.006) 206563.91 ng




response 363687

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.56
264.00	62.90	64.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020122\
 Data File : BP008978.D
 Acq On : 01 Feb 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 01 14:02:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 04:16:03 2022
 Response via : Initial Calibration

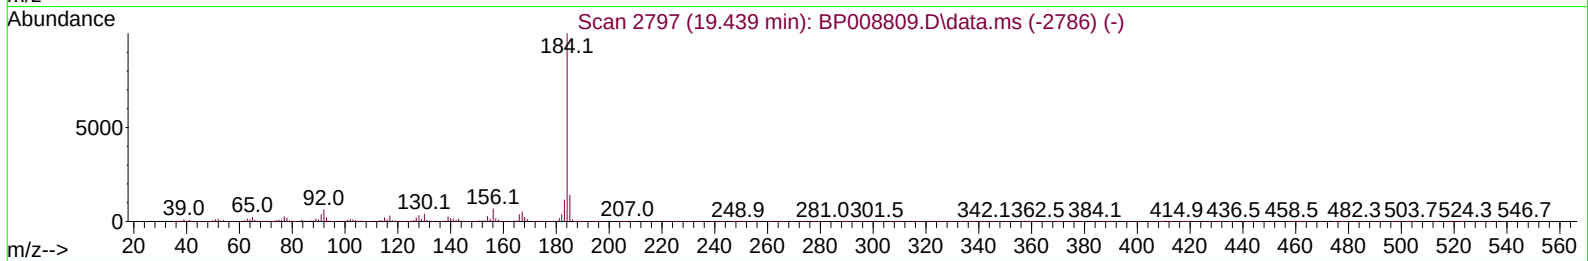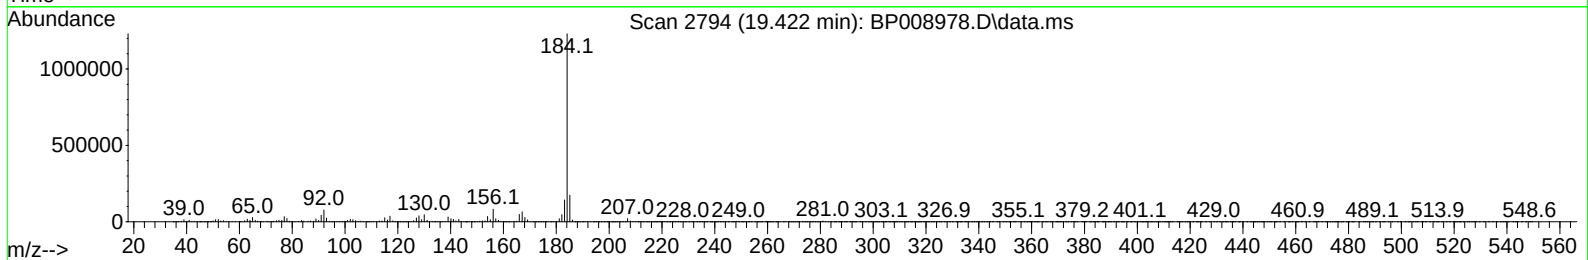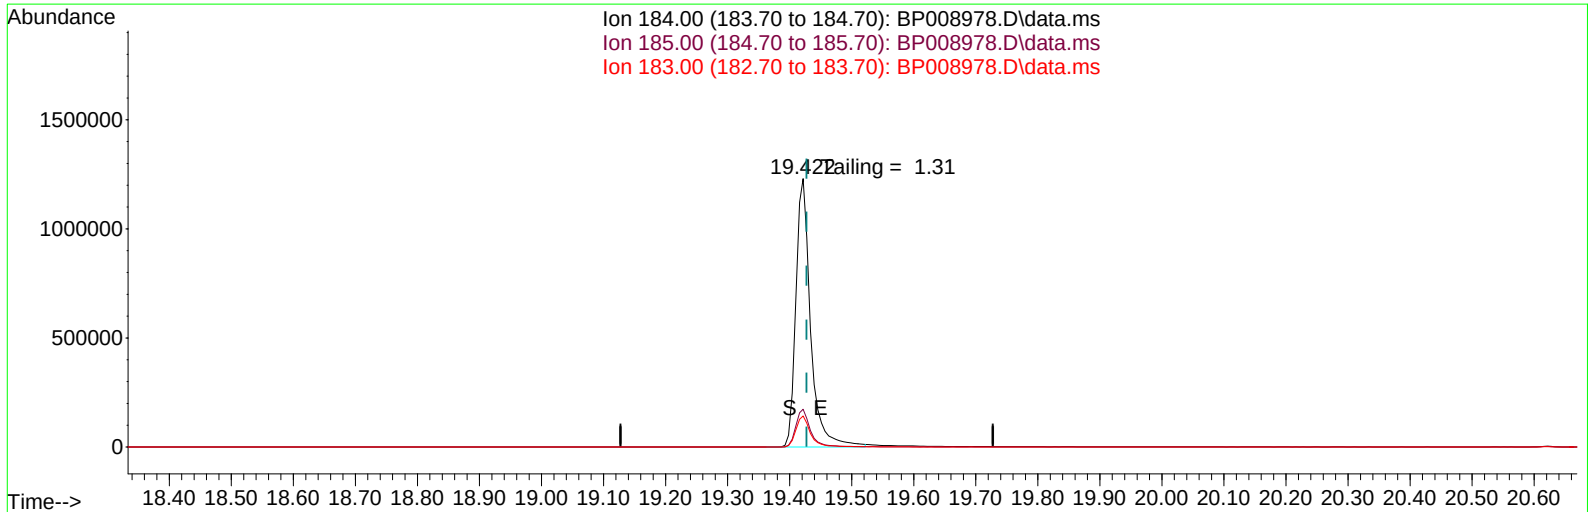

TIC: BP008978.D\data.ms

(77) Benzidine

19.422min (-0.006) 32626.91 ng

response 2078204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.10
183.00	11.90	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/1/2022	BNA_P	<u>BP008978.D</u>
Compound Name	Response	Retention Time
DDT	1006028	20.62
DDD	25416	20.19
DDE	3106	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28522	1034550	2.76

Instrument :
BNA_P
ClientSampleId :
DFTPP