

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020123\
 Data File : BP013689.D
 Acq On : 01 Feb 2023 11:16
 Operator : CG/JU
 Sample : SST02025
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST020605

Quant Time: Feb 02 00:17:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:14:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	275769	20.000	ng/ul	0.00
20) Naphthalene-d8	10.969	136	1145449	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.775	164	816999	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.528	188	2012543	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240	2146168	20.000	ng/ul	0.00
88) Perylene-d12	24.180	264	2438812	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.481	96	52250	8.033	ng/uL	0.00
4) Pyridine-d5	3.911	84	372758	19.973	ng/ul	0.00
7) Phenol-d5	7.281	99	483548	19.951	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	291076	20.477	ng/ul	0.00
11) 2-Chlorophenol-d4	7.664	132	363766	20.474	ng/ul	0.00
15) 4-Methylphenol-d8	8.846	113	387265	20.043	ng/ul	0.00
21) Nitrobenzene-d5	9.310	128	149154	20.412	ng/ul	0.00
24) 2-Nitrophenol-d4	10.040	143	179383	21.065	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	416570	20.919	ng/ul	0.00
31) 4-Chloroaniline-d4	11.099	131	559512	21.274	ng/ul	0.00
46) Dimethylphthalate-d6	14.175	166	1335493	20.737	ng/ul	0.00
49) Acenaphthylene-d8	14.469	160	1486482	20.891	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	218259	20.107	ng/ul	0.00
60) Fluorene-d10	15.763	176	1145243	20.631	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	192248	17.046	ng/ul	0.00
73) Anthracene-d10	17.628	188	1952470	20.813	ng/ul	0.00
81) Pyrene-d10	19.845	212	2423295	20.245	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.010	264	2565023	20.603	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.517	88	55053	8.122	ng/uL	100
5) Pyridine	3.934	79	380628	20.255	ng/ul	100
6) Benzaldehyde	7.269	77	208551	21.422	ng/ul	100
8) Phenol	7.311	94	499494	20.138	ng/ul	100
10) Bis(2-Chloroethyl)ether	7.552	93	410241	20.582	ng/ul	100
12) 2-Chlorophenol	7.693	128	366449	20.358	ng/ul	100
13) 2-Methylphenol	8.575	108	379848	20.057	ng/ul	100
14) 2,2'-oxybis(1-Chloropr...	8.669	45	482103	20.429	ng/ul	100
16) Acetophenone	8.969	105	625719	20.774	ng/ul	100
17) N-Nitroso-di-n-propyla...	8.952	70	312245	20.694	ng/ul	100
18) 4-Methylphenol	8.905	108	415863	20.219	ng/ul	100
19) Hexachloroethane	9.234	117	143302	20.339	ng/ul	100
22) Nitrobenzene	9.352	77	415188	21.037	ng/ul	100
23) Isophorone	9.881	82	941992	20.848	ng/ul	100
25) 2-Nitrophenol	10.069	139	201706	21.407	ng/ul	100
26) 2,4-Dimethylphenol	10.122	107	447001	20.997	ng/ul	100
27) Bis(2-Chloroethoxy)met...	10.363	93	571633	20.875	ng/ul	100
29) 2,4-Dichlorophenol	10.605	162	406282	21.081	ng/ul	100
30) Naphthalene	11.016	128	1262462	20.853	ng/ul	100
32) 4-Chloroaniline	11.122	127	569940	21.532	ng/ul	100
33) Hexachlorobutadiene	11.299	225	279264	20.546	ng/ul	100
34) Caprolactam	11.899	113	133684	20.533	ng/ul	100
35) 4-Chloro-3-methylphenol	12.228	107	433538	21.224	ng/ul	100
36) 2-Methylnaphthalene	12.610	142	924506	21.454	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020123\
 Data File : BP013689.D
 Acq On : 01 Feb 2023 11:16
 Operator : CG/JU
 Sample : SSTD02025
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020605

Quant Time: Feb 02 00:17:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:14:26 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.834	142	918611	21.107	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.975	216	561851	20.819	ng/ul	100
40) Hexachlorocyclopentadiene	12.957	237	275227	18.138	ng/ul	100
41) 2,4,6-Trichlorophenol	13.210	196	378434	21.168	ng/ul	100
42) 2,4,5-Trichlorophenol	13.281	196	419483	21.530	ng/ul	100
43) 1,1'-Biphenyl	13.610	154	1350811	21.837	ng/ul	100
44) 2-Chloronaphthalene	13.657	162	1067113	21.805	ng/ul	100
45) 2-Nitroaniline	13.857	65	196353	21.078	ng/ul	100
47) Dimethylphthalate	14.222	163	1311261	20.667	ng/ul	100
48) 2,6-Dinitrotoluene	14.346	165	188525	20.850	ng/ul	100
50) Acenaphthylene	14.498	152	1569400	20.917	ng/ul	100
51) 3-Nitroaniline	14.675	138	180638	18.901	ng/ul	100
52) Acenaphthene	14.840	153	1070185	20.756	ng/ul	100
53) 2,4-Dinitrophenol	14.875	184	114418	16.292	ng/ul	100
55) 4-Nitrophenol	14.969	109	169199	20.448	ng/ul	100
56) Dibenzofuran	15.169	168	1549770	20.693	ng/ul	100
57) 2,4-Dinitrotoluene	15.128	165	308741	21.740	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.393	232	370314	20.223	ng/ul	100
59) Diethylphthalate	15.581	149	1255000	20.604	ng/ul	100
61) Fluorene	15.822	166	1253778	20.571	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.810	204	670002	20.177	ng/ul	100
63) 4-Nitroaniline	15.834	138	173874	19.430	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.892	198	201052	17.912	ng/ul	100
67) N-Nitrosodiphenylamine	16.022	169	1095986	20.176	ng/ul	100
68) 4-Bromophenyl-phenylether	16.710	248	469627	20.510	ng/ul	100
69) Hexachlorobenzene	16.828	284	554841	20.655	ng/ul	100
70) Atrazine	16.975	200	448542	20.516	ng/ul	100
71) Pentachlorophenol	17.169	266	329622	19.224	ng/ul	100
72) Phenanthrene	17.569	178	2213539	20.822	ng/ul	100
74) Anthracene	17.663	178	2251892	20.914	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.581	216	602892	21.027	ng/ul	100
76) Pentachlorobenzene	15.093	250	575562	19.581	ng/ul	100
77) Carbazole	17.922	167	1997129	21.380	ng/ul	100
78) Di-n-butylphthalate	18.457	149	2285107	20.704	ng/ul	100
80) Fluoranthene	19.522	202	2803717	20.096	ng/ul	100
82) Pyrene	19.875	202	2911909	20.414	ng/ul	100
83) Butylbenzylphthalate	20.728	149	813806	19.857	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.510	252	991659	20.344	ng/ul	100
85) Benzo(a)anthracene	21.586	228	3054191	20.700	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.486	149	1365970	19.441	ng/ul	100
87) Chrysene	21.645	228	2870028	20.661	ng/ul	100
89) Di-n-octyl phthalate	22.469	149	2415156	18.799	ng/ul	100
90) Benzo(b)fluoranthene	23.386	252	3190986	20.043	ng/ul	100
91) Benzo(k)fluoranthene	23.439	252	3167493	20.817	ng/ul	100
93) Benzo(a)pyrene	24.063	252	2846712	20.712	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.892	276	3701785	21.738	ng/ul	100
95) Dibenzo(a,h)anthracene	26.915	278	3072904	21.767	ng/ul	100
96) Benzo(g,h,i)perylene	27.733	276	2951405	21.908	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020123\
Data File : BP013689.D
Acq On : 01 Feb 2023 11:16
Operator : CG/JU
Sample : SSTD02025
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD020605

Quant Time: Feb 02 00:17:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:14:26 2023
Response via : Initial Calibration




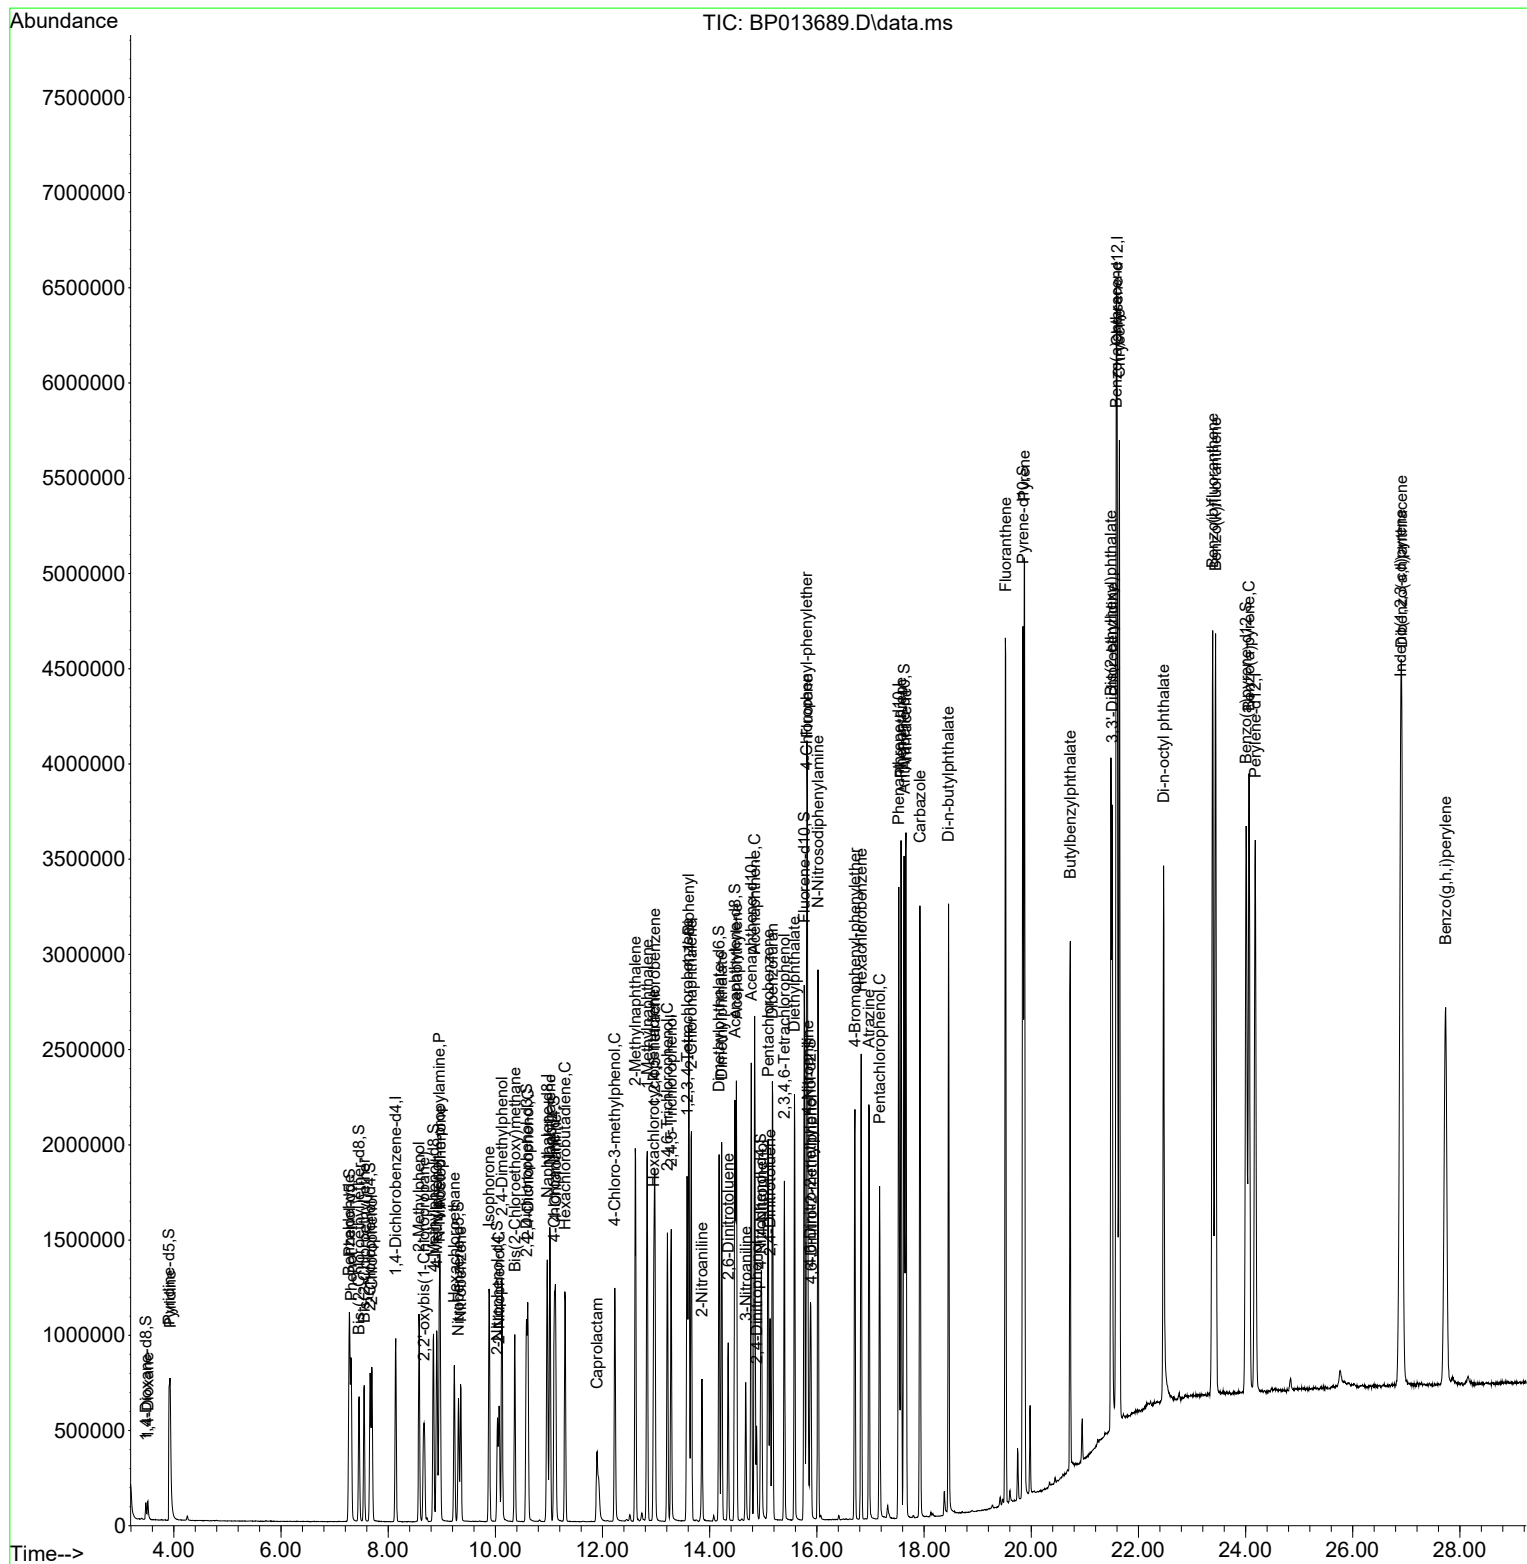




#2
1,4-Dioxane
Concen: 8.122 ng/uL
RT: 3.517 min Scan# 50
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion: 88 Resp: 55053
Ion Ratio Lower Upper
88 100
43 27.8 22.2 33.4
58 68.6 54.9 82.3

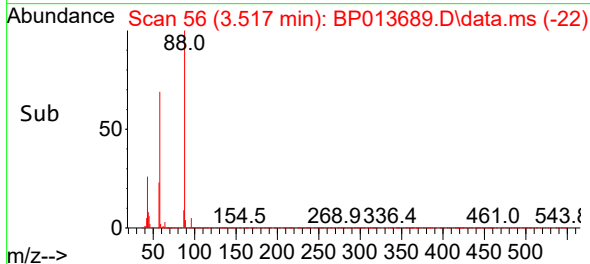

#5
Pyridine
Concen: 20.255 ng/uL
RT: 3.934 min Scan# 127
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion: 79 Resp: 380628
Ion Ratio Lower Upper
79 100
52 67.2 53.8 80.6
51 31.4 25.1 37.7


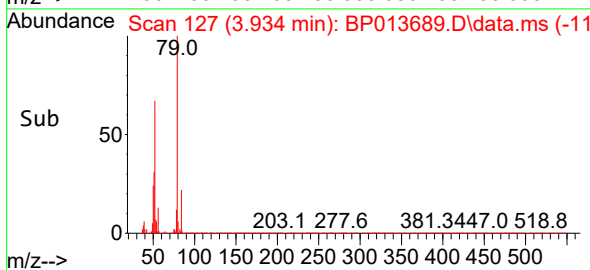

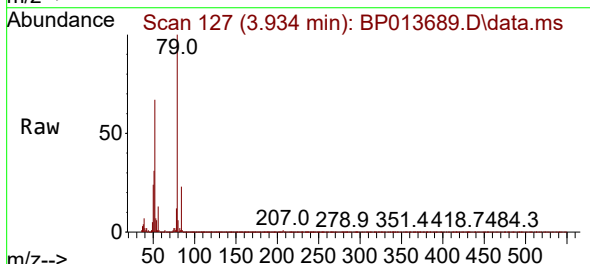




#6
Benzaldehyde
Concen: 21.422 ng/ul
RT: 7.269 min Scan# 694
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion: 77 Resp: 208551
Ion Ratio Lower Upper
77 100
105 100.8 80.6 121.0
106 93.7 75.0 112.4



#8
Phenol
Concen: 20.138 ng/ul
RT: 7.311 min Scan# 701
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion: 94 Resp: 499494
Ion Ratio Lower Upper
94 100
65 26.2 21.0 31.4
66 34.3 27.4 41.2




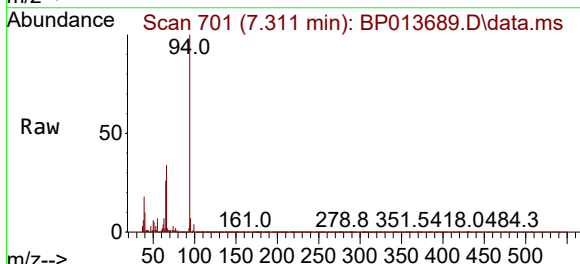




#10
Bis(2-Chloroethyl)ether
Concen: 20.582 ng/ul
RT: 7.552 min Scan# 742
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion: 93 Resp: 410241
Ion Ratio Lower Upper
93 100
63 69.7 55.8 83.6
95 31.4 25.1 37.7



#12
2-Chlorophenol
Concen: 20.358 ng/ul
RT: 7.693 min Scan# 766
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:128 Resp: 366449
Ion Ratio Lower Upper
128 100
64 47.4 37.9 56.9
130 31.5 25.2 37.8









#13
2-Methylphenol
Concen: 20.057 ng/ul
RT: 8.575 min Scan# 916
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:108 Resp: 379848
Ion Ratio Lower Upper
108 100
107 88.6 70.9 106.3



#14
2,2'-oxybis(1-Chloropropane)
Concen: 20.429 ng/ul
RT: 8.669 min Scan# 932
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion: 45 Resp: 482103
Ion Ratio Lower Upper
45 100
77 15.8 12.6 19.0
79 12.5 10.0 15.0



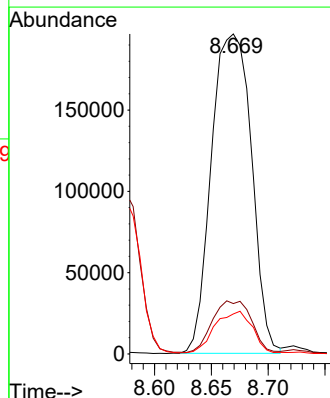





#16
Acetophenone
Concen: 20.774 ng/ul
RT: 8.969 min Scan# 983
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:105 Resp: 625719
Ion Ratio Lower Upper
105 100
77 76.5 61.2 91.8
51 23.1 18.5 27.7



#17
N-Nitroso-di-n-propylamine
Concen: 20.694 ng/ul
RT: 8.952 min Scan# 980
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion: 70 Resp: 312245
Ion Ratio Lower Upper
70 100
42 47.8 38.2 57.4
101 9.3 7.4 11.2
130 19.7 15.8 23.6





#18

4-Methylphenol

Concen: 20.219 ng/ul

RT: 8.905 min Scan# 91

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :





SSTD020605

Tgt Ion:108 Resp: 415863

Ion Ratio Lower Upper

108 100

107 112.4 89.9 134.9



#19

Hexachloroethane

Concen: 20.339 ng/ul

RT: 9.234 min Scan# 1028

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:117 Resp: 143302


Ion Ratio Lower Upper

117 100

201 118.5 94.8 142.2

199 75.1 60.1 90.1


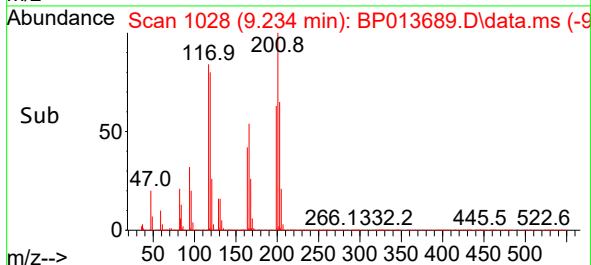
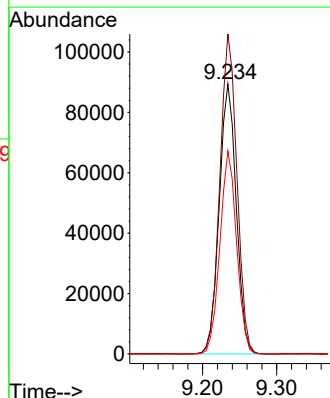
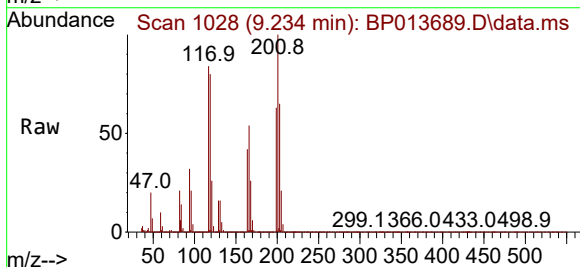




#22
Nitrobenzene
Concen: 21.037 ng/ul
RT: 9.352 min Scan# 1048
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion: 77 Resp: 415188
Ion Ratio Lower Upper
77 100
123 42.6 34.1 51.1
65 12.3 9.8 14.8



#23
Isophorone
Concen: 20.848 ng/ul
RT: 9.881 min Scan# 1138
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion: 82 Resp: 941992
Ion Ratio Lower Upper
82 100
95 6.7 5.4 8.0
138 17.0 13.6 20.4









#25
2-Nitrophenol
Concen: 21.407 ng/ul
RT: 10.069 min Scan# 1170
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:139 Resp: 201706
Ion Ratio Lower Upper
139 100
65 51.1 40.9 61.3
109 30.4 24.3 36.5



#26
2,4-Dimethylphenol
Concen: 20.997 ng/ul
RT: 10.122 min Scan# 1179
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:107 Resp: 447001
Ion Ratio Lower Upper
107 100
121 49.8 39.8 59.8
122 84.5 67.6 101.4









#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.875 ng/ul
 RT: 10.363 min Scan# 1220
 Delta R.T. 0.000 min
 Lab File: BP013689.D
 Acq: 01 Feb 2023 11:16




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020605


Tgt Ion: 93 Resp: 571633
 Ion Ratio Lower Upper
 93 100
 95 31.6 25.3 37.9
 123 10.7 8.6 12.8



#29
 2,4-Dichlorophenol
 Concen: 21.081 ng/ul
 RT: 10.605 min Scan# 1261
 Delta R.T. 0.000 min
 Lab File: BP013689.D
 Acq: 01 Feb 2023 11:16

Tgt Ion:162 Resp: 406282
 Ion Ratio Lower Upper
 162 100
 164 65.1 52.1 78.1
 98 34.6 27.7 41.5




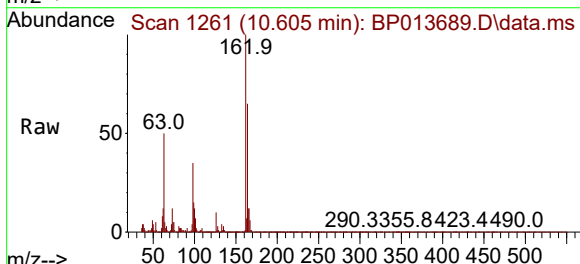




#30
Naphthalene
Concen: 20.853 ng/ul
RT: 11.016 min Scan# 1331
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:128 Resp: 1262462
Ion Ratio Lower Upper
128 100
129 11.3 9.0 13.6
127 12.8 10.2 15.4

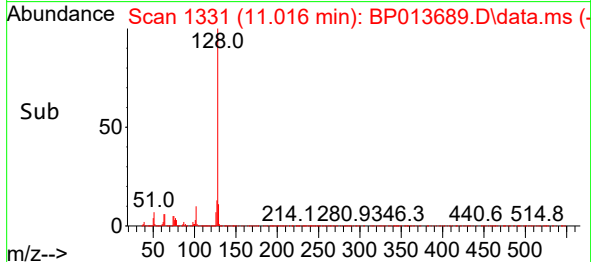

#32
4-Chloroaniline
Concen: 21.532 ng/ul
RT: 11.122 min Scan# 1349
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:127 Resp: 569940
Ion Ratio Lower Upper
127 100
129 32.6 26.1 39.1





#33

Hexachlorobutadiene

Concen: 20.546 ng/ul

RT: 11.299 min Scan# 11

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:225 Resp: 279264

Ion Ratio Lower Upper

225 100

223 64.3 51.4 77.2

227 63.6 50.9 76.3



#34

Caprolactam

Concen: 20.533 ng/ul

RT: 11.899 min Scan# 1481

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:113 Resp: 133684


Ion Ratio Lower Upper

113 100

55 160.5 128.4 192.6

56 115.2 92.2 138.2









#35
4-Chloro-3-methylphenol
Concen: 21.224 ng/ul
RT: 12.228 min Scan# 1537
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:107 Resp: 433538
Ion Ratio Lower Upper
107 100
144 26.7 21.4 32.0
142 82.0 65.6 98.4



#36
2-Methylnaphthalene
Concen: 21.454 ng/ul
RT: 12.610 min Scan# 1602
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:142 Resp: 924506
Ion Ratio Lower Upper
142 100
141 89.3 71.4 107.2









#37
1-Methylnaphthalene
Concen: 21.107 ng/ul
RT: 12.834 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:142 Resp: 918611
Ion Ratio Lower Upper
142 100
141 93.0 74.4 111.6
116 3.5 2.8 4.2

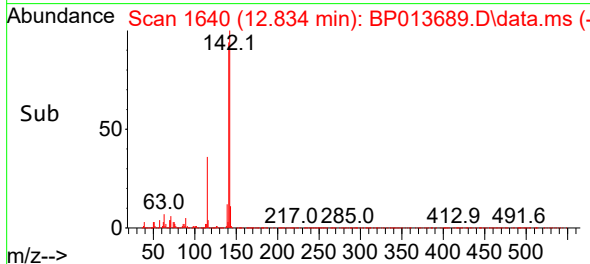

#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.819 ng/ul
RT: 12.975 min Scan# 1664
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:216 Resp: 561851
Ion Ratio Lower Upper
216 100
214 76.9 61.5 92.3
179 18.7 15.0 22.4
108 13.8 11.0 16.6


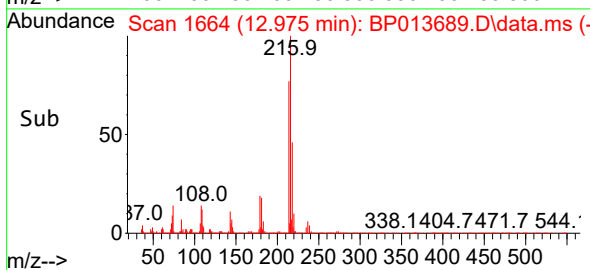

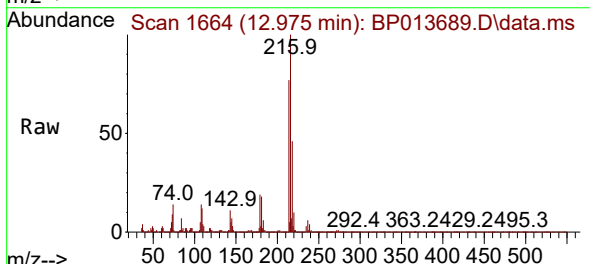




#40
Hexachlorocyclopentadiene
Concen: 18.138 ng/ul
RT: 12.957 min Scan# 1661
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:237 Resp: 275227
Ion Ratio Lower Upper
237 100
235 63.4 50.7 76.1
272 13.3 10.6 16.0



#41
2,4,6-Trichlorophenol
Concen: 21.168 ng/ul
RT: 13.210 min Scan# 1704
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:196 Resp: 378434
Ion Ratio Lower Upper
196 100
198 98.8 79.0 118.6
200 31.5 25.2 37.8





#42

2,4,5-Trichlorophenol

Concen: 21.530 ng/ul

RT: 13.281 min Scan# 1716

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:196 Resp: 419483

Ion Ratio Lower Upper

196 100

198 97.3 77.8 116.8

200 32.7 26.2 39.2



#43

1,1'-Biphenyl

Concen: 21.837 ng/ul

RT: 13.610 min Scan# 1772

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:154 Resp: 1350811


Ion Ratio Lower Upper

154 100

153 40.2 32.2 48.2

76 12.5 10.0 15.0









#44
2-Chloronaphthalene
Concen: 21.805 ng/ul
RT: 13.657 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:162 Resp: 1067113
Ion Ratio Lower Upper
162 100
164 33.2 26.6 39.8
127 34.4 27.5 41.3



#45
2-Nitroaniline
Concen: 21.078 ng/ul
RT: 13.857 min Scan# 1814
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion: 65 Resp: 196353
Ion Ratio Lower Upper
65 100
92 75.8 60.6 91.0
138 112.4 89.9 134.9



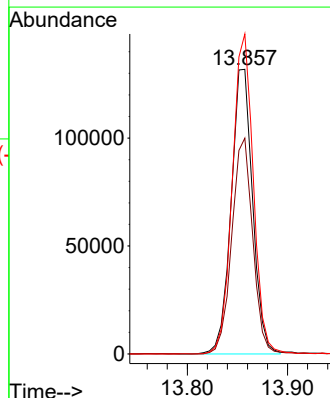
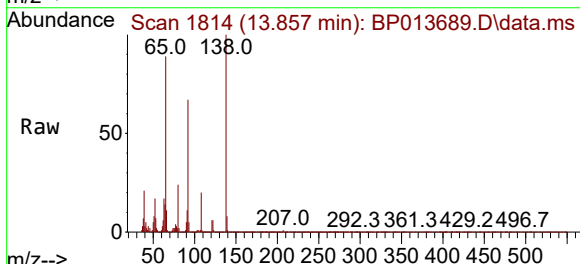




#47
Dimethylphthalate
Concen: 20.667 ng/ul
RT: 14.222 min Scan# 1876
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:163 Resp: 1311261
Ion Ratio Lower Upper
163 100
194 4.5 3.6 5.4
164 10.3 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 20.850 ng/ul
RT: 14.346 min Scan# 1897
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:165 Resp: 188525
Ion Ratio Lower Upper
165 100
89 55.8 44.6 67.0
121 19.7 15.8 23.6



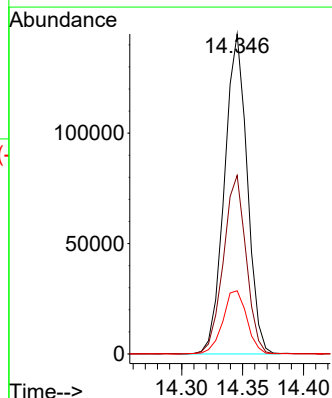
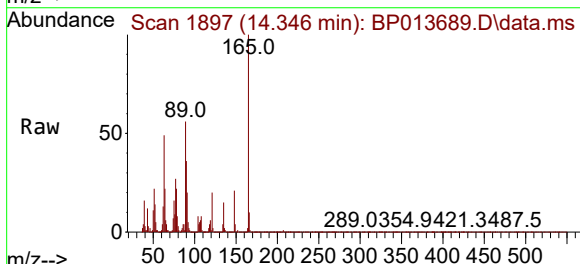




#50
Acenaphthylene
Concen: 20.917 ng/ul
RT: 14.498 min Scan# 1923
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:152 Resp: 1569400
Ion Ratio Lower Upper
152 100
151 19.9 15.9 23.9
153 13.4 10.7 16.1

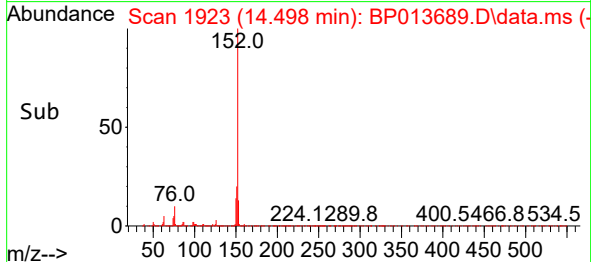

#51
3-Nitroaniline
Concen: 18.901 ng/ul
RT: 14.675 min Scan# 1953
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:138 Resp: 180638
Ion Ratio Lower Upper
138 100
108 12.5 10.0 15.0
92 118.5 94.8 142.2


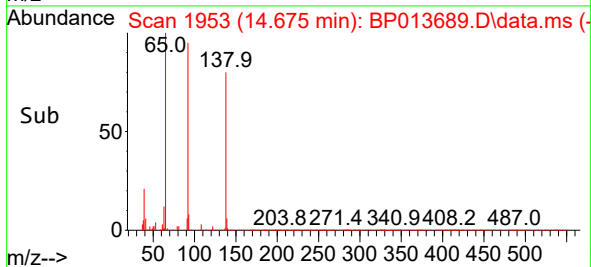

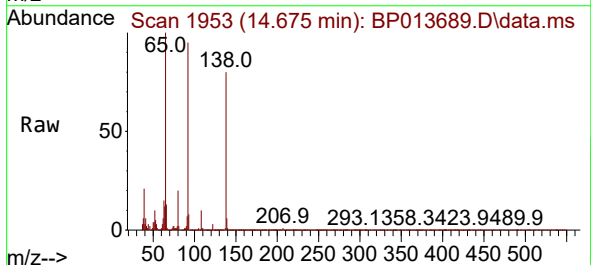




#52
Acenaphthene
Concen: 20.756 ng/ul
RT: 14.840 min Scan# 1981
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:153 Resp: 1070185
Ion Ratio Lower Upper
153 100
152 47.6 38.1 57.1
154 88.2 70.6 105.8

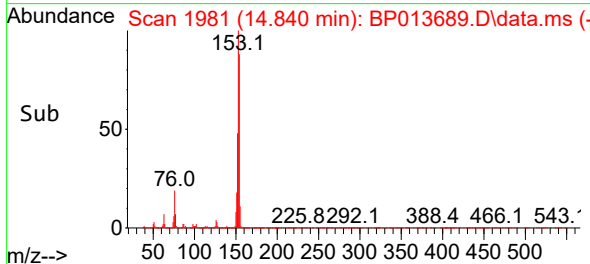

#53
2,4-Dinitrophenol
Concen: 16.292 ng/ul
RT: 14.875 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:184 Resp: 114418
Ion Ratio Lower Upper
184 100
63 53.1 42.5 63.7
154 57.5 46.0 69.0


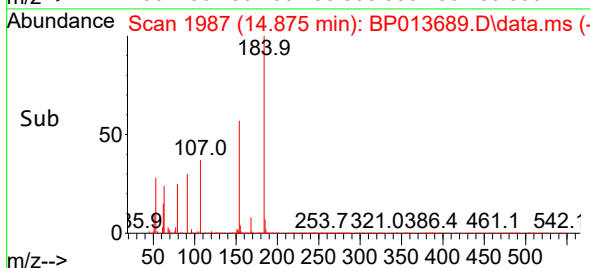
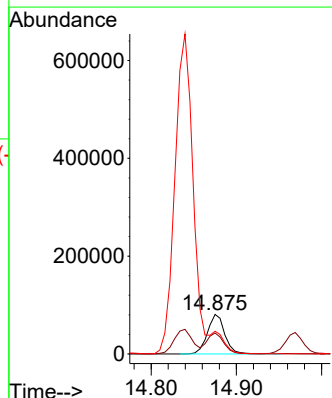
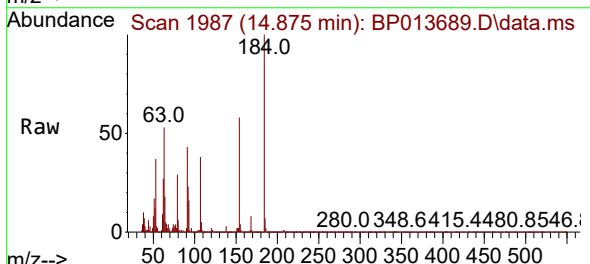




#55
4-Nitrophenol
Concen: 20.448 ng/ul
RT: 14.969 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:109 Resp: 169199
Ion Ratio Lower Upper
109 100
139 136.4 109.1 163.7
65 129.4 103.5 155.3



#56
Dibenzofuran
Concen: 20.693 ng/ul
RT: 15.169 min Scan# 2037
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:168 Resp: 1549770
Ion Ratio Lower Upper
168 100
139 34.0 27.2 40.8









#57
2,4-Dinitrotoluene
Concen: 21.740 ng/ul
RT: 15.128 min Scan# 2030
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:165 Resp: 308741
Ion Ratio Lower Upper
165 100
63 36.8 29.4 44.2
182 2.5 2.0 3.0



#58
2,3,4,6-Tetrachlorophenol
Concen: 20.223 ng/ul
RT: 15.393 min Scan# 2075
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:232 Resp: 370314
Ion Ratio Lower Upper
232 100
131 35.4 28.3 42.5
130 1.9 1.5 2.3
166 26.8 21.4 32.2




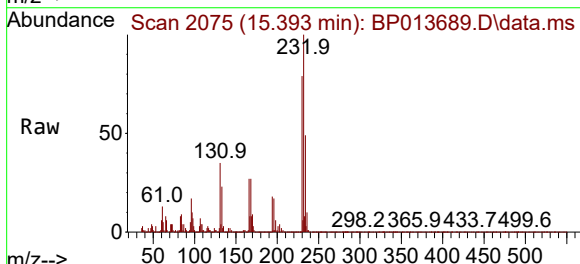




#59
Diethylphthalate
Concen: 20.604 ng/ul
RT: 15.581 min Scan# 2107
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:149 Resp: 1255000
Ion Ratio Lower Upper
149 100
177 24.0 19.2 28.8
150 12.5 10.0 15.0



#61
Fluorene
Concen: 20.571 ng/ul
RT: 15.822 min Scan# 2148
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:166 Resp: 1253778
Ion Ratio Lower Upper
166 100
165 98.2 78.6 117.8
167 13.6 10.9 16.3




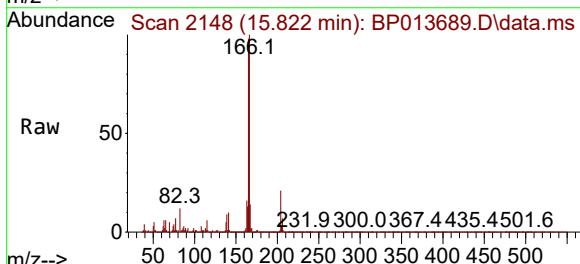




#62
4-Chlorophenyl-phenylether
Concen: 20.177 ng/ul
RT: 15.810 min Scan# 2146
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:204 Resp: 670002
Ion Ratio Lower Upper
204 100
206 32.7 26.2 39.2
141 49.6 39.7 59.5

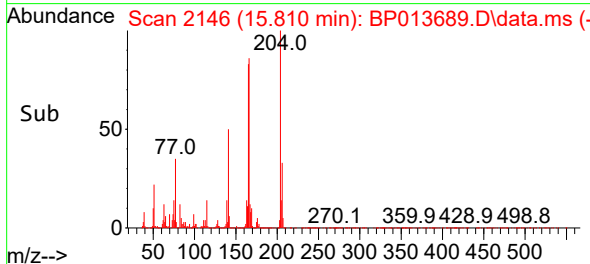

#63
4-Nitroaniline
Concen: 19.430 ng/ul
RT: 15.834 min Scan# 2150
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:138 Resp: 173874
Ion Ratio Lower Upper
138 100
92 52.1 41.7 62.5
108 77.5 62.0 93.0


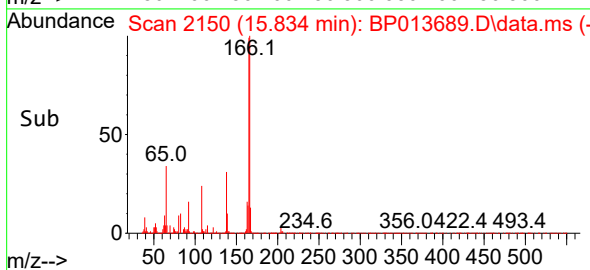

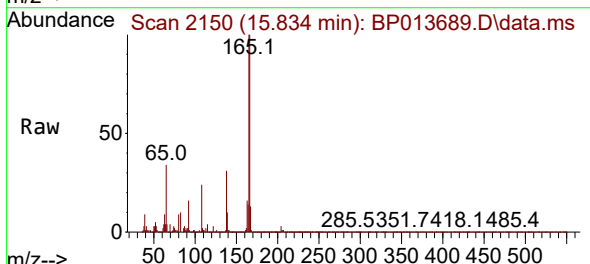




#66
4,6-Dinitro-2-methylphenol
Concen: 17.912 ng/ul
RT: 15.892 min Scan# 2160
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:198 Resp: 201052
Ion Ratio Lower Upper
198 100
182 4.4 3.5 5.3
77 20.9 16.7 25.1



#67
N-Nitrosodiphenylamine
Concen: 20.176 ng/ul
RT: 16.022 min Scan# 2182
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:169 Resp: 1095986
Ion Ratio Lower Upper
169 100
168 66.2 53.0 79.4
167 36.1 28.9 43.3




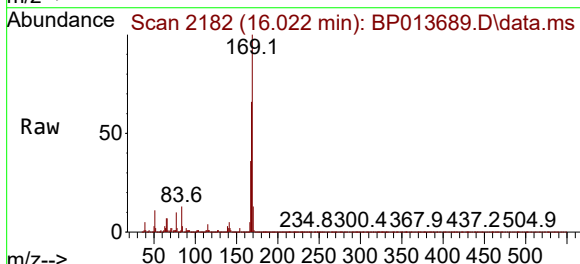




#68
4-Bromophenyl-phenylether
Concen: 20.510 ng/ul
RT: 16.710 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:248 Resp: 469627
Ion Ratio Lower Upper
248 100
250 98.0 78.4 117.6
141 55.2 44.2 66.2



#69
Hexachlorobenzene
Concen: 20.655 ng/ul
RT: 16.828 min Scan# 2319
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:284 Resp: 554841
Ion Ratio Lower Upper
284 100
142 26.8 21.4 32.2
249 30.6 24.5 36.7





#70

Atrazine

Concen: 20.516 ng/ul

RT: 16.975 min Scan# 2344

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:200 Resp: 448542

Ion Ratio Lower Upper

200 100

173 24.3 19.4 29.2

215 50.3 40.2 60.4



#71

Pentachlorophenol

Concen: 19.224 ng/ul

RT: 17.169 min Scan# 2377

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:266 Resp: 329622


Ion Ratio Lower Upper

266 100

264 64.0 51.2 76.8

268 64.8 51.8 77.8





#72

Phenanthrene

Concen: 20.822 ng/ul

RT: 17.569 min Scan# 2445

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:178 Resp: 2213539

Ion Ratio Lower Upper

178 100

179 15.7 12.6 18.8

176 19.3 15.4 23.2



#74

Anthracene

Concen: 20.914 ng/ul

RT: 17.663 min Scan# 2461

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:178 Resp: 2251892


Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.4

176 18.7 15.0 22.4









#75
1,2,3,4-Tetrachlorobenzene
Concen: 21.027 ng/uL
RT: 13.581 min Scan# 1767
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16




Instrument :
BNA_P
ClientSampleId :
SSTD020605


Tgt Ion:216 Resp: 602892
Ion Ratio Lower Upper
216 100
214 76.7 61.4 92.0
218 48.0 38.4 57.6



#76
Pentachlorobenzene
Concen: 19.581 ng/uL
RT: 15.093 min Scan# 2024
Delta R.T. 0.000 min
Lab File: BP013689.D
Acq: 01 Feb 2023 11:16

Tgt Ion:250 Resp: 575562
Ion Ratio Lower Upper
250 100
248 62.9 50.3 75.5
252 64.8 51.8 77.8





#77

Carbazole

Concen: 21.380 ng/ul

RT: 17.922 min Scan# 2505

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:167 Resp: 1997129

Ion Ratio Lower Upper

167 100

166 21.4 17.1 25.7

139 11.8 9.4 14.2



#78

Di-n-butylphthalate

Concen: 20.704 ng/ul

RT: 18.457 min Scan# 2596

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:149 Resp: 2285107


Ion Ratio Lower Upper

149 100

150 9.2 7.4 11.0

104 4.8 3.8 5.8

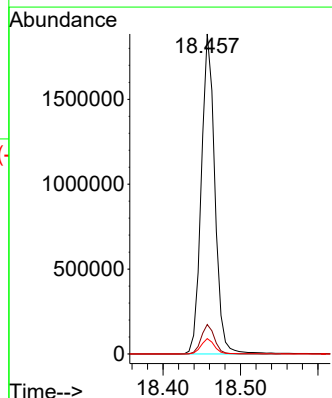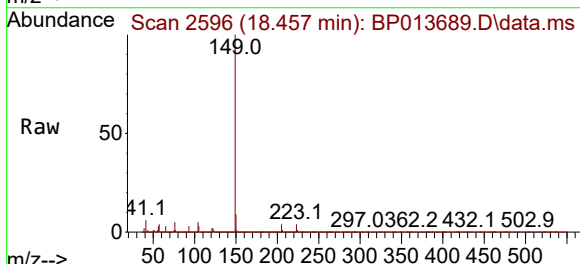



#80

Fluoranthene

Concen: 20.096 ng/ul

RT: 19.522 min Scan# 2777

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:202 Resp: 2803717

Ion Ratio Lower Upper

202 100

101 9.5 7.6 11.4

100 7.1 5.7 8.5

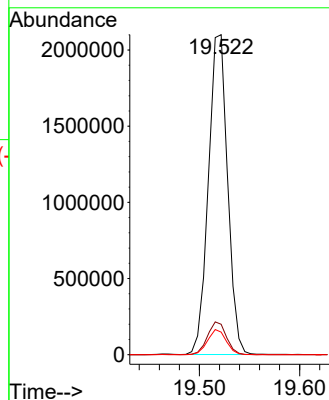

#82

Pyrene

Concen: 20.414 ng/ul

RT: 19.875 min Scan# 2837

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:202 Resp: 2911909


Ion Ratio Lower Upper

202 100

101 11.0 8.8 13.2

100 9.1 7.3 10.9

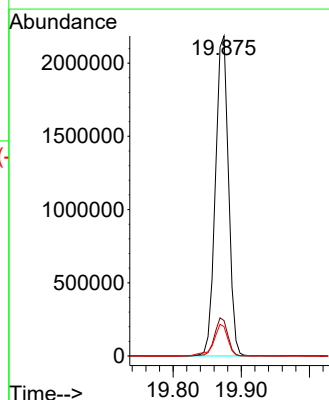



#83

Butylbenzylphthalate

Concen: 19.857 ng/ul

RT: 20.728 min Scan# 2982

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:149 Resp: 813806

Ion Ratio Lower Upper

149 100

91 67.4 53.9 80.9

206 24.3 19.4 29.2



#84

3,3'-Dichlorobenzidine

Concen: 20.344 ng/ul

RT: 21.510 min Scan# 3115

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:252 Resp: 991659


Ion Ratio Lower Upper

252 100

254 65.8 52.6 79.0

126 8.8 7.0 10.6





#85

Benzo(a)anthracene

Concen: 20.700 ng/ul

RT: 21.586 min Scan# 3128

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:228 Resp: 3054191

Ion Ratio Lower Upper

228 100

229 19.8 15.8 23.8

226 27.5 22.0 33.0



#86

Bis(2-ethylhexyl)phthalate

Concen: 19.441 ng/ul

RT: 21.486 min Scan# 3111

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:149 Resp: 1365970


Ion Ratio Lower Upper

149 100

167 28.4 22.7 34.1

279 4.9 3.9 5.9





#87

Chrysene

Concen: 20.661 ng/ul

RT: 21.645 min Scan# 3138

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:228 Resp: 2870028

Ion Ratio Lower Upper

228 100

226 30.6 24.5 36.7

229 19.6 15.7 23.5



#89

Di-n-octyl phthalate

Concen: 18.799 ng/ul




RT: 22.469 min Scan# 3278


Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Tgt Ion:149 Resp: 2415156





#90

Benzo(b)fluoranthene

Concen: 20.043 ng/ul

RT: 23.386 min Scan# 3434

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:252 Resp: 3190986

Ion Ratio Lower Upper

252 100

253 22.3 17.8 26.8

125 8.1 6.5 9.7

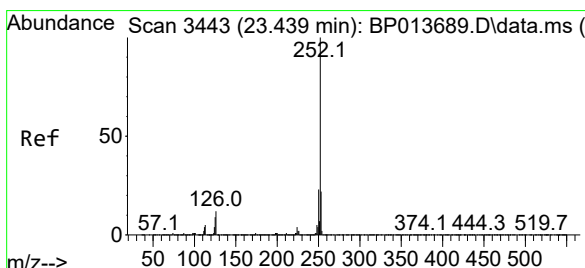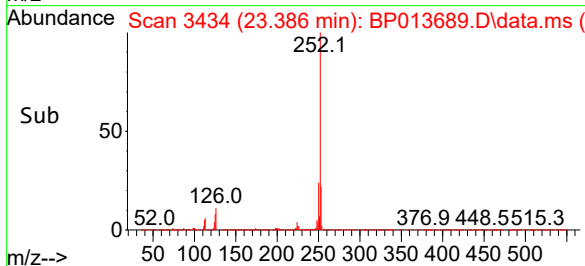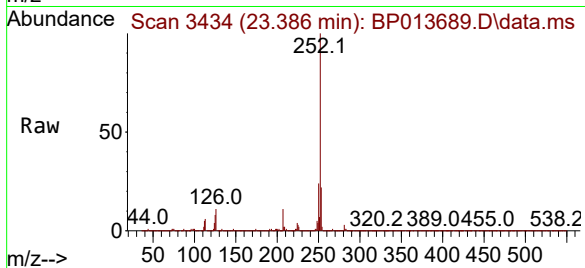

#91

Benzo(k)fluoranthene

Concen: 20.817 ng/ul

RT: 23.439 min Scan# 3443

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:252 Resp: 3167493


Ion Ratio Lower Upper

252 100

253 21.9 17.5 26.3

125 8.4 6.7 10.1

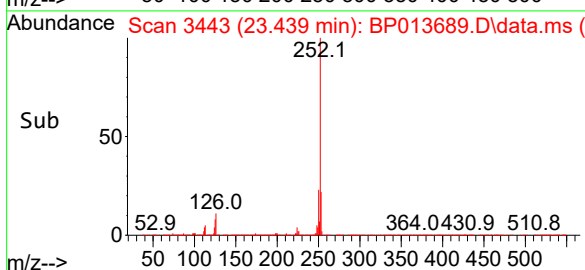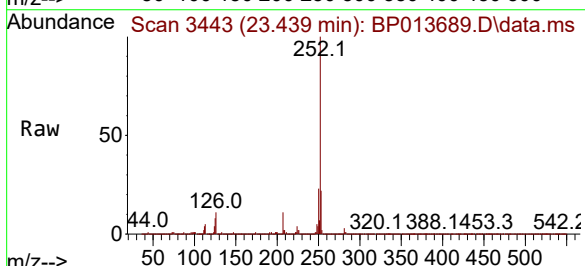



#93

Benzo(a)pyrene

Concen: 20.712 ng/ul

RT: 24.063 min Scan# 3549

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16

Instrument :

BNA_P

ClientSampleId :

SSTD020605





Tgt Ion:252 Resp: 2846712

Ion Ratio Lower Upper

252 100

253 21.9 17.5 26.3

125 9.1 7.3 10.9



#94

Indeno(1,2,3-cd)pyrene

Concen: 21.738 ng/ul

RT: 26.892 min Scan# 4030

Delta R.T. 0.000 min

Lab File: BP013689.D

Acq: 01 Feb 2023 11:16




Tgt Ion:276 Resp: 3701785


Ion Ratio Lower Upper

276 100

138 18.8 15.0 22.6

277 25.2 20.2 30.2









#95
 Dibenzo(a,h)anthracene
 Concen: 21.767 ng/ul
 RT: 26.915 min Scan# 4034
 Delta R.T. 0.000 min
 Lab File: BP013689.D
 Acq: 01 Feb 2023 11:16

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020605

Tgt Ion:278 Resp: 3072904

Ion	Ratio	Lower	Upper
278	100		
139	12.8	10.2	15.4
279	23.8	19.0	28.6

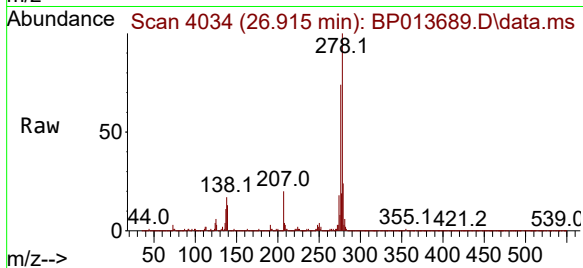

#96
 Benzo(g,h,i)perylene
 Concen: 21.908 ng/ul
 RT: 27.733 min Scan# 4173
 Delta R.T. 0.000 min
 Lab File: BP013689.D
 Acq: 01 Feb 2023 11:16

Tgt Ion:276 Resp: 2951405

Ion	Ratio	Lower	Upper
276	100		
138	17.9	14.3	21.5
277	24.0	19.2	28.8

