

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013737.D
 Acq On : 03 Feb 2023 13:09
 Operator : CG/JU
 Sample : 01316-14
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44J3

Quant Time: Feb 03 23:16:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	234223	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1043517	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.769	164	771456	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.522	188	1940672	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	2132656	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	2208256	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.475	96	25966	4.700	ng/uL	0.00
4) Pyridine-d5	3.917	84	151489	9.557	ng/u1	0.00
7) Phenol-d5	7.275	99	144602	7.024	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	386871	32.043	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.658	132	365972	24.252	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	276439	16.845	ng/u1	-0.01
21) Nitrobenzene-d5	9.305	128	220635	33.144	ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	239923	30.926	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	525842	28.985	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.093	131	578866	24.159	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	2109389	34.688	ng/u1	0.00
49) Acenaphthylene-d8	14.463	160	2202574	32.783	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	42877	4.183	ng/u1	0.00
60) Fluorene-d10	15.757	176	1848594	35.268	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	265507	24.414	ng/u1	0.00
73) Anthracene-d10	17.622	188	3361221	37.157	ng/u1	0.00
81) Pyrene-d10	19.839	212	4555098	38.295	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	4458564	39.551	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.511	88	22569	3.920 ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013737.D
Acq On : 03 Feb 2023 13:09
Operator : CG/JU
Sample : 01316-14
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44J3

Quant Time: Feb 03 23:16:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

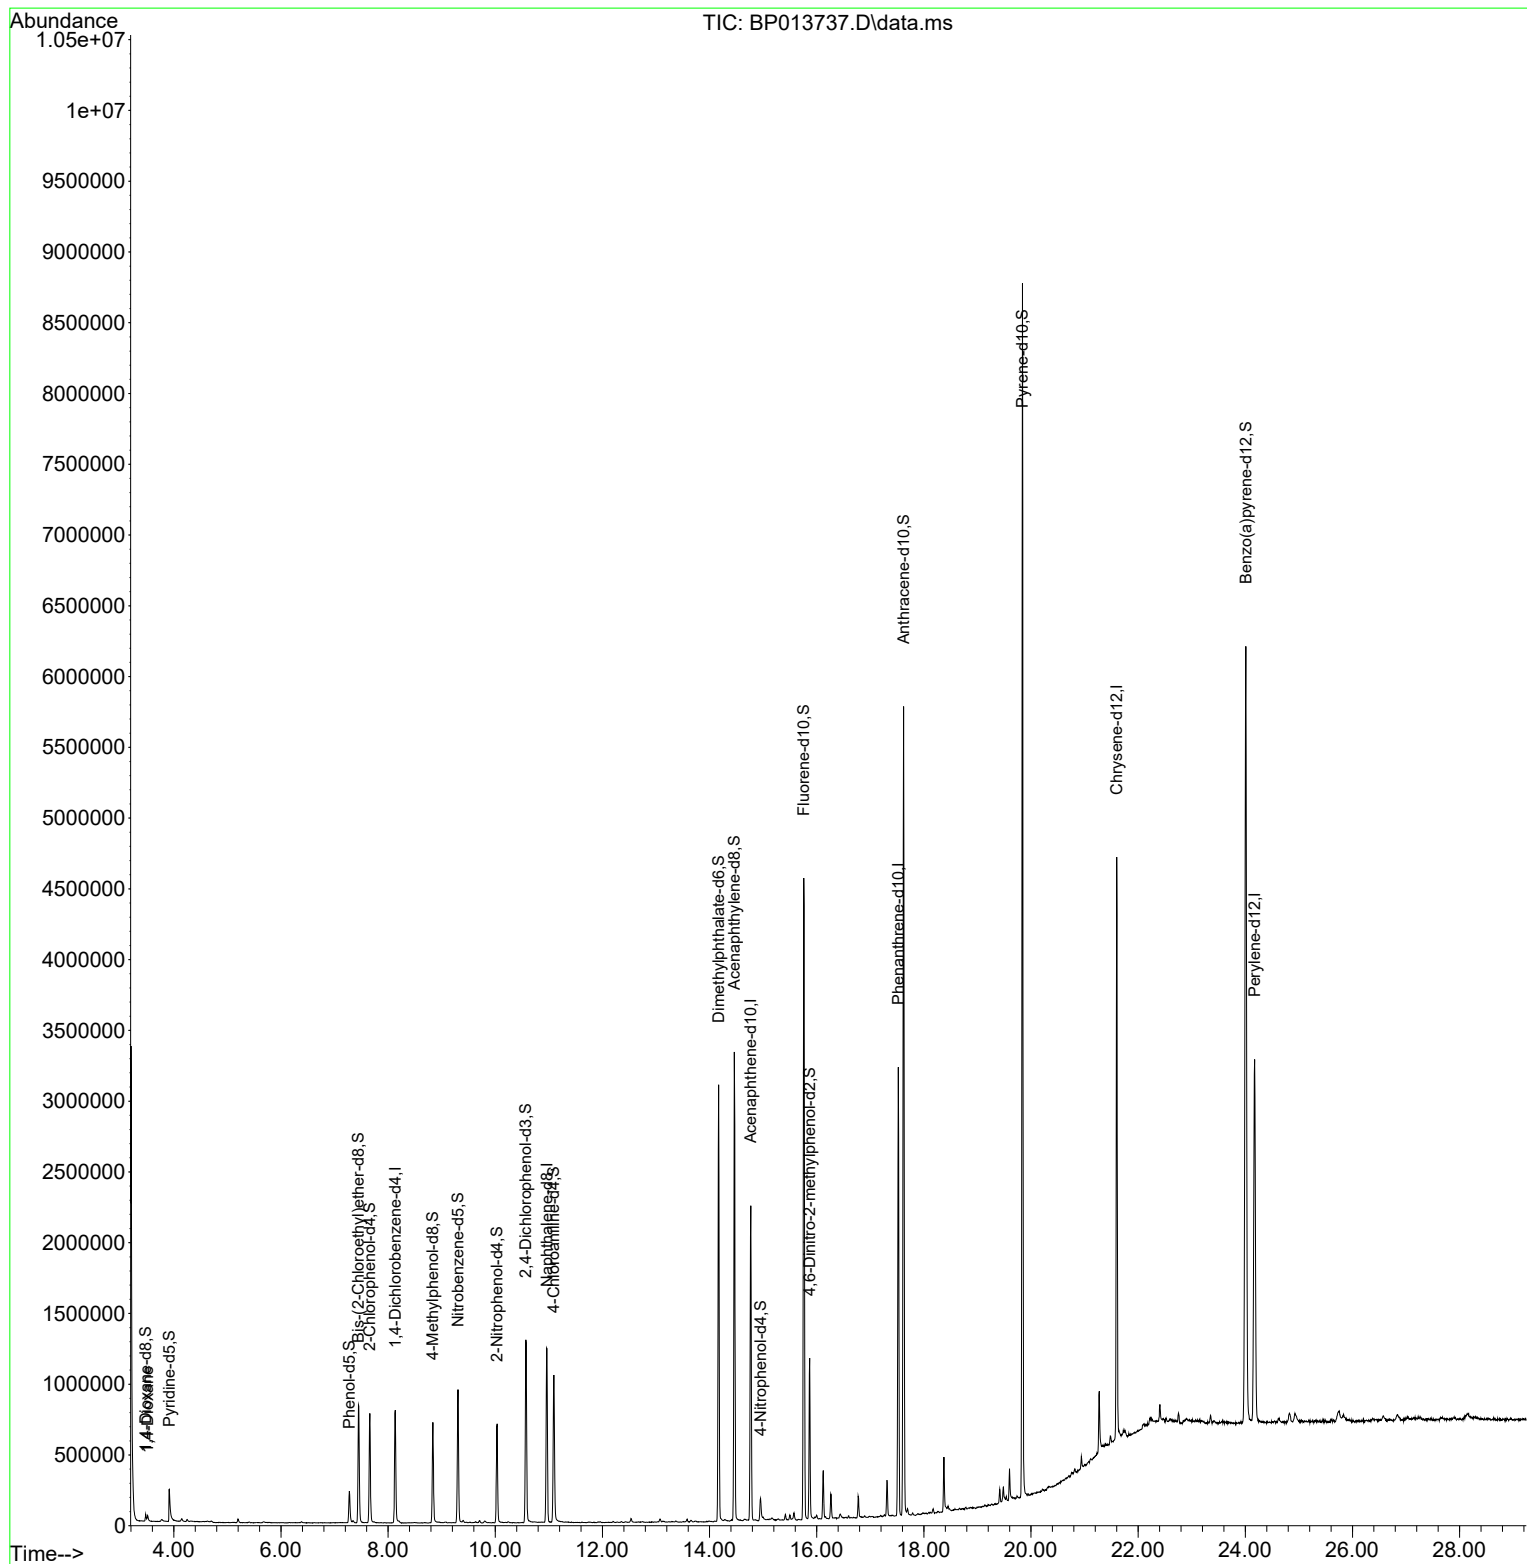

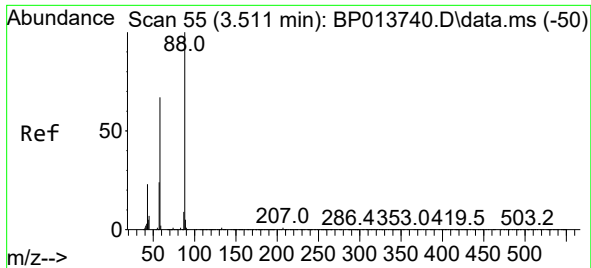

#2
 1,4-Dioxane
 Concen: 3.920 ng/uL
 RT: 3.511 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: BP013737.D
 Acq: 03 Feb 2023 13:09

Instrument :
 BNA_P
 ClientSampleId :
 A44J3

Tgt Ion: 88 Resp: 22569
 Ion Ratio Lower Upper
 88 100
 43 28.8 22.2 33.4
 58 68.0 54.9 82.3

