

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013747.D
 Acq On : 03 Feb 2023 18:57
 Operator : CG/JU
 Sample : 01381-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44N2

Quant Time: Feb 03 23:53:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	203142	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	843619	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.769	164	632794	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.522	188	1629745	20.000	ng/ul	0.00
79) Chrysene-d12	21.598	240	1902673	20.000	ng/ul	0.00
88) Perylene-d12	24.168	264	2195025	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.440	96	194076	40.505	ng/uL	-0.04
4) Pyridine-d5	3.917	84	91891	6.684	ng/ul	0.00
7) Phenol-d5	7.275	99	92096	5.158	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	305413	29.167	ng/ul	0.00
11) 2-Chlorophenol-d4	7.658	132	284379	21.729	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	171368	12.040	ng/ul	0.00
21) Nitrobenzene-d5	9.305	128	172916	32.130	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	206004	32.846	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	402475	27.442	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	358404	18.503	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	1537513	30.824	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	1643226	29.817	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	32695	3.889	ng/ul	0.00
60) Fluorene-d10	15.757	176	1444181	33.590	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	187099	20.486	ng/ul	0.00
73) Anthracene-d10	17.622	188	2524579	33.232	ng/ul	0.00
81) Pyrene-d10	19.833	212	3335558	31.432	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.998	264	3726844	33.260	ng/ul	0.00
Target Compounds						
					Qvalue	
13) 2-Methylphenol	8.505	108	81415	5.836	ng/ul	98
22) Nitrobenzene	9.346	77	1103663	75.929	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013747.D
Acq On : 03 Feb 2023 18:57
Operator : CG/JU
Sample : 01381-13
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44N2

Quant Time: Feb 03 23:53:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 03 23:44:43 2023
Response via : Initial Calibration




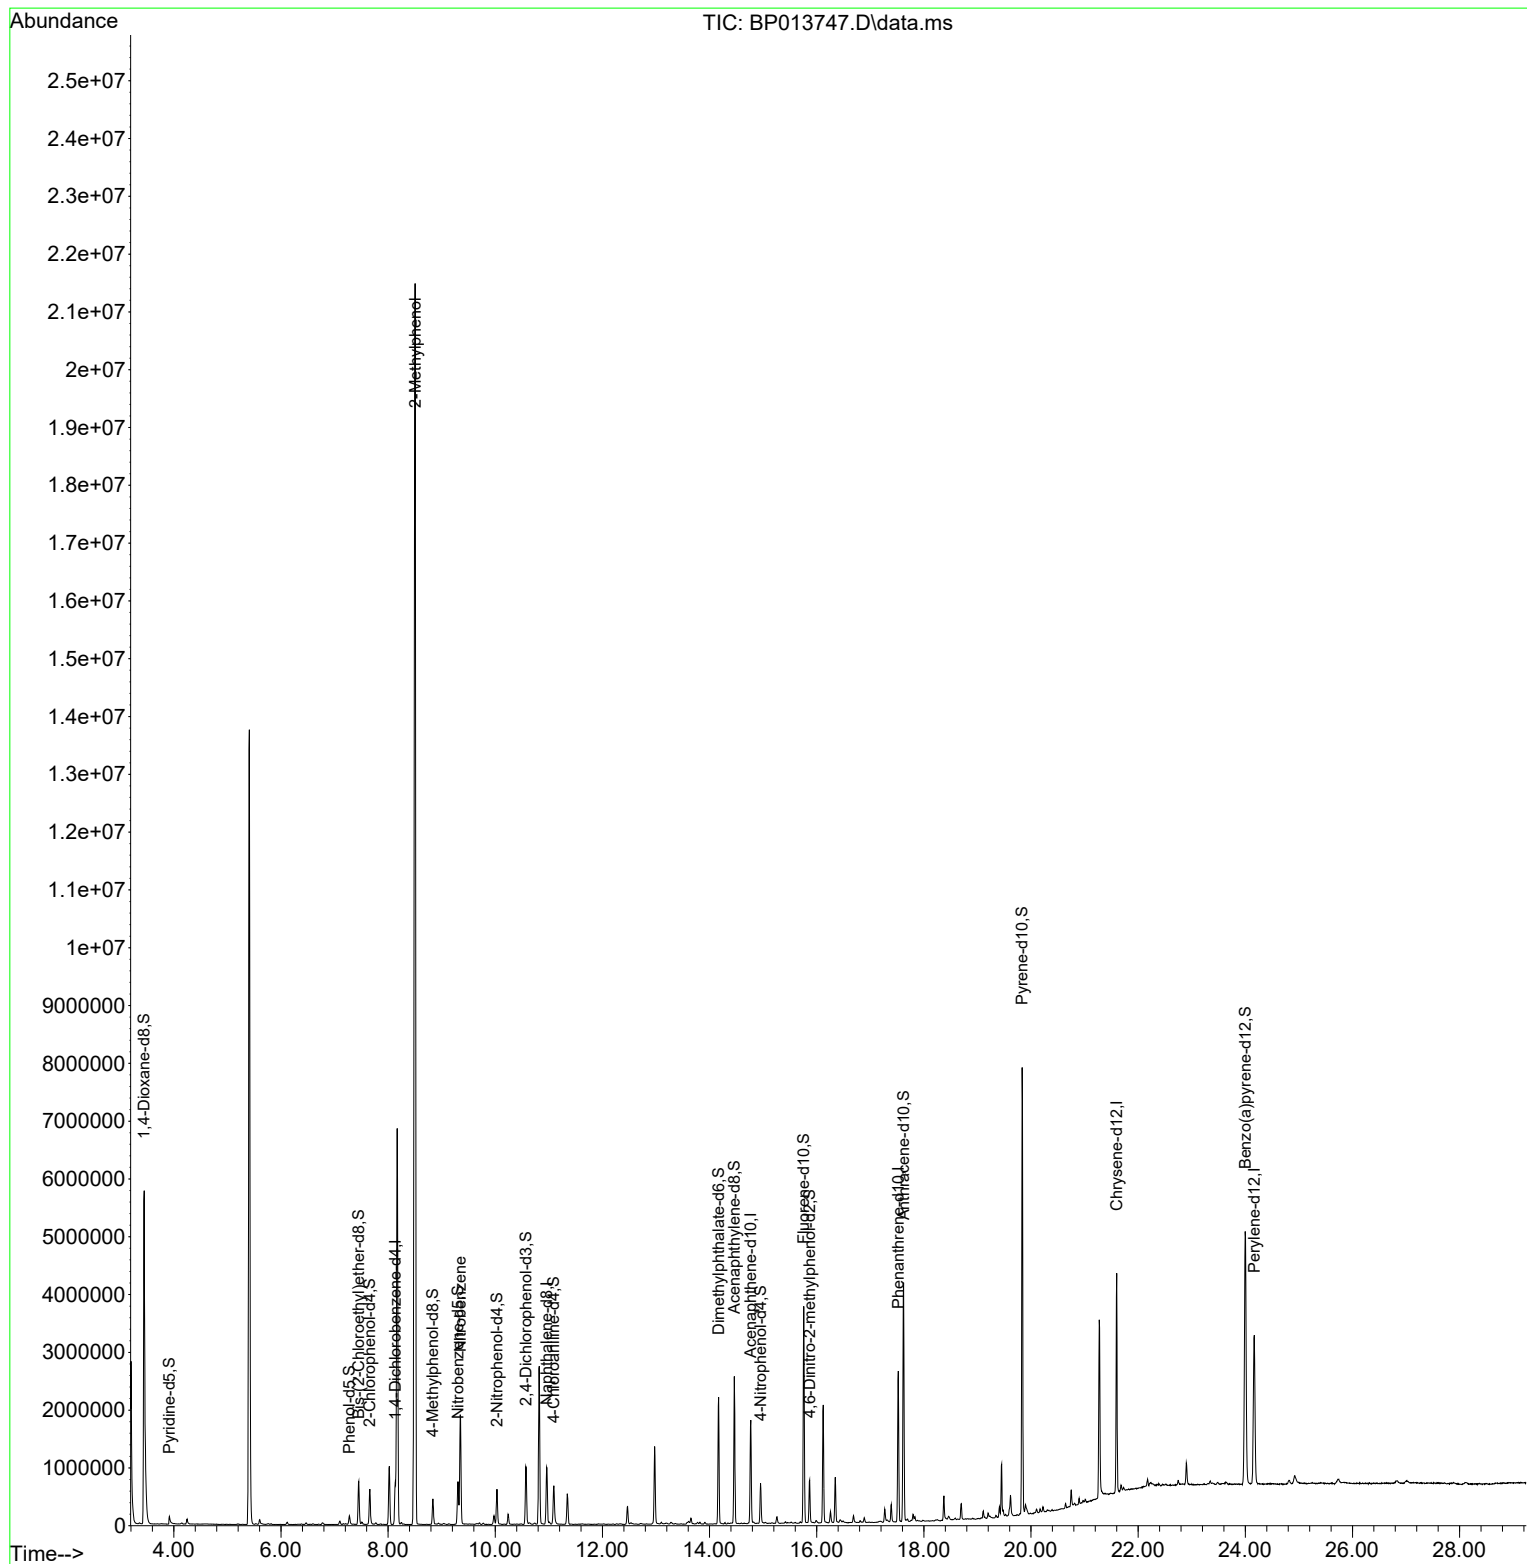


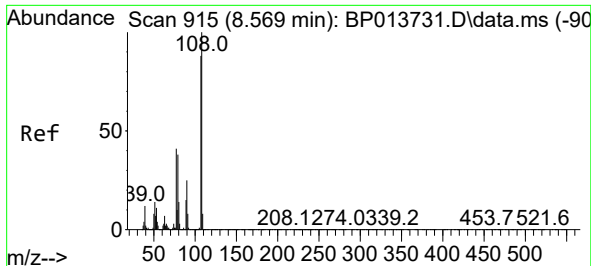

#13
2-Methylphenol
Concen: 5.836 ng/ul
RT: 8.505 min Scan# 904
Delta R.T. -0.065 min
Lab File: BP013747.D
Acq: 03 Feb 2023 18:57

Instrument :
BNA_P
ClientSampleId :
A44N2

Tgt Ion:108 Resp: 81415
Ion Ratio Lower Upper
108 100
107 90.1 70.9 106.3

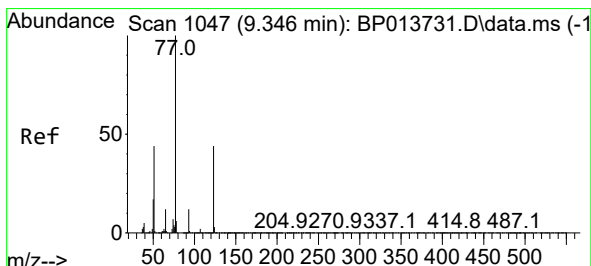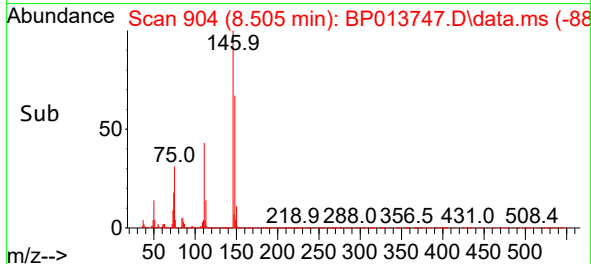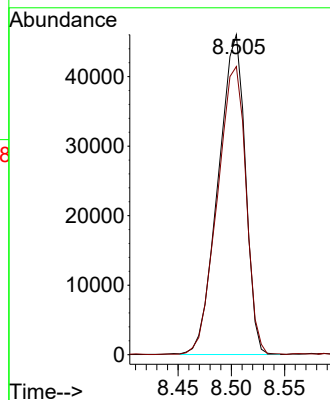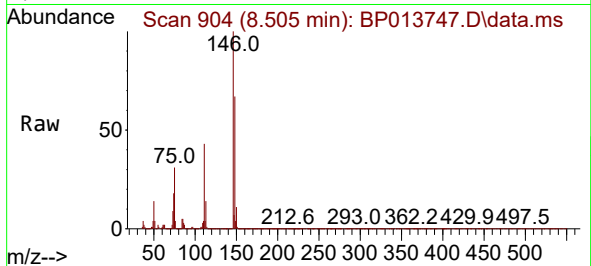

#22
Nitrobenzene
Concen: 75.929 ng/ul
RT: 9.346 min Scan# 1047
Delta R.T. -0.000 min
Lab File: BP013747.D
Acq: 03 Feb 2023 18:57

Tgt Ion: 77 Resp: 1103663
Ion Ratio Lower Upper
77 100
123 43.4 34.1 51.1
65 12.8 9.8 14.8

