

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013753.D
 Acq On : 03 Feb 2023 22:21
 Operator : CG/JU
 Sample : 01381-17
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q5

Quant Time: Feb 03 23:54:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	285950	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1230797	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.769	164	929141	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.522	188	2392753	20.000	ng/ul	0.00
79) Chrysene-d12	21.598	240	2726356	20.000	ng/ul	0.00
88) Perylene-d12	24.168	264	3018659	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.475	96	39937	5.921	ng/uL	0.00
4) Pyridine-d5	3.916	84	126260	6.524	ng/ul	0.00
7) Phenol-d5	7.275	99	118874	4.730	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	443318	30.076	ng/ul	0.00
11) 2-Chlorophenol-d4	7.657	132	397910	21.599	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	243365	12.147	ng/ul	0.00
21) Nitrobenzene-d5	9.304	128	256510	32.670	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	306459	33.492	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	581654	27.183	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	626911	22.183	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	2378699	32.478	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	2520787	31.152	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	42932	3.478	ng/ul	0.00
60) Fluorene-d10	15.757	176	2134930	33.818	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	325985	24.311	ng/ul	0.00
73) Anthracene-d10	17.616	188	3829511	34.335	ng/ul	0.00
81) Pyrene-d10	19.839	212	5105128	33.573	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.998	264	5414960	35.139	ng/ul	0.00
Target Compounds						
13) 2-Methylphenol	8.499	108	59111	3.010	ng/ul	98
22) Nitrobenzene	9.346	77	1486780	70.109	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013753.D
Acq On : 03 Feb 2023 22:21
Operator : CG/JU
Sample : 01381-17
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q5

Quant Time: Feb 03 23:54:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 03 23:44:43 2023
Response via : Initial Calibration

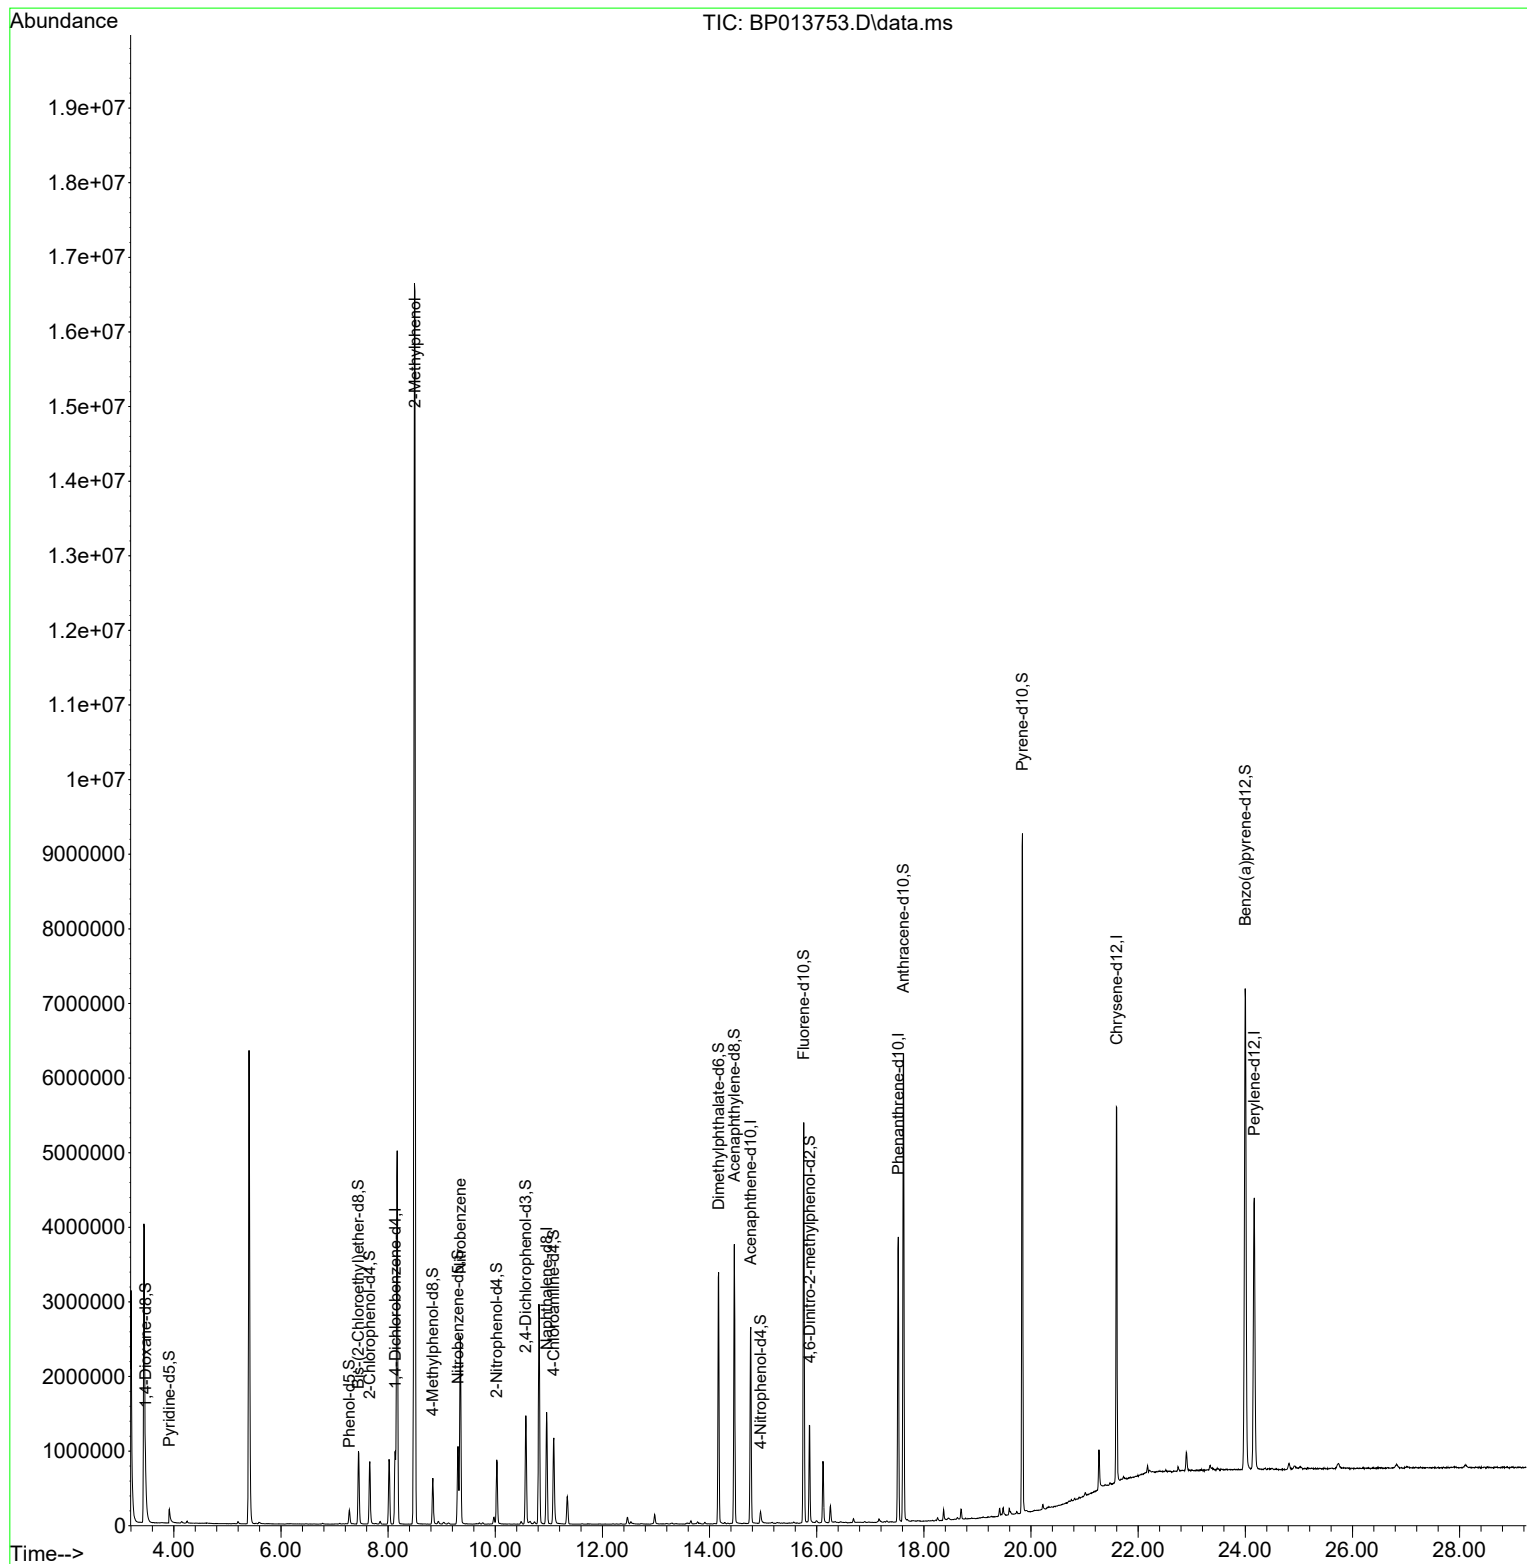

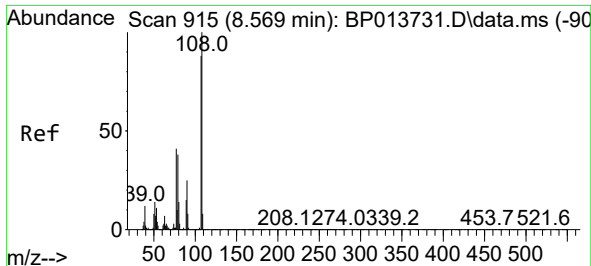

#13

2-Methylphenol

Concen: 3.010 ng/ul

RT: 8.499 min Scan# 90

Delta R.T. -0.071 min

Lab File: BP013753.D

Acq: 03 Feb 2023 22:21

Instrument :

BNA_P

ClientSampleId :





A44Q5

Tgt Ion:108 Resp: 59111

Ion Ratio Lower Upper

108 100

107 90.7 70.9 106.3

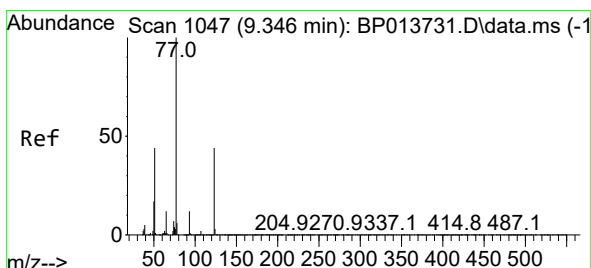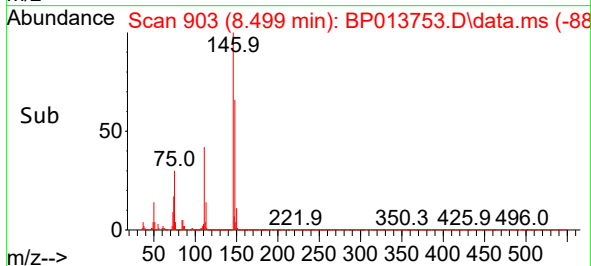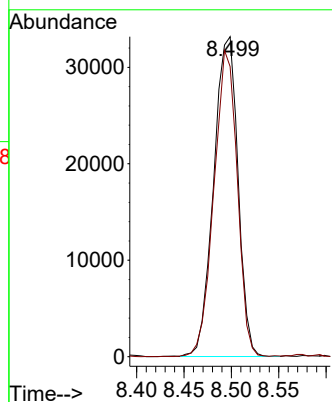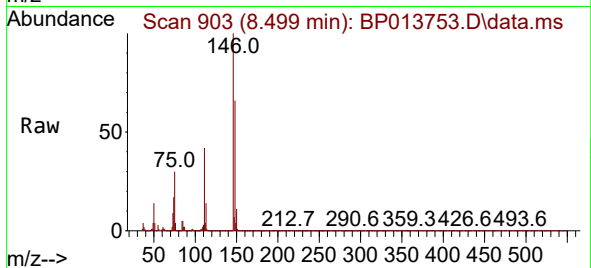

#22

Nitrobenzene

Concen: 70.109 ng/ul

RT: 9.346 min Scan# 1047

Delta R.T. -0.000 min

Lab File: BP013753.D

Acq: 03 Feb 2023 22:21

Tgt Ion: 77 Resp: 1486780

Ion Ratio Lower Upper

77 100

123 43.7 34.1 51.1

65 12.4 9.8 14.8

