




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013729.D
 Acq On : 03 Feb 2023 02:19
 Operator : CG/JU
 Sample : 01362-15
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4489

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 02/03/2023
 Supervised By :Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 03:01:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

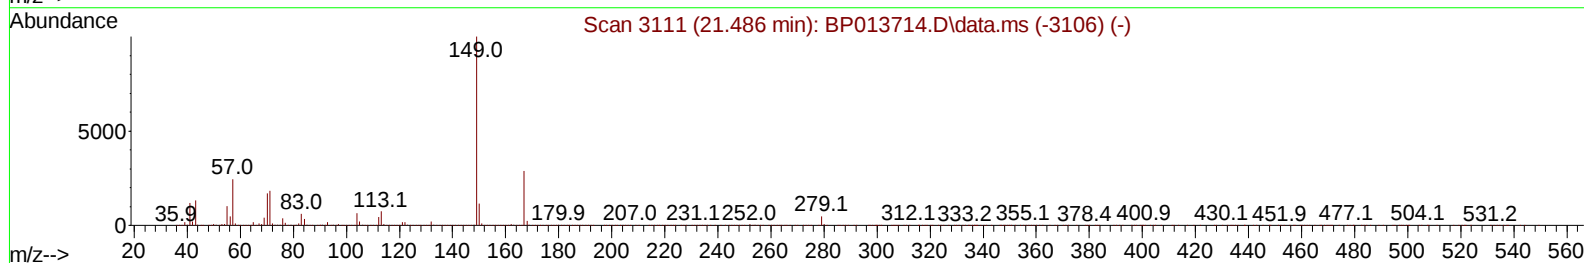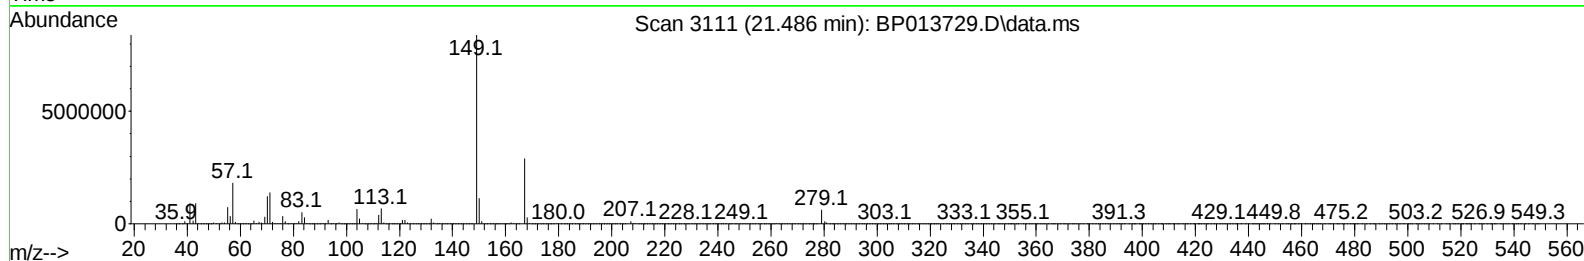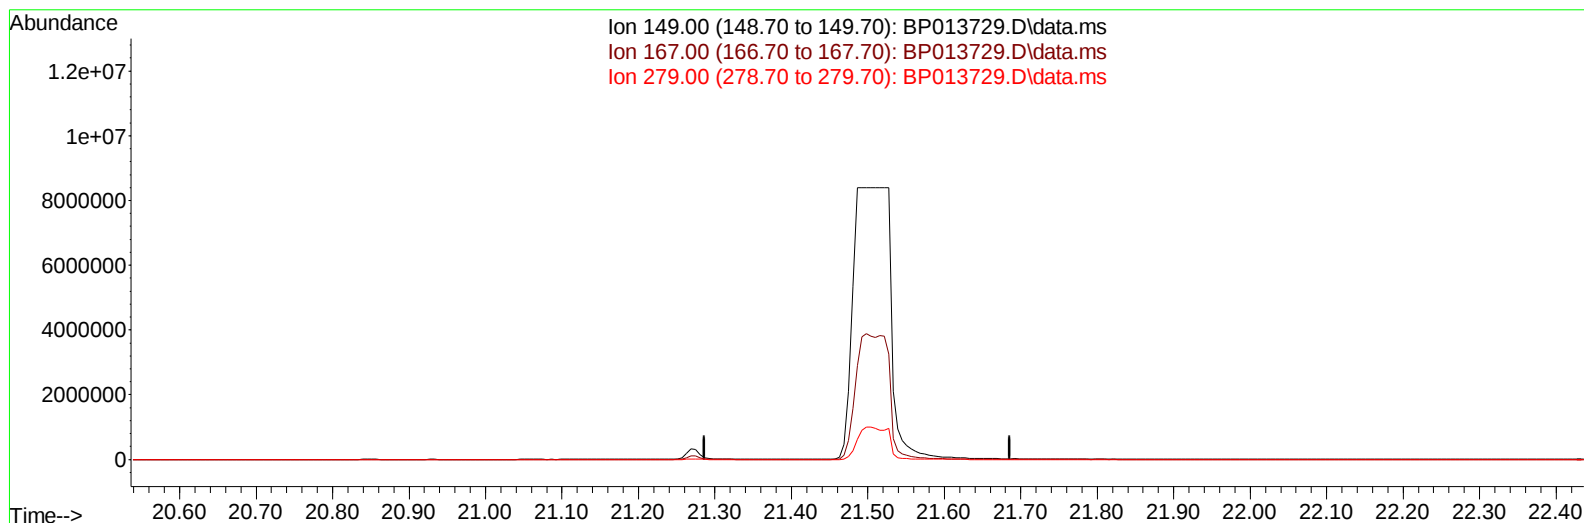

TIC: BP013729.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.486min (-21.486) 0.00 ng/u1

response 0

Ion	Exp%	Act%
149.00	100.00	0.00
167.00	28.40	0.00#
279.00	4.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013729.D
Acq On : 03 Feb 2023 02:19
Operator : CG/JU
Sample : 01362-15
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4489

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 02/03/2023
Supervised By :Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 03:01:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

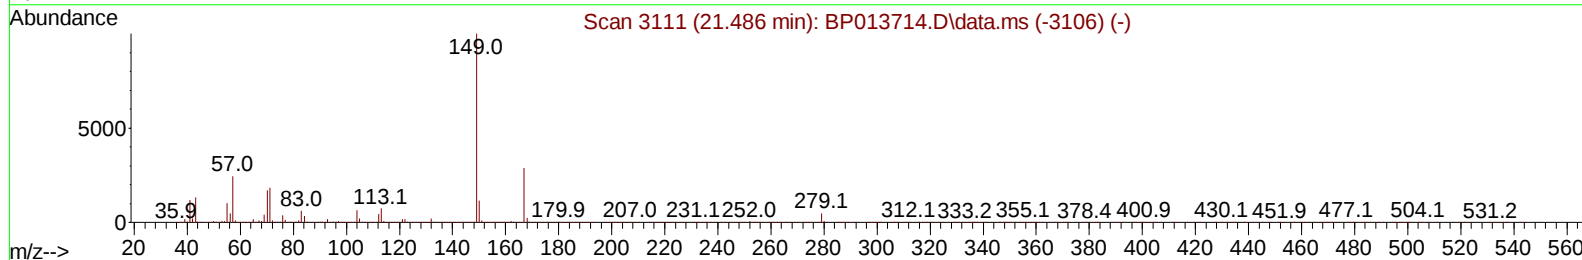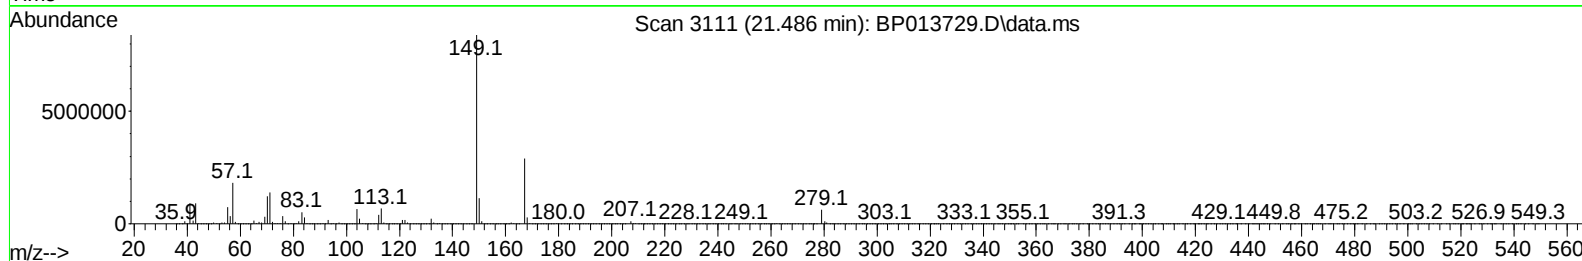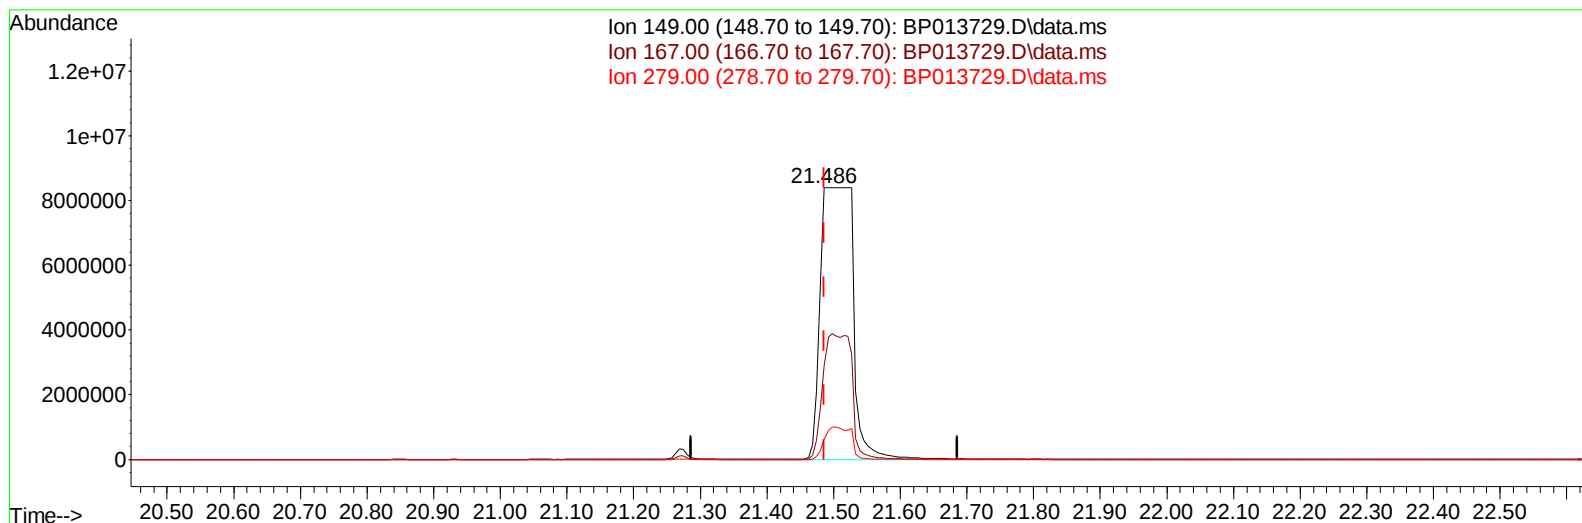

TIC: BP013729.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.486min (-0.000) 477.42 ng/ul m

response 28515428

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	28.40	34.60#
279.00	4.90	7.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013729.D
 Acq On : 03 Feb 2023 02:19
 Operator : CG/JU
 Sample : 01362-15
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4489

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 02/03/2023
 Supervised By :Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 03:01:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	409259	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	1685446	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.769	164	1148268	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.528	188	2521409	20.000	ng/ul	0.00
79) Chrysene-d12	21.598	240	1824370	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1749074	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0d	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0d	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0d	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0d	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
						Qvalue
43) 1,1'-Biphenyl	13.604	154	1227874	14.123	ng/ul	98
61) Fluorene	15.816	166	1834169	21.411	ng/ul#	54
86) Bis(2-ethylhexyl)phtha...	21.486	149	28515428m	477.417	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013729.D
Acq On : 03 Feb 2023 02:19
Operator : CG/JU
Sample : 01362-15
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4489

Manual IntegrationsAPPROVED

Quant Time: Feb 03 03:01:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 02/03/2023
Supervised By :Jagrut Upadhyay 02/03/2023

