

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013748.D
 Acq On : 03 Feb 2023 19:31
 Operator : CG/JU
 Sample : 01381-21
 Misc :
 ALS Vial : 49 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 A44Q6

Manual IntegrationsAPPROVED

Quant Time: Feb 03 23:53:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/06/2023
 Supervised By :mohammad ahmed 02/06/2023

02/06/2023
 Supervised By :mohammad
 ahmed

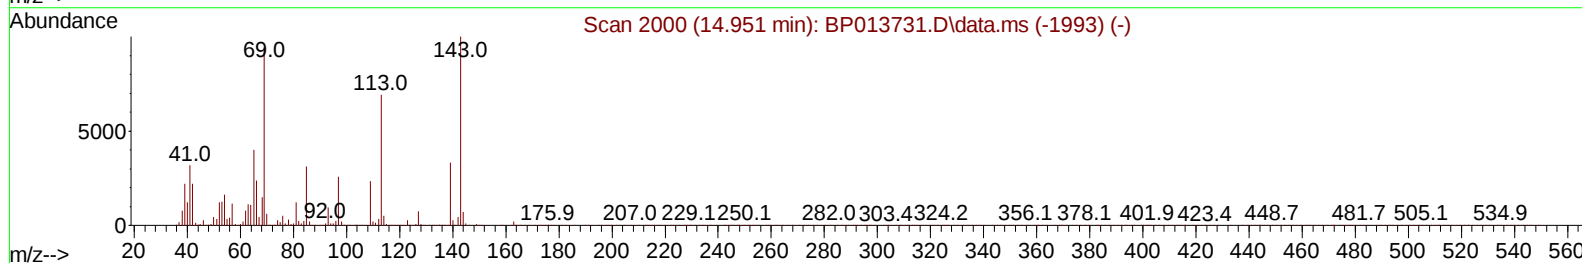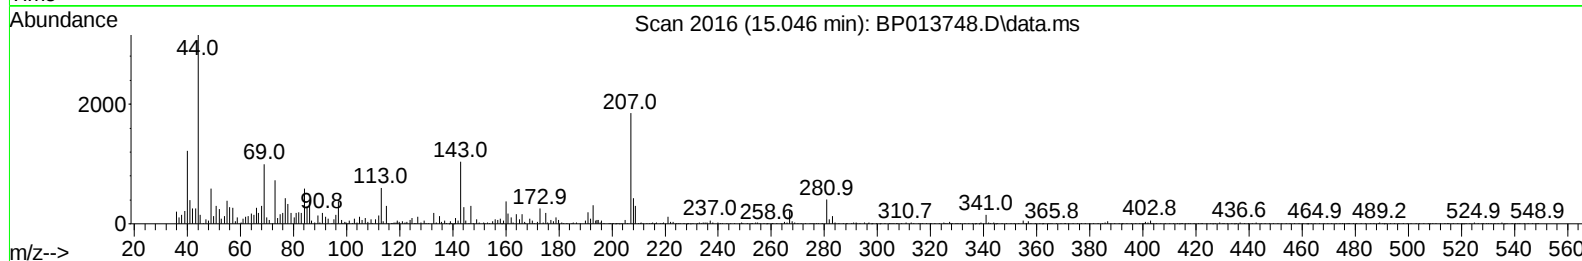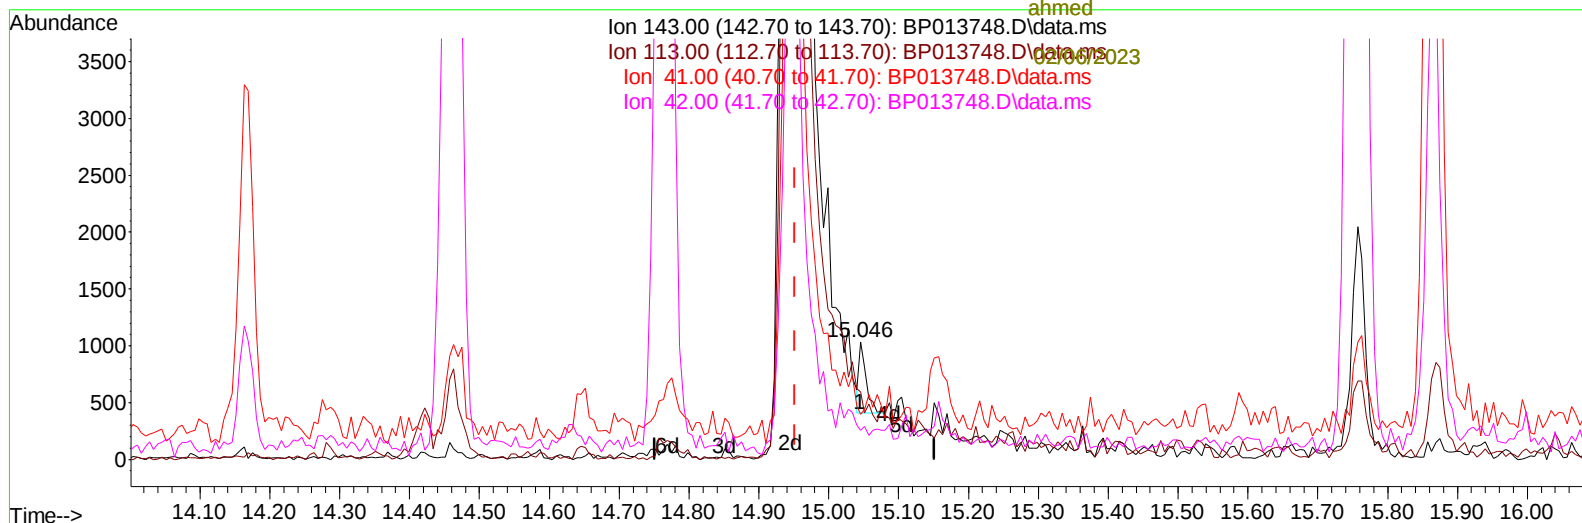

TIC: BP013748.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.046min (+ 0.094) 0.05 ng/u1

response 453

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	69.30	57.54
41.00	33.60	38.59
42.00	21.80	24.66

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013748.D
 Acq On : 03 Feb 2023 19:31
 Operator : CG/JU
 Sample : 01381-21
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6


Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/06/2023
 Supervised By :mohammad ahmed 02/06/2023


02/06/2023
 Supervised By :mohammad
 ahmed

Quant Time: Feb 03 23:53:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration


Ion 143.00 (142.70 to 143.70): BP013748.D\data.ms
 Ion 113.00 (112.70 to 113.70): BP013748.D\data.ms
 Ion 41.00 (40.70 to 41.70): BP013748.D\data.ms
 Ion 42.00 (41.70 to 42.70): BP013748.D\data.ms

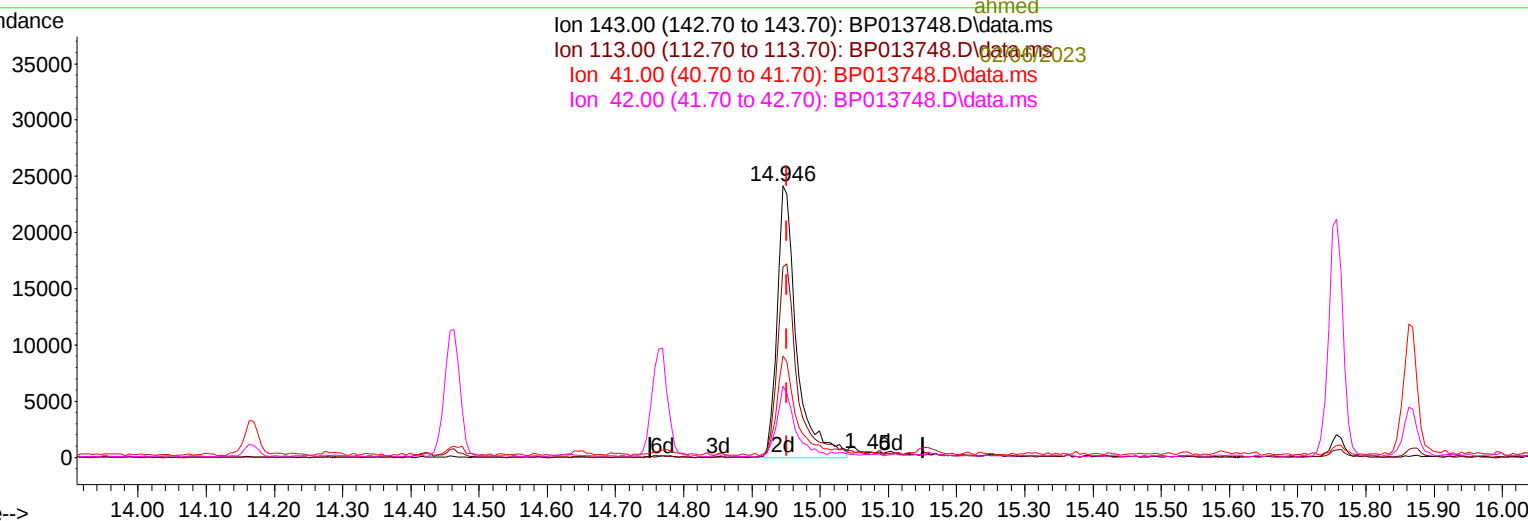

Scan 1999 (14.946 min): BP013748.D\data.ms

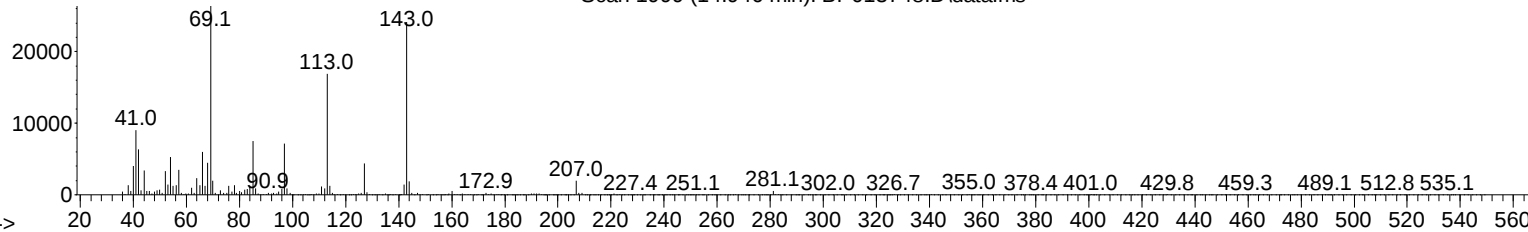

Scan 2000 (14.951 min): BP013731.D\data.ms (-1993) (-)

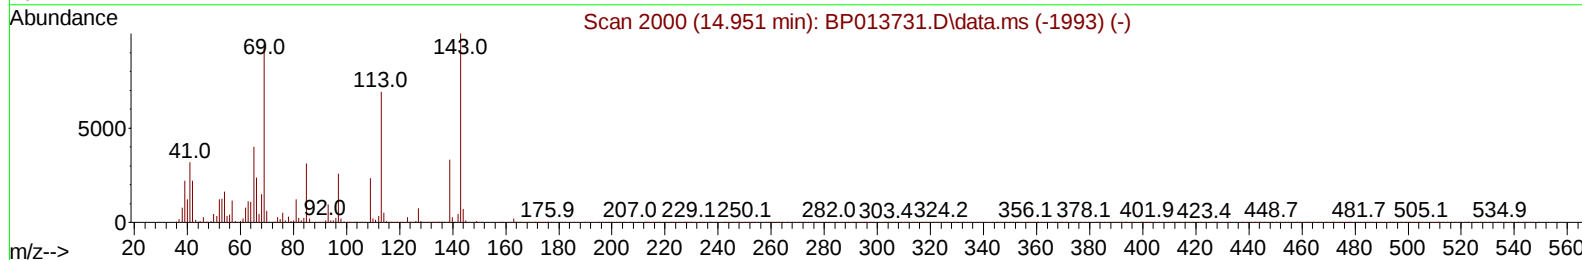

TIC: BP013748.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.946min (-0.006) 5.46 ng/ul m

response 47985

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	69.30	70.11
41.00	33.60	37.42
42.00	21.80	26.41#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013748.D
 Acq On : 03 Feb 2023 19:31
 Operator : CG/JU
 Sample : 01381-21
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/06/2023
 Supervised By :mohammad ahmed 02/06/2023

Quant Time: Feb 03 23:53:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----02/06/2023						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	211765	20.000	ng/ul	0.00
20) Naphthalene-d8	10.958	136	913815	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	661594	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.522	188	1807960	20.000	ng/ul	0.00
79) Chrysene-d12	21.598	240	2065317	20.000	ng/ul	0.00
88) Perylene-d12	24.169	264	2276333	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.476	96	25137	5.033	ng/uL	0.00
4) Pyridine-d5	3.917	84	104319	7.279	ng/ul	0.00
7) Phenol-d5	7.275	99	122118	6.561	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	351246	32.178	ng/ul	0.00
11) 2-Chlorophenol-d4	7.658	132	327953	24.038	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	222686	15.009	ng/ul	0.00
21) Nitrobenzene-d5	9.305	128	197074	33.806	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	239257	35.218	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	454537	28.611	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	360539	17.183	ng/ul	0.00
46) Dimethylphthalate-d6	14.169	166	1807301	34.655	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	1932131	33.533	ng/ul	0.00
54) 4-Nitrophenol-d4	14.946	143	47985m	5.459	ng/ul	0.00
60) Fluorene-d10	15.757	176	1740751	38.725	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	270793	26.727	ng/ul	0.00
73) Anthracene-d10	17.622	188	3235167	38.388	ng/ul	0.00
81) Pyrene-d10	19.839	212	4346919	37.737	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.004	264	4630823	39.851	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.352	77	3391764	215.419	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013748.D
Acq On : 03 Feb 2023 19:31
Operator : CG/JU
Sample : 01381-21
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/06/2023
Supervised By :mohammad ahmed 02/06/2023

02/06/2023
Supervised By :mohammad
ahmed

