

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013704.D
 Acq On : 02 Feb 2023 12:03
 Operator : CG/JU
 Sample : 01314-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L2

Quant Time: Feb 02 13:49:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.146	152	269064	20.000	ng/u1	0.00
20) Naphthalene-d8	10.975	136	1220793	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	895411	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.540	188	2259360	20.000	ng/u1	0.01
79) Chrysene-d12	21.616	240	2304299	20.000	ng/u1	0.01
88) Perylene-d12	24.198	264	2612629	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.481	96	24146	3.805	ng/uL	0.00
4) Pyridine-d5	3.923	84	158582	8.709	ng/u1	0.01
7) Phenol-d5	7.287	99	116325	4.919	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.464	67	341100	24.594	ng/u1	0.00
11) 2-Chlorophenol-d4	7.669	132	313545	18.088	ng/u1	0.00
15) 4-Methylphenol-d8	8.852	113	239094	12.683	ng/u1	0.00
21) Nitrobenzene-d5	9.316	128	177436	22.784	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	208534	22.977	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	497750	23.453	ng/u1	0.00
31) 4-Chloroaniline-d4	11.105	131	610298	21.772	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	1941242	27.503	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2072423	26.575	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	36829	3.096	ng/u1	0.01
60) Fluorene-d10	15.775	176	1799817	29.584	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.887	200	191187	15.100	ng/u1	0.01
73) Anthracene-d10	17.634	188	3077210	29.219	ng/u1	0.00
81) Pyrene-d10	19.851	212	3751981	29.194	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.033	264	3952118	29.632	ng/u1	0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.498	149	425938	5.646	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013704.D
Acq On : 02 Feb 2023 12:03
Operator : CG/JU
Sample : 01314-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L2

Quant Time: Feb 02 13:49:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

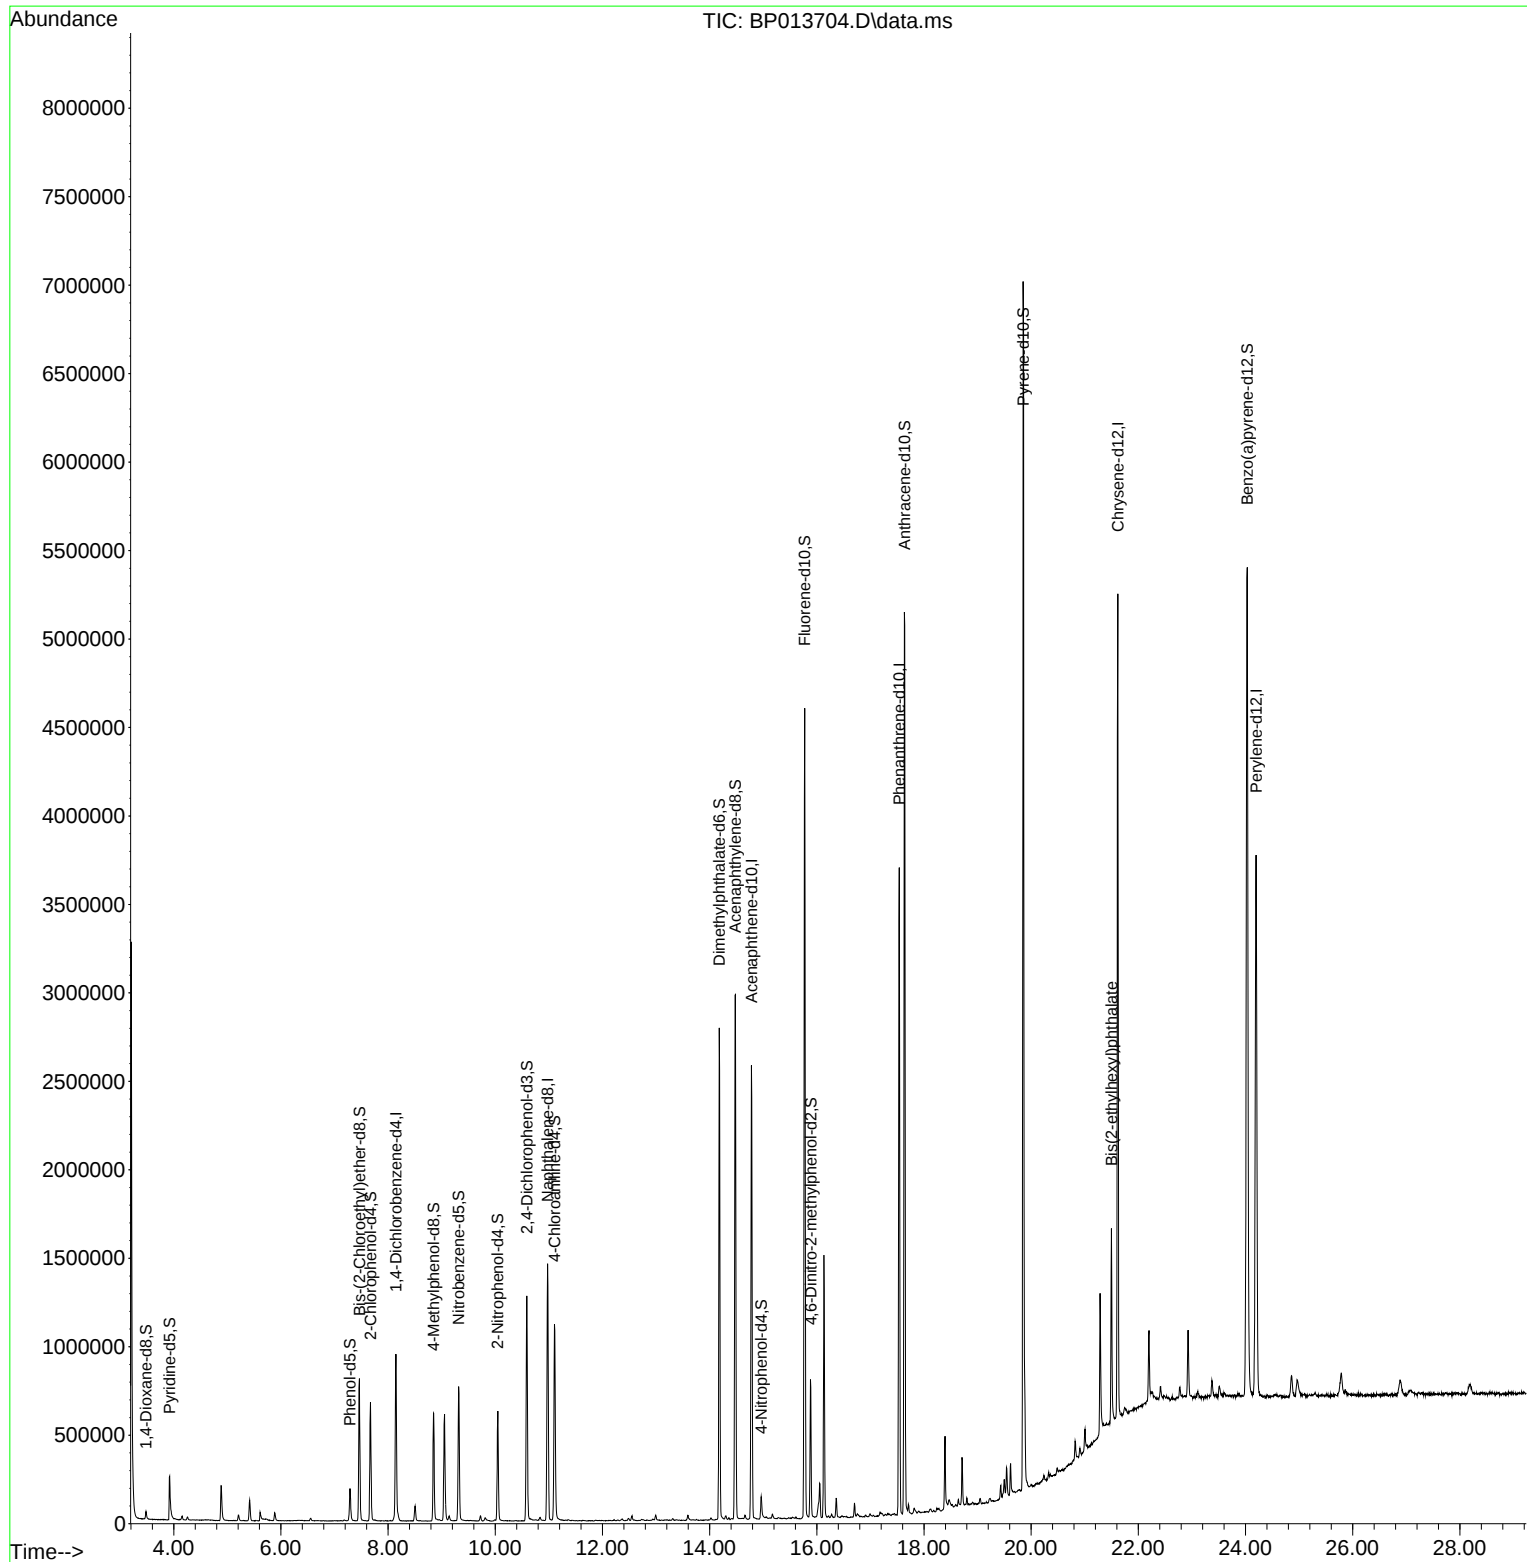

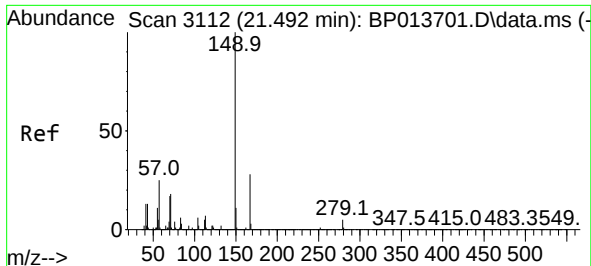

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 5.646 ng/ul
 RT: 21.498 min Scan# 3113
 Delta R.T. 0.012 min
 Lab File: BP013704.D
 Acq: 02 Feb 2023 12:03

Instrument :
 BNA_P
 ClientSampleId :
 A44L2

Tgt Ion:149 Resp: 425938
 Ion Ratio Lower Upper
 149 100
 167 29.0 22.7 34.1
 279 4.9 3.9 5.9

