

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013705.D
 Acq On : 02 Feb 2023 12:37
 Operator : CG/JU
 Sample : 01314-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L3

Quant Time: Feb 02 13:51:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	8.134	152	297247	20.000 ng/u1	0.00
20) Naphthalene-d8	10.963	136	1275783	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.775	164	928807	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.528	188	2332000	20.000 ng/u1	0.00
79) Chrysene-d12	21.604	240	2150574	20.000 ng/u1	0.00
88) Perylene-d12	24.180	264	2027489	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.481	96	29497	4.207 ng/uL	0.00
4) Pyridine-d5	3.911	84	216261	10.750 ng/u1	0.00
7) Phenol-d5	7.281	99	149403	5.719 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	416942	27.212 ng/u1	0.00
11) 2-Chlorophenol-d4	7.658	132	404663	21.131 ng/u1	0.00
15) 4-Methylphenol-d8	8.840	113	298381	14.327 ng/u1	0.00
21) Nitrobenzene-d5	9.311	128	230787	28.357 ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	268284	28.286 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	616065	27.776 ng/u1	0.00
31) 4-Chloroaniline-d4	11.099	131	691321	23.600 ng/u1	0.00
46) Dimethylphthalate-d6	14.175	166	2194422	29.973 ng/u1	0.00
49) Acenaphthylene-d8	14.469	160	2380088	29.423 ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	40989	3.321 ng/u1	0.00
60) Fluorene-d10	15.763	176	2026152	32.107 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	242421	18.550 ng/u1	0.00
73) Anthracene-d10	17.622	188	3354675	30.861 ng/u1	0.00
81) Pyrene-d10	19.845	212	3839621	32.011 ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	3283364	31.723 ng/u1	0.00
Target Compounds					
86) Bis(2-ethylhexyl)phtha...	21.486	149	373092	5.299 ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013705.D
Acq On : 02 Feb 2023 12:37
Operator : CG/JU
Sample : 01314-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L3

Quant Time: Feb 02 13:51:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

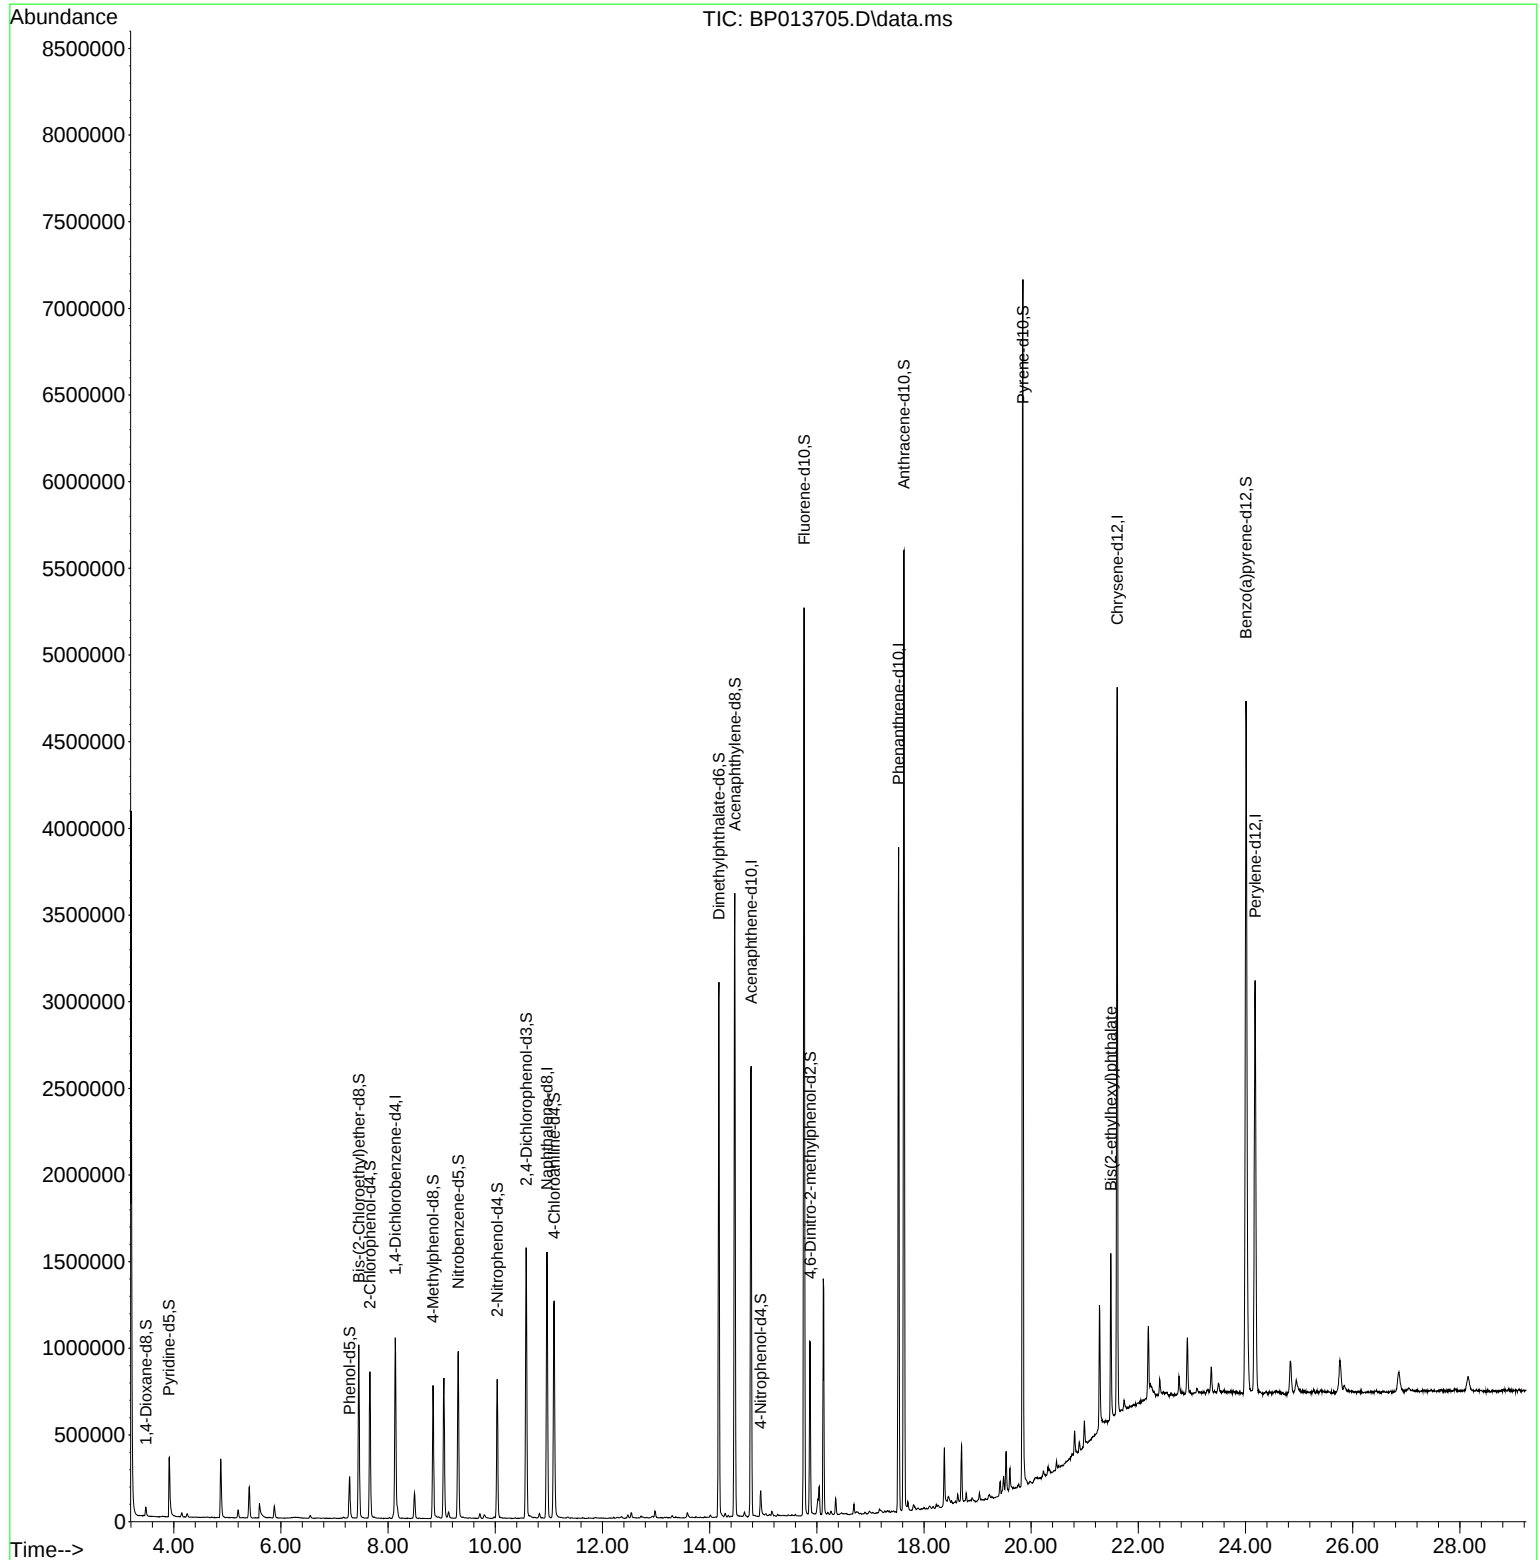

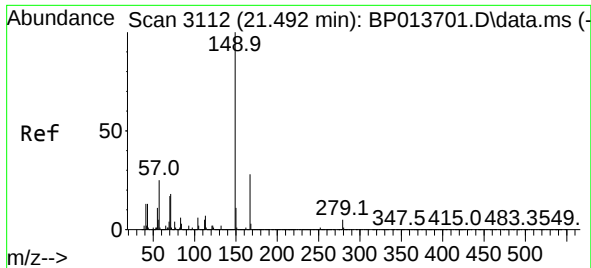

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 5.299 ng/ul
 RT: 21.486 min Scan# 3111
 Delta R.T. 0.000 min
 Lab File: BP013705.D
 Acq: 02 Feb 2023 12:37

Instrument :
 BNA_P
 ClientSampleId :
 A44L3

Tgt Ion:149 Resp: 373092
 Ion Ratio Lower Upper
 149 100
 167 28.9 22.7 34.1
 279 5.0 3.9 5.9

