

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013706.D
 Acq On : 02 Feb 2023 13:11
 Operator : CG/JU
 Sample : 01314-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L4

Quant Time: Feb 02 13:52:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	247164	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1112278	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.774	164	830215	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.527	188	2075701	20.000	ng/u1	0.00
79) Chrysene-d12	21.603	240	2027291	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	2194584	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.475	96	24684	4.234	ng/uL	0.00
4) Pyridine-d5	3.916	84	139135	8.318	ng/u1	0.00
7) Phenol-d5	7.281	99	102939	4.739	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.451	67	317954	24.956	ng/u1	0.00
11) 2-Chlorophenol-d4	7.663	132	288855	18.140	ng/u1	0.00
15) 4-Methylphenol-d8	8.839	113	206923	11.949	ng/u1	0.00
21) Nitrobenzene-d5	9.310	128	169805	23.931	ng/u1	0.00
24) 2-Nitrophenol-d4	10.039	143	194286	23.495	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	425127	21.985	ng/u1	0.00
31) 4-Chloroaniline-d4	11.098	131	534549	20.931	ng/u1	0.00
46) Dimethylphthalate-d6	14.174	166	1791696	27.378	ng/u1	0.00
49) Acenaphthylene-d8	14.469	160	1845292	25.521	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	33334	3.022	ng/u1	0.00
60) Fluorene-d10	15.763	176	1511247	26.791	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.874	200	182576	15.696	ng/u1	0.00
73) Anthracene-d10	17.627	188	2740458	28.324	ng/u1	0.00
81) Pyrene-d10	19.845	212	3409878	30.157	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.009	264	3254055	29.046	ng/u1	0.00
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.486	149	247275	3.726	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013706.D
Acq On : 02 Feb 2023 13:11
Operator : CG/JU
Sample : 01314-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L4

Quant Time: Feb 02 13:52:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

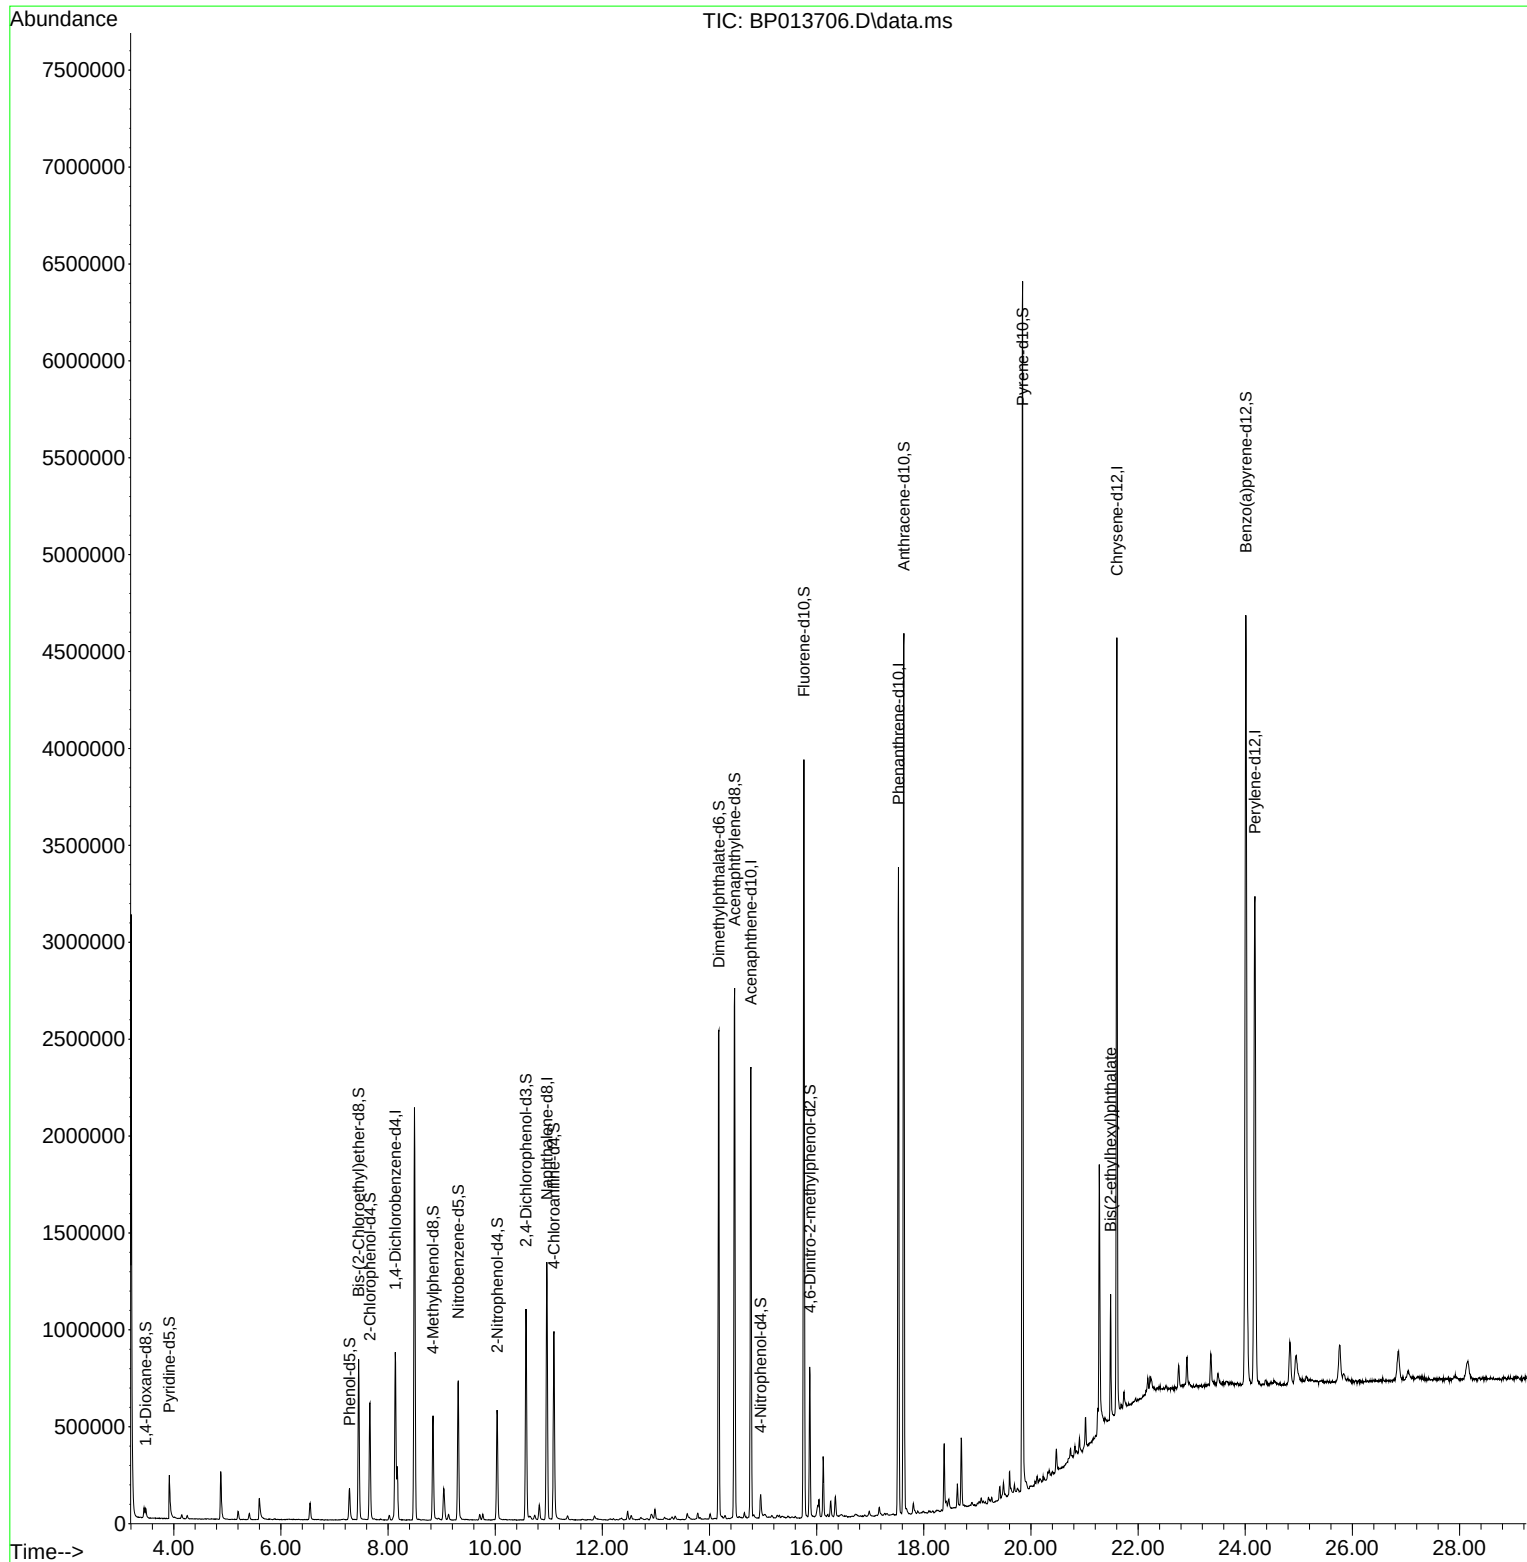

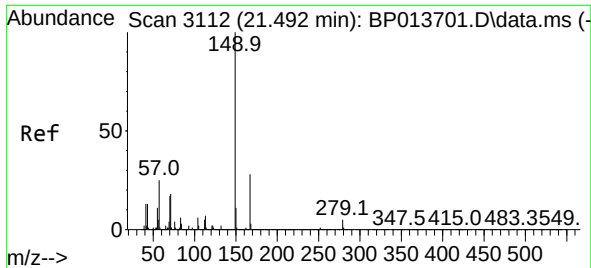

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.726 ng/ul
 RT: 21.486 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BP013706.D
 Acq: 02 Feb 2023 13:11

Instrument :
 BNA_P
 ClientSampleId :
 A44L4

Tgt Ion:149 Resp: 247275
 Ion Ratio Lower Upper
 149 100
 167 28.0 22.7 34.1
 279 4.9 3.9 5.9

