

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020223\  
 Data File : BP013707.D  
 Acq On : 02 Feb 2023 13:45  
 Operator : CG/JU  
 Sample : 01314-02  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A44K9

Quant Time: Feb 02 14:12:53 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP020123.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Feb 02 00:55:26 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| -----                         |        |      |          |        |       |          |
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.134  | 152  | 245816   | 20.000 | ng/u1 | 0.00     |
| 20) Naphthalene-d8            | 10.963 | 136  | 1109656  | 20.000 | ng/u1 | 0.00     |
| 38) Acenaphthene-d10          | 14.769 | 164  | 830037   | 20.000 | ng/u1 | 0.00     |
| 64) Phenanthrene-d10          | 17.528 | 188  | 2073852  | 20.000 | ng/u1 | 0.00     |
| 79) Chrysene-d12              | 21.604 | 240  | 2010375  | 20.000 | ng/u1 | 0.00     |
| 88) Perylene-d12              | 24.180 | 264  | 2140649  | 20.000 | ng/u1 | 0.00     |
|                               |        |      |          |        |       |          |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.475  | 96   | 24553    | 4.235  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.917  | 84   | 143921   | 8.651  | ng/u1 | 0.00     |
| 7) Phenol-d5                  | 7.281  | 99   | 134789   | 6.239  | ng/u1 | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.452  | 67   | 399507   | 31.529 | ng/u1 | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.657  | 132  | 369702   | 23.344 | ng/u1 | 0.00     |
| 15) 4-Methylphenol-d8         | 8.840  | 113  | 272430   | 15.818 | ng/u1 | 0.00     |
| 21) Nitrobenzene-d5           | 9.310  | 128  | 225342   | 31.833 | ng/u1 | 0.00     |
| 24) 2-Nitrophenol-d4          | 10.034 | 143  | 256986   | 31.151 | ng/u1 | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.575 | 165  | 534775   | 27.721 | ng/u1 | 0.00     |
| 31) 4-Chloroaniline-d4        | 11.098 | 131  | 640855   | 25.152 | ng/u1 | 0.00     |
| 46) Dimethylphthalate-d6      | 14.175 | 166  | 2180505  | 33.326 | ng/u1 | 0.00     |
| 49) Acenaphthylene-d8         | 14.463 | 160  | 2275560  | 31.479 | ng/u1 | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.951 | 143  | 42030    | 3.811  | ng/u1 | 0.00     |
| 60) Fluorene-d10              | 15.763 | 176  | 1867764  | 33.119 | ng/u1 | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.869 | 200  | 233174   | 20.064 | ng/u1 | 0.00     |
| 73) Anthracene-d10            | 17.622 | 188  | 3282154  | 33.953 | ng/u1 | 0.00     |
| 81) Pyrene-d10                | 19.839 | 212  | 4030304  | 35.944 | ng/u1 | 0.00     |
| 92) Benzo(a)pyrene-d12        | 24.015 | 264  | 3770968  | 34.508 | ng/u1 | 0.00     |
|                               |        |      |          |        |       |          |
| Target Compounds              |        |      |          |        |       | Qvalue   |
| 86) Bis(2-ethylhexyl)phtha... | 21.486 | 149  | 110313   | 1.676  | ng/u1 | 99       |
| -----                         |        |      |          |        |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020223\  
Data File : BP013707.D  
Acq On : 02 Feb 2023 13:45  
Operator : CG/JU  
Sample : 01314-02  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
A44K9

Quant Time: Feb 02 14:12:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP020123.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Feb 02 00:55:26 2023  
Response via : Initial Calibration

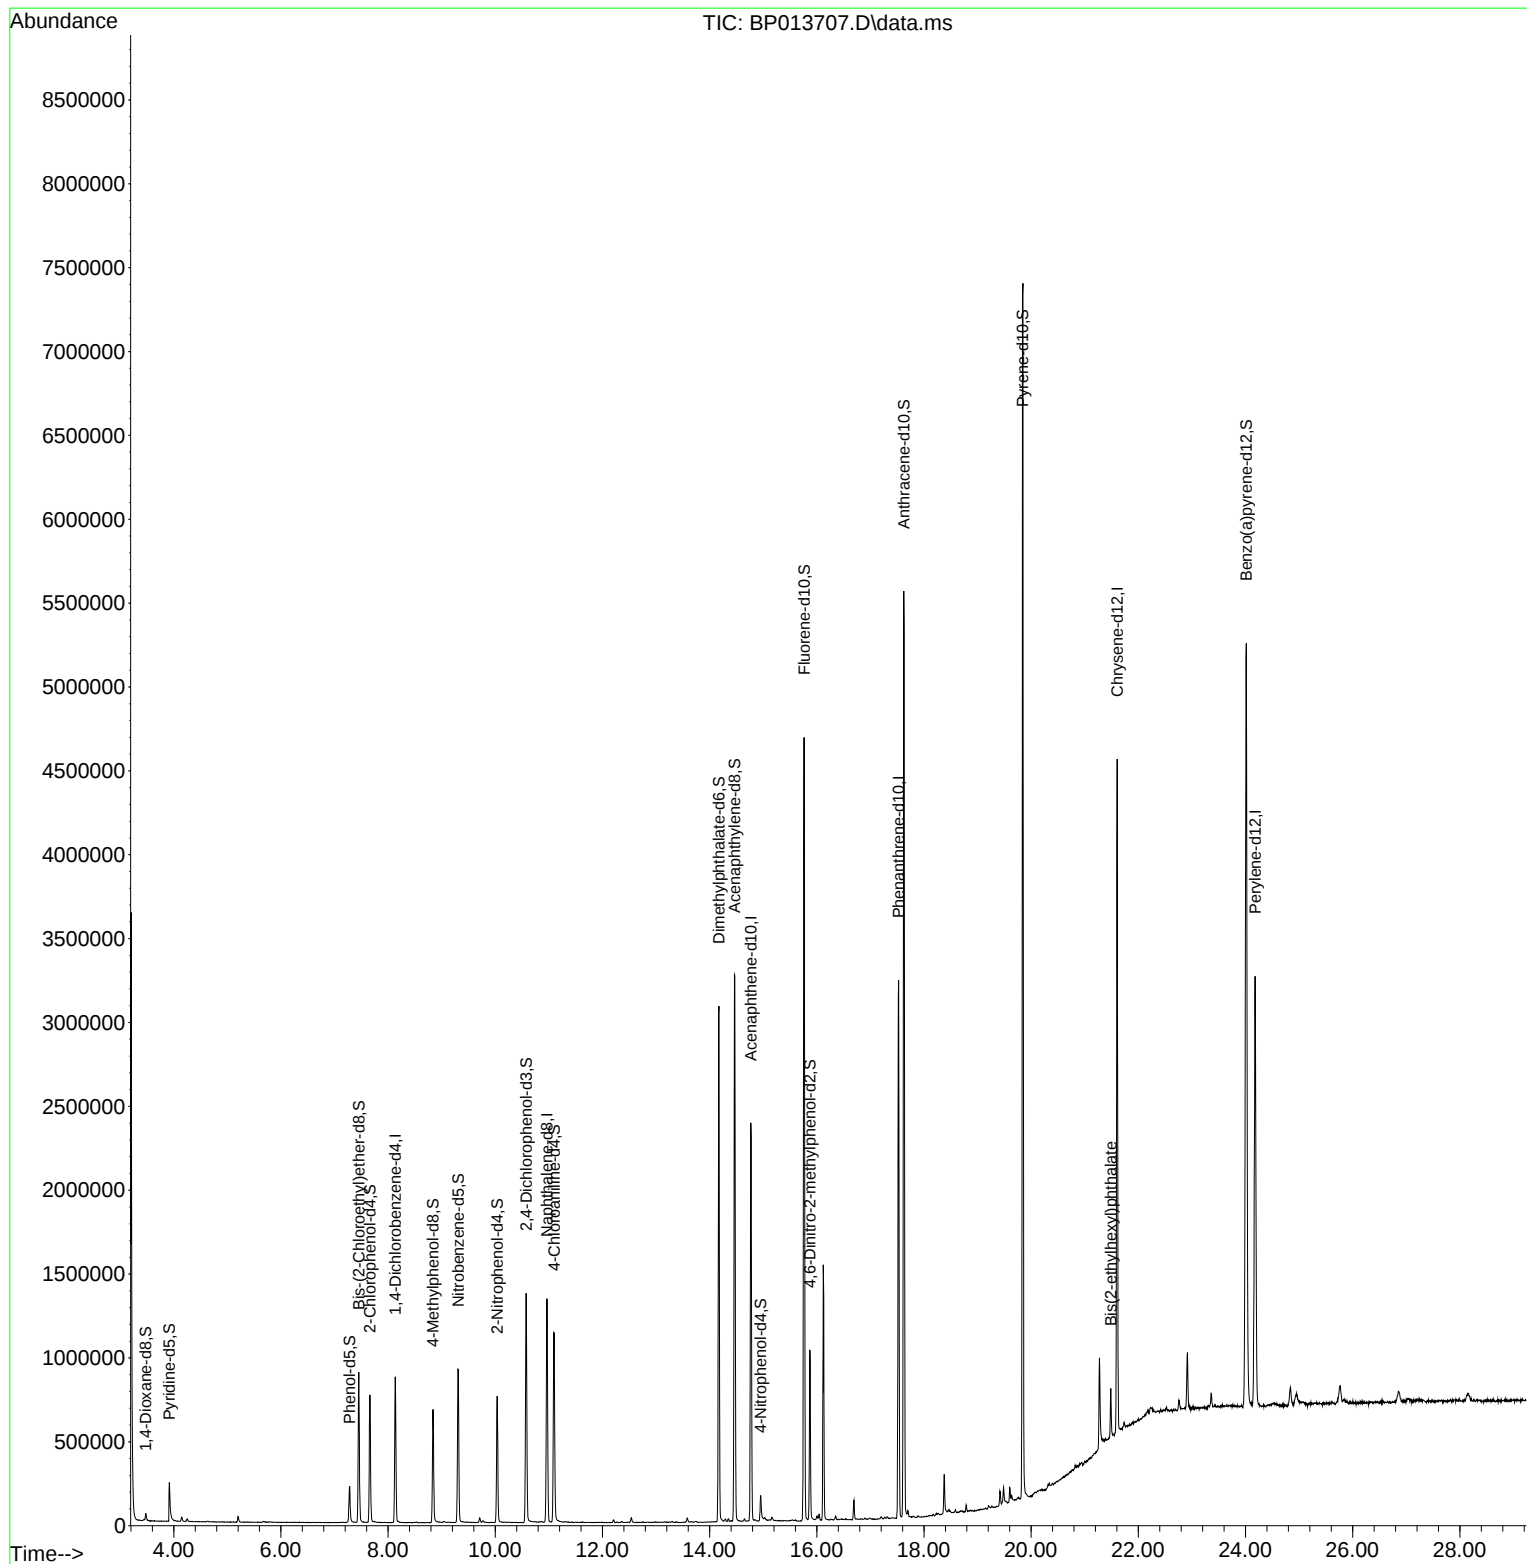

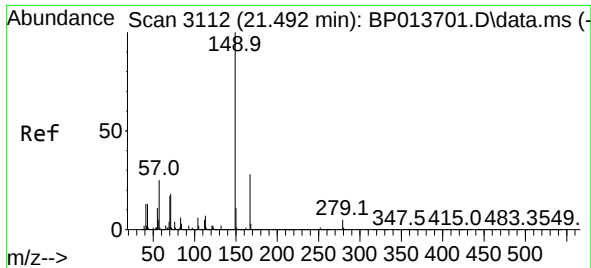

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 1.676 ng/ul  
 RT: 21.486 min Scan# 31  
 Delta R.T. -0.000 min  
 Lab File: BP013707.D  
 Acq: 02 Feb 2023 13:45

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A44K9

Tgt Ion:149 Resp: 110313  
 Ion Ratio Lower Upper  
 149 100  
 167 29.1 22.7 34.1  
 279 4.6 3.9 5.9

