

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013708.D
 Acq On : 02 Feb 2023 14:19
 Operator : CG/JU
 Sample : 01314-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L0

Quant Time: Feb 02 14:48:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	260458	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1182566	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.769	164	883870	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.527	188	2195294	20.000	ng/u1	0.00
79) Chrysene-d12	21.604	240	2083589	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	2150975	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.481	96	28778	4.684	ng/uL	0.00
4) Pyridine-d5	3.916	84	145885	8.276	ng/u1	0.00
7) Phenol-d5	7.281	99	115671	5.053	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.451	67	378856	28.219	ng/u1	0.00
11) 2-Chlorophenol-d4	7.663	132	339419	20.227	ng/u1	0.00
15) 4-Methylphenol-d8	8.839	113	237928	13.038	ng/u1	0.00
21) Nitrobenzene-d5	9.310	128	208978	27.702	ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	243258	27.669	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	492151	23.938	ng/u1	0.00
31) 4-Chloroaniline-d4	11.098	131	614857	22.644	ng/u1	0.00
46) Dimethylphthalate-d6	14.174	166	2071580	29.733	ng/u1	0.00
49) Acenaphthylene-d8	14.469	160	2185096	28.386	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	38279	3.260	ng/u1	0.00
60) Fluorene-d10	15.763	176	1810636	30.150	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.874	200	255001	20.728	ng/u1	0.00
73) Anthracene-d10	17.627	188	3399792	33.224	ng/u1	0.00
81) Pyrene-d10	19.845	212	4220011	36.314	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.009	264	3820172	34.791	ng/u1	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.351	77	62436	3.064	ng/u1	97
86) Bis(2-ethylhexyl)phtha...	21.486	149	92150	1.351	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013708.D
Acq On : 02 Feb 2023 14:19
Operator : CG/JU
Sample : 01314-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L0

Quant Time: Feb 02 14:48:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration




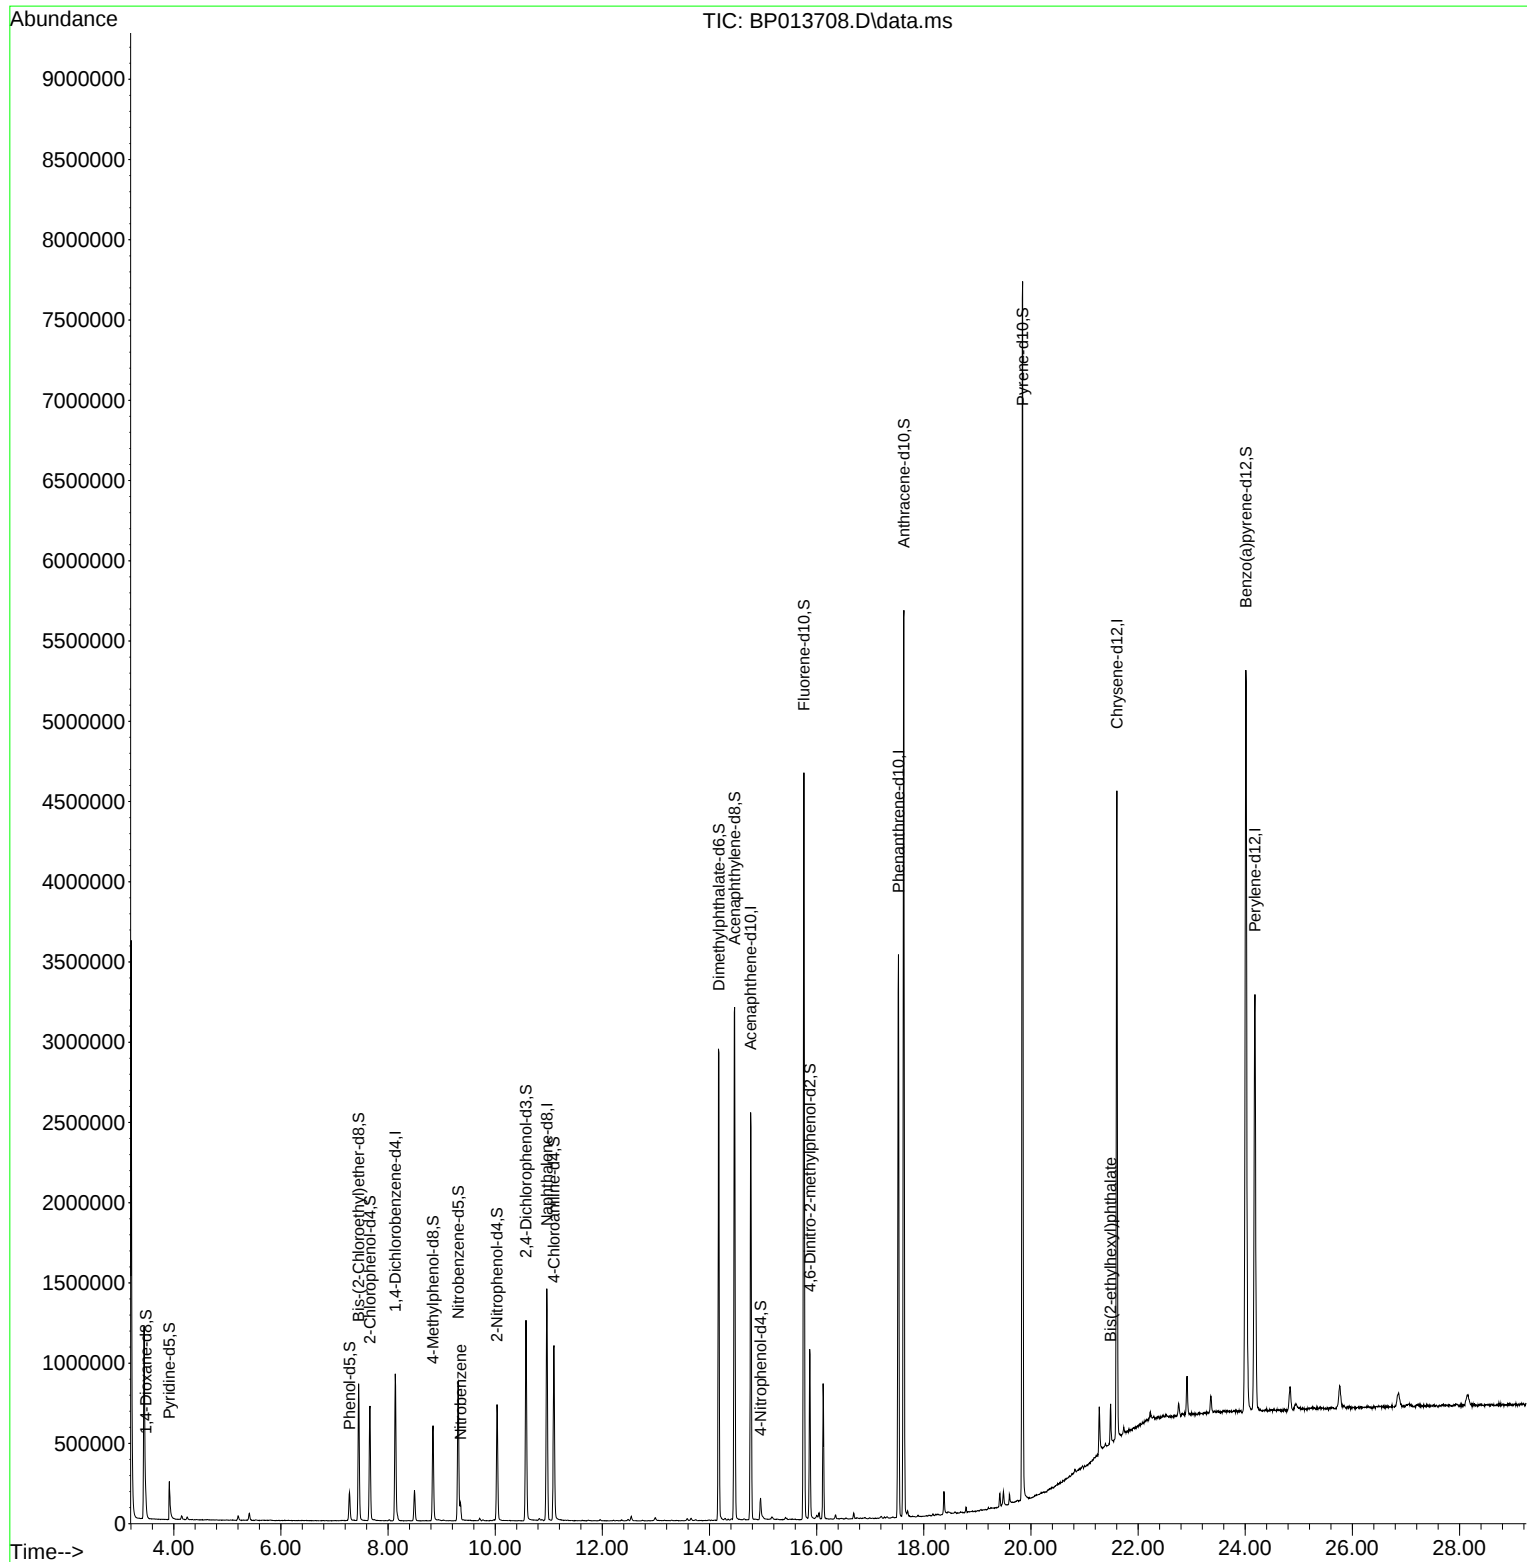


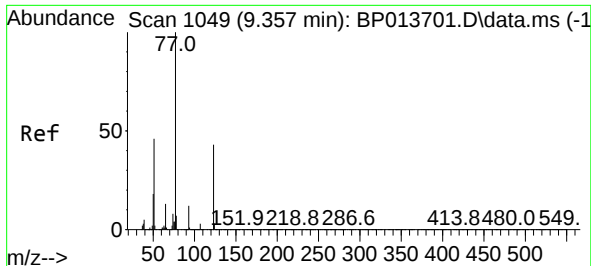

#22
Nitrobenzene
Concen: 3.064 ng/ul
RT: 9.351 min Scan# 1048
Delta R.T. -0.000 min
Lab File: BP013708.D
Acq: 02 Feb 2023 14:19

Instrument :
BNA_P
ClientSampleId :
A44L0

Tgt Ion:	77	Resp:	62436
Ion	Ratio	Lower	Upper
77	100		
123	44.9	34.1	51.1
65	13.1	9.8	14.8

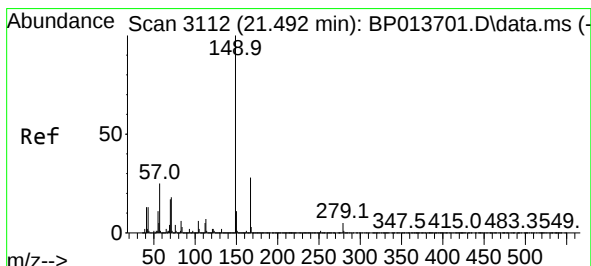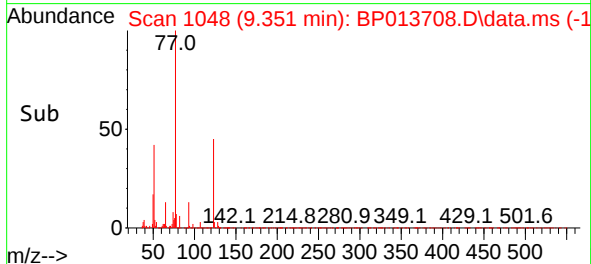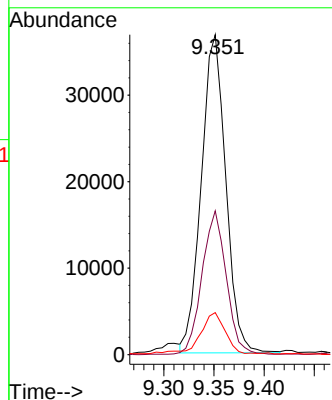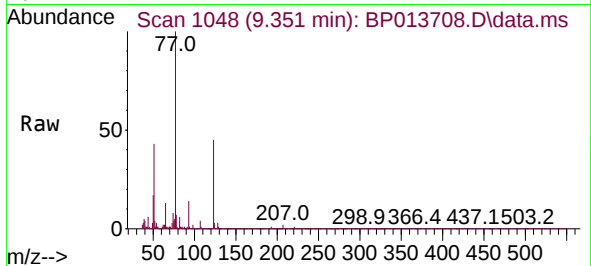

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.351 ng/ul
RT: 21.486 min Scan# 3111
Delta R.T. -0.000 min
Lab File: BP013708.D
Acq: 02 Feb 2023 14:19

Tgt Ion:	149	Resp:	92150
Ion	Ratio	Lower	Upper
149	100		
167	28.2	22.7	34.1
279	4.7	3.9	5.9

