

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013724.D
 Acq On : 02 Feb 2023 23:29
 Operator : CG/JU
 Sample : 01314-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L1

Quant Time: Feb 03 00:30:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	255893	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1151587	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.769	164	872716	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.522	188	2158543	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	2231977	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	2349724	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.476	96	24328	4.031	ng/uL	0.00
4) Pyridine-d5	3.917	84	139558	8.059	ng/u1	0.00
7) Phenol-d5	7.275	99	122762	5.459	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	425156	32.232	ng/u1	0.00
11) 2-Chlorophenol-d4	7.658	132	378395	22.952	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	254458	14.193	ng/u1	-0.01
21) Nitrobenzene-d5	9.305	128	246194	33.513	ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	269562	31.486	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	558975	27.920	ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	711409	26.905	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	2276777	33.096	ng/u1	0.00
49) Acenaphthylene-d8	14.463	160	2452136	32.262	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	35482	3.060	ng/u1	0.00
60) Fluorene-d10	15.757	176	2088772	35.226	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	287081	23.733	ng/u1	0.00
73) Anthracene-d10	17.622	188	3657197	36.348	ng/u1	0.00
81) Pyrene-d10	19.839	212	4593558	36.900	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	4579813	38.181	ng/u1	0.00
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.480	149	79343	1.086	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013724.D
Acq On : 02 Feb 2023 23:29
Operator : CG/JU
Sample : 01314-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L1

Quant Time: Feb 03 00:30:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

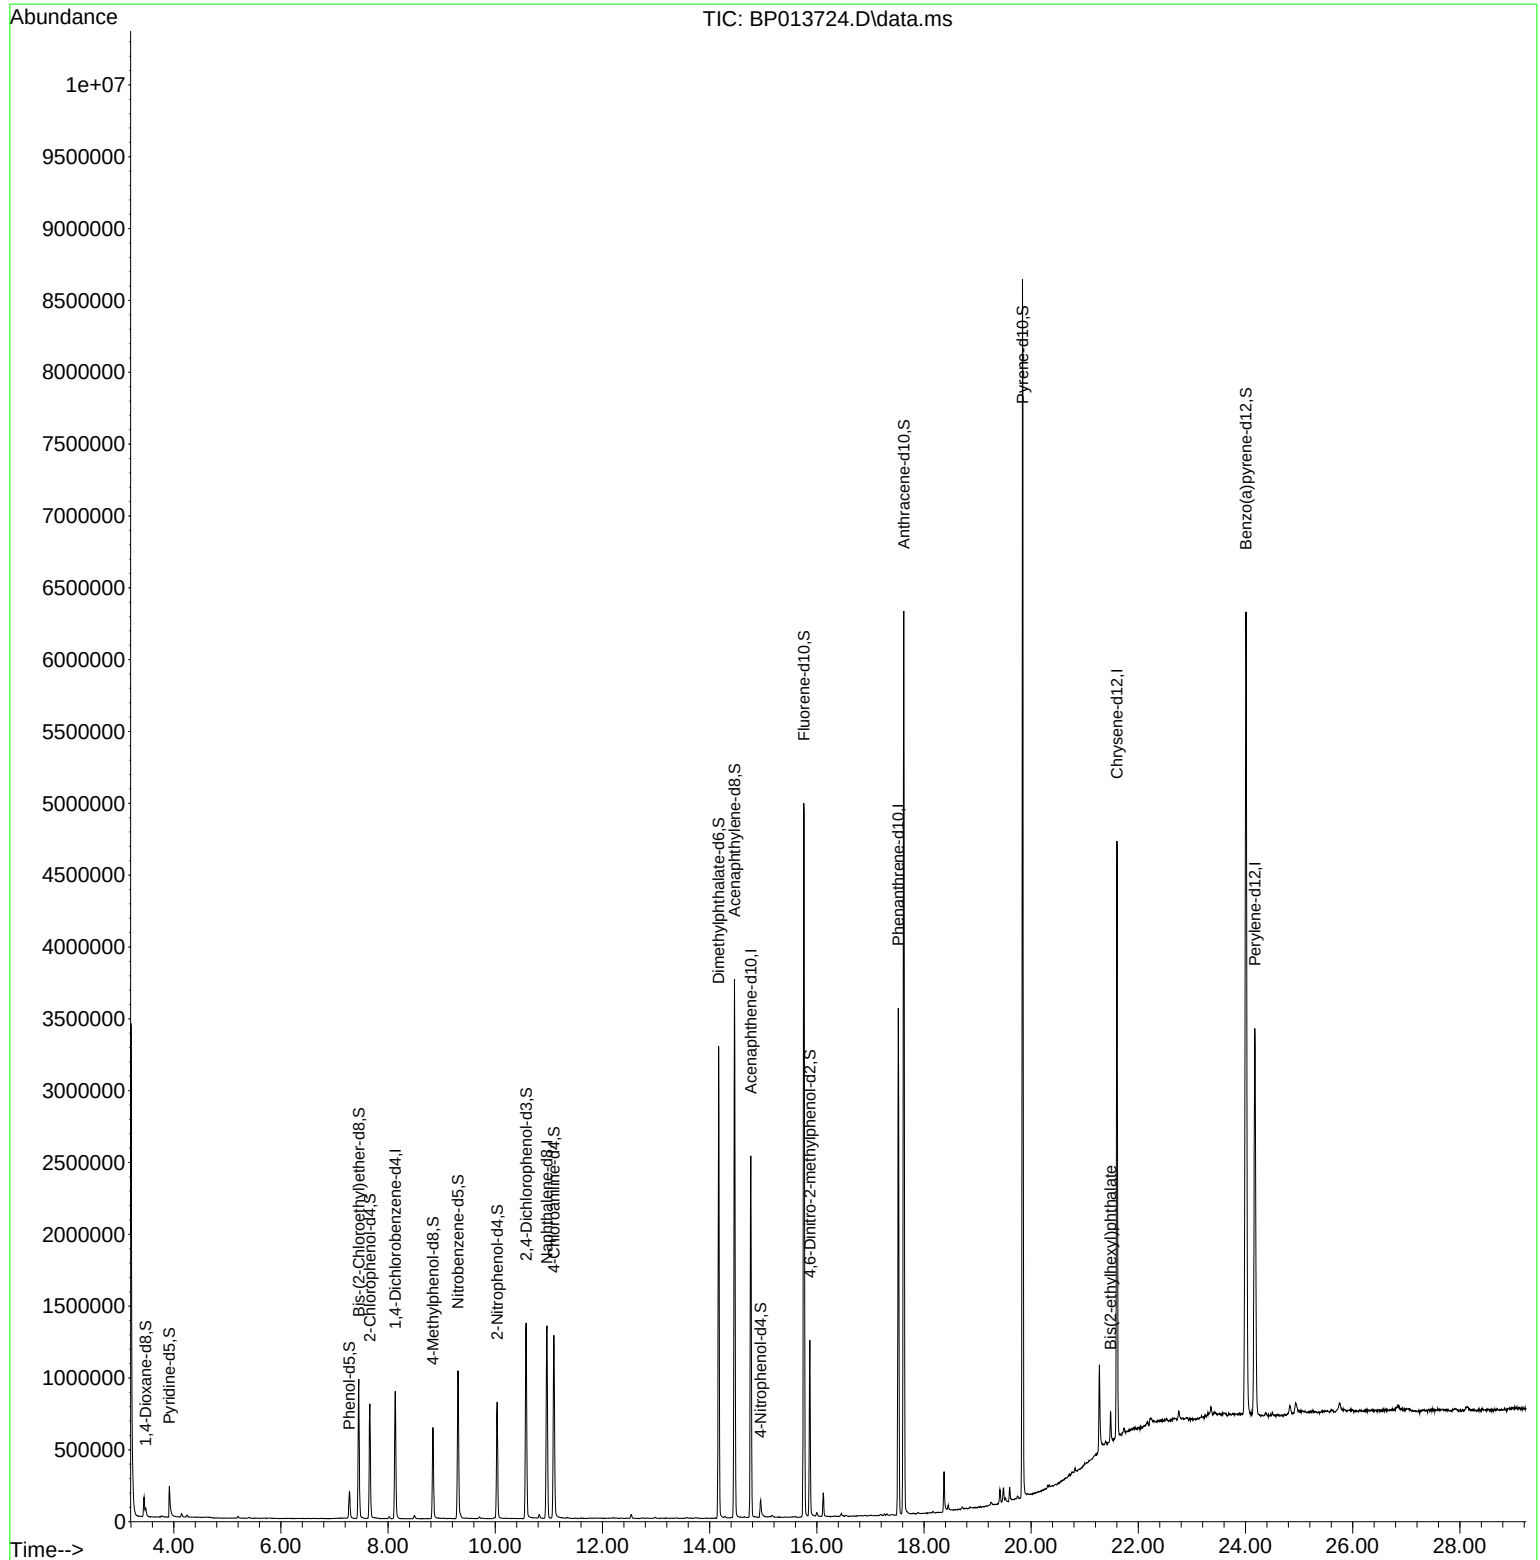

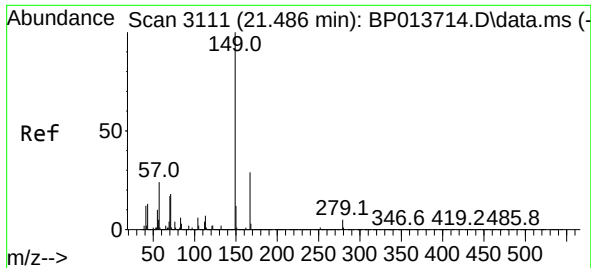

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.086 ng/ul
 RT: 21.480 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BP013724.D
 Acq: 02 Feb 2023 23:29

Instrument :
 BNA_P
 ClientSampleId :
 A44L1

Tgt Ion:	149	Resp:	79343
Ion	Ratio	Lower	Upper
149	100		
167	30.2	22.7	34.1
279	5.3	3.9	5.9

