

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013725.D
 Acq On : 03 Feb 2023 00:03
 Operator : CG/JU
 Sample : 01314-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44P0

Quant Time: Feb 03 00:30:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	277754	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1225347	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.769	164	924336	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.522	188	2282544	20.000	ng/u1	0.00
79) Chrysene-d12	21.604	240	2337451	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	2497733	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.475	96	30769	4.697	ng/uL	0.00
4) Pyridine-d5	3.916	84	149402	7.948	ng/u1	0.00
7) Phenol-d5	7.275	99	164252	6.728	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	473092	33.043	ng/u1	0.00
11) 2-Chlorophenol-d4	7.657	132	450193	25.158	ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	322926	16.594	ng/u1	-0.01
21) Nitrobenzene-d5	9.304	128	276722	35.401	ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	319050	35.023	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	630875	29.615	ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	698216	24.816	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	2497889	34.282	ng/u1	0.00
49) Acenaphthylene-d8	14.463	160	2720519	33.795	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	47182	3.842	ng/u1	0.00
60) Fluorene-d10	15.763	176	2272713	36.188	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	323518	25.292	ng/u1	0.00
73) Anthracene-d10	17.622	188	3899331	36.649	ng/u1	0.00
81) Pyrene-d10	19.839	212	4954222	38.002	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	4790455	37.570	ng/u1	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.351	77	570646	27.029	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013725.D
Acq On : 03 Feb 2023 00:03
Operator : CG/JU
Sample : 01314-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44P0

Quant Time: Feb 03 00:30:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

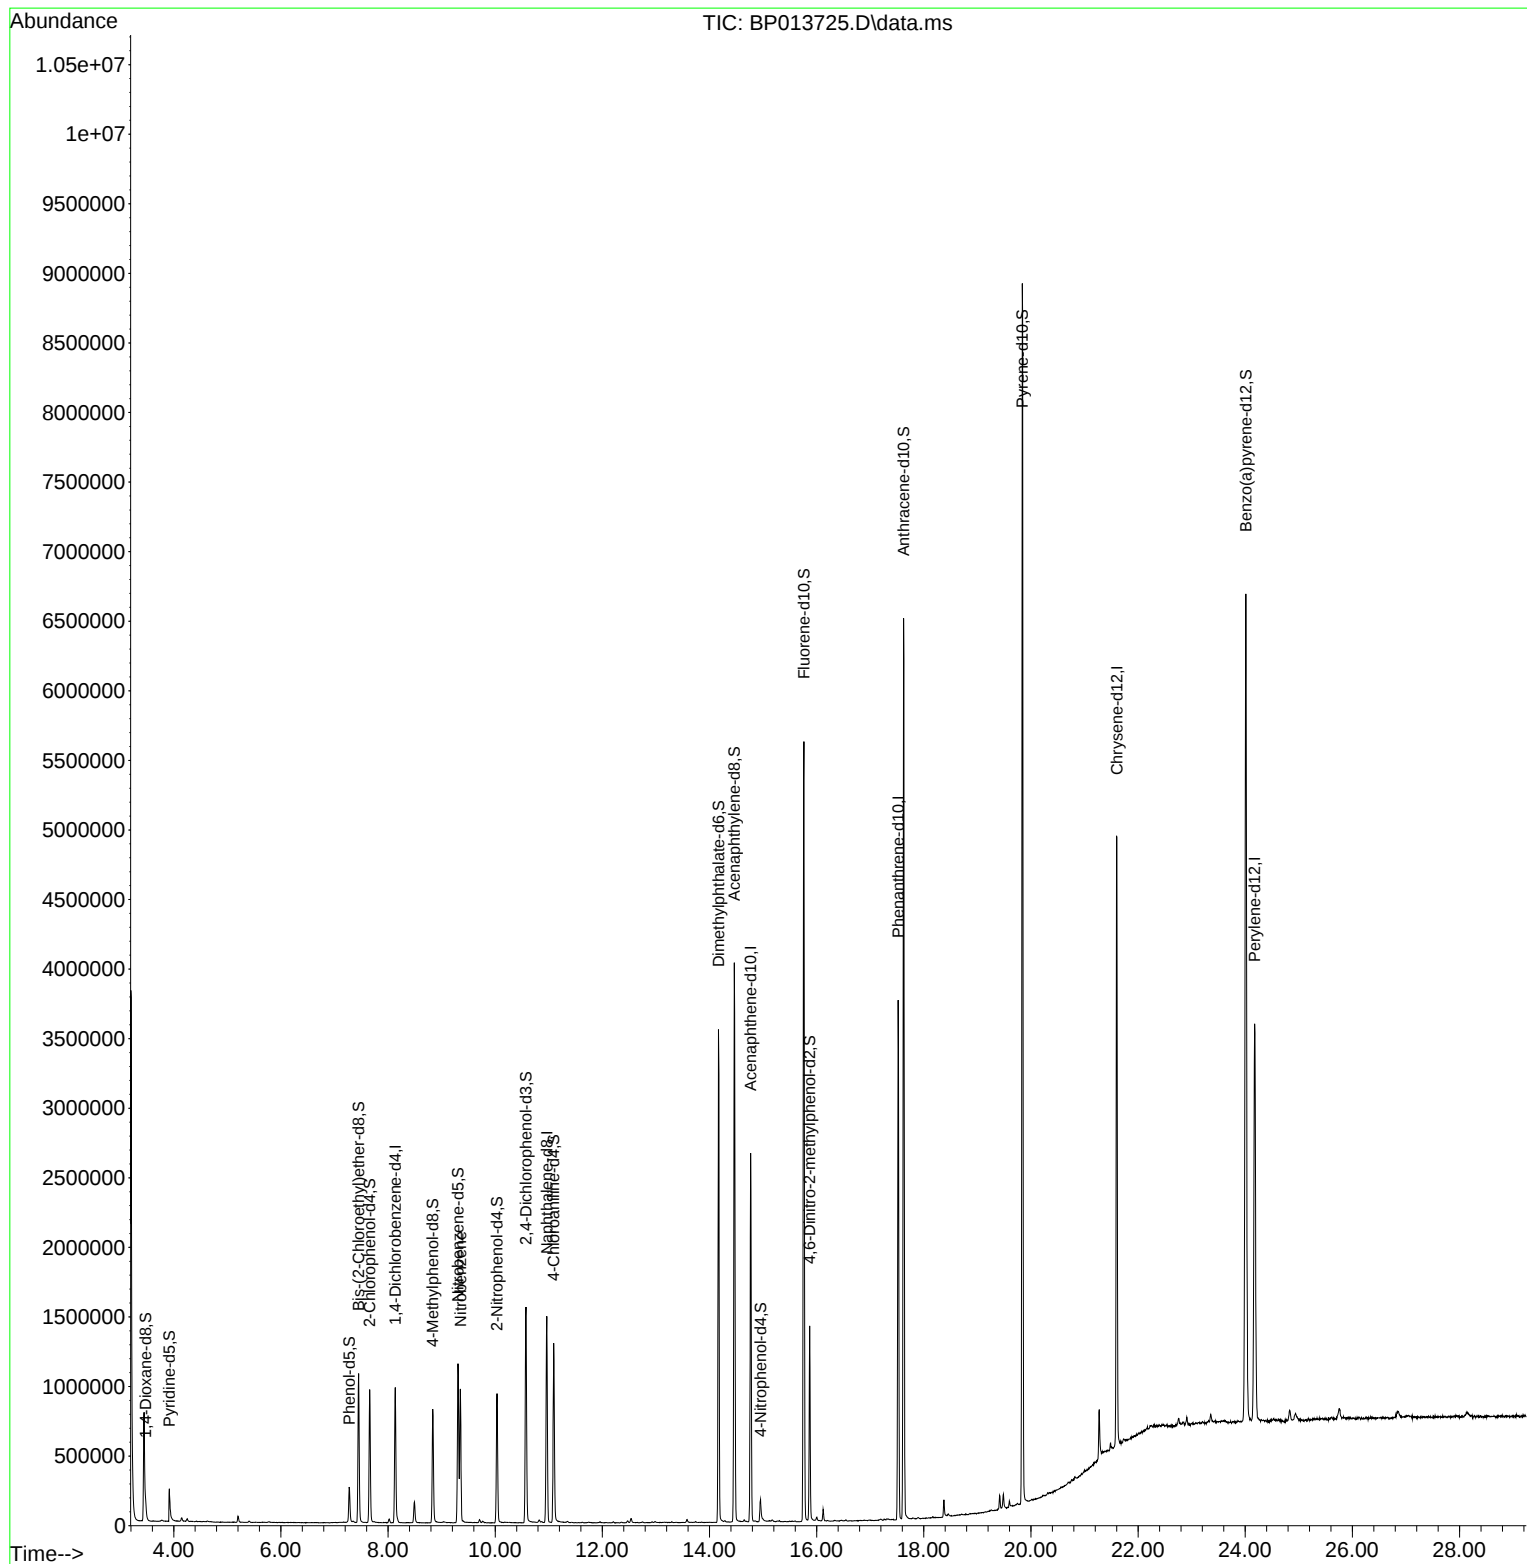

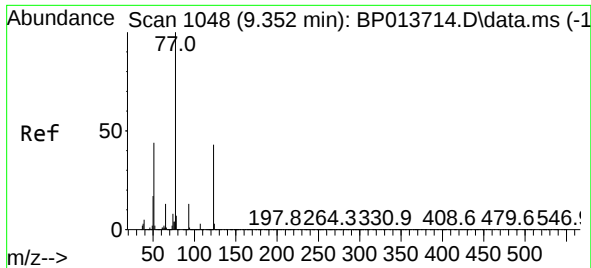

#22
 Nitrobenzene
 Concen: 27.029 ng/ul
 RT: 9.351 min Scan# 1048
 Delta R.T. -0.000 min
 Lab File: BP013725.D
 Acq: 03 Feb 2023 00:03

Instrument :
 BNA_P
 ClientSampleId :
 A44P0

Tgt Ion:	77	Resp:	570646
Ion	Ratio	Lower	Upper
77	100		
123	43.7	34.1	51.1
65	12.5	9.8	14.8

