

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013733.D
 Acq On : 03 Feb 2023 10:05
 Operator : CG/JU
 Sample : 01316-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44H2

Quant Time: Feb 03 10:30:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 00:55:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	8.134	152	222544	20.000 ng/u1	0.00
20) Naphthalene-d8	10.963	136	1002434	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.769	164	775796	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.522	188	1992893	20.000 ng/u1	0.00
79) Chrysene-d12	21.604	240	2169546	20.000 ng/u1	0.00
88) Perylene-d12	24.180	264	2365235	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.475	96	29972	5.710 ng/uL	0.00
4) Pyridine-d5	3.911	84	467120	31.016 ng/u1	0.00
7) Phenol-d5	7.275	99	606411	31.004 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	374010	32.604 ng/u1	-0.01
11) 2-Chlorophenol-d4	7.658	132	453413	31.624 ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	490846	31.480 ng/u1	-0.01
21) Nitrobenzene-d5	9.305	128	201078	31.444 ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	249547	33.485 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	523858	30.059 ng/u1	-0.01
31) 4-Chloroaniline-d4	11.093	131	747777	32.488 ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	1978872	32.359 ng/u1	0.00
49) Acenaphthylene-d8	14.463	160	2079515	30.778 ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	246649	23.929 ng/u1	0.00
60) Fluorene-d10	15.757	176	1827614	34.673 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	245812	22.010 ng/u1	0.00
73) Anthracene-d10	17.622	188	3223516	34.701 ng/u1	0.00
81) Pyrene-d10	19.839	212	4170446	34.465 ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	4262342	35.301 ng/u1	0.00
Target Compounds					
2) 1,4-Dioxane	3.511	88	36110	6.601 ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013733.D
Acq On : 03 Feb 2023 10:05
Operator : CG/JU
Sample : 01316-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44H2


Quant Time: Feb 03 10:30:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 00:55:26 2023
Response via : Initial Calibration

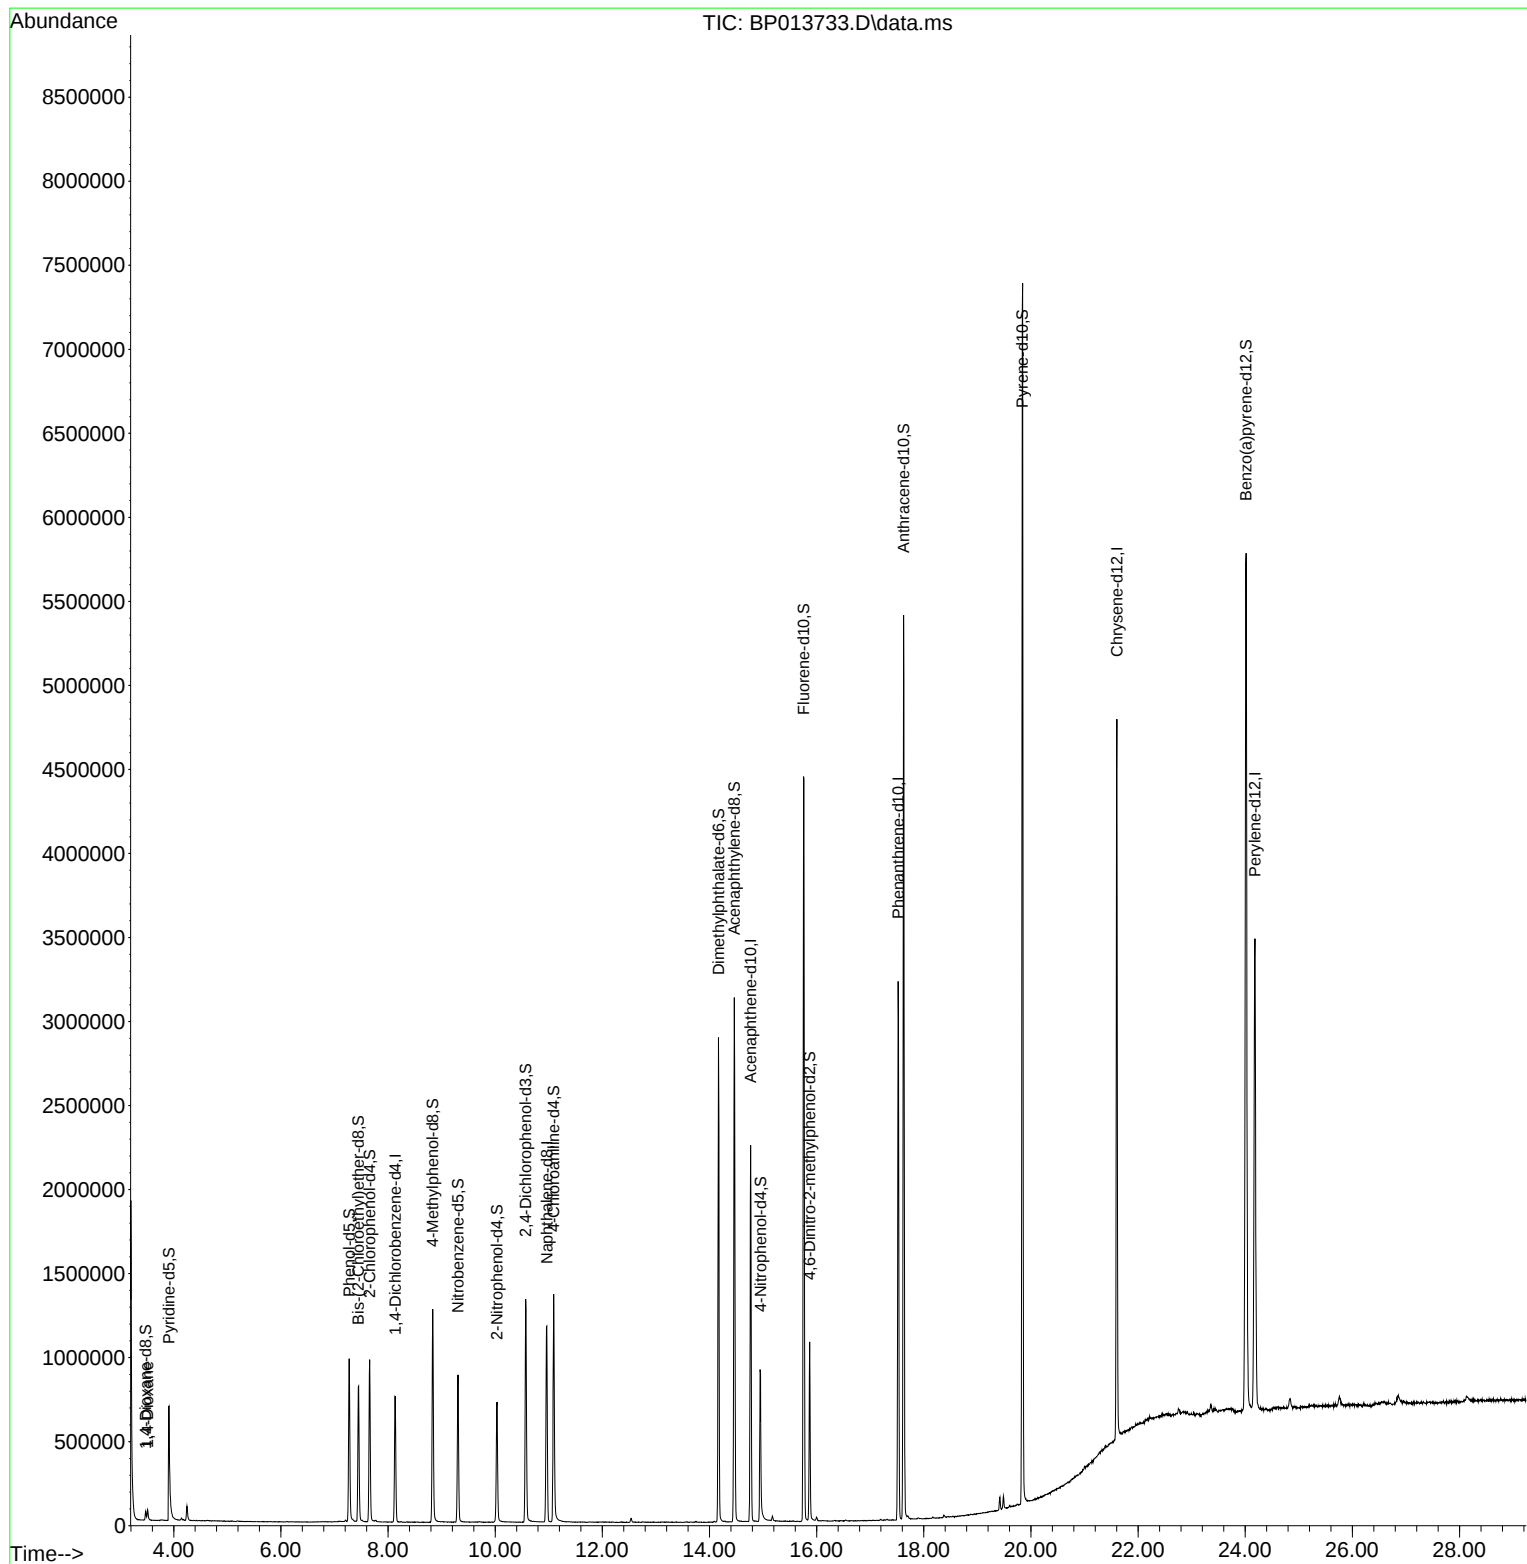

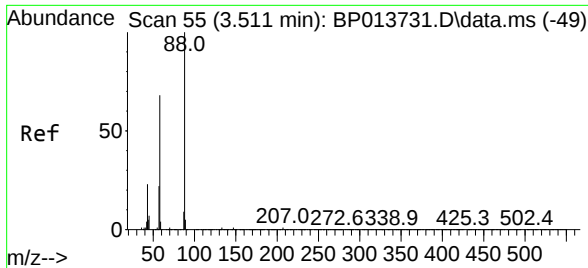

#2
 1,4-Dioxane
 Concen: 6.601 ng/uL
 RT: 3.511 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: BP013733.D
 Acq: 03 Feb 2023 10:05

Instrument :
 BNA_P
 ClientSampleId :
 A44H2

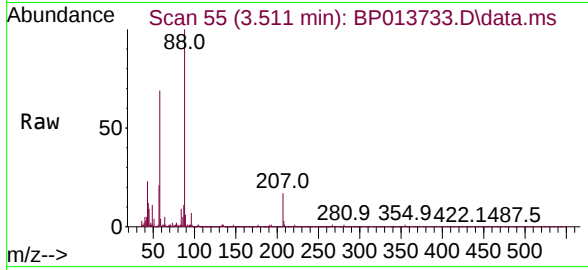

Tgt Ion:	88	Resp:	36110
Ion	Ratio	Lower	Upper
88	100		
43	23.3	22.2	33.4
58	68.5	54.9	82.3

