

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013753.D
 Acq On : 03 Feb 2023 22:21
 Operator : CG/JU
 Sample : 01381-17
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q5

Quant Time: Feb 03 23:54:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	8.134	152	285950	20.000 ng/u1	0.00
20) Naphthalene-d8	10.957	136	1230797	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.769	164	929141	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.522	188	2392753	20.000 ng/u1	0.00
79) Chrysene-d12	21.598	240	2726356	20.000 ng/u1	0.00
88) Perylene-d12	24.168	264	3018659	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.475	96	39937	5.921 ng/uL	0.00
4) Pyridine-d5	3.916	84	126260	6.524 ng/u1	0.00
7) Phenol-d5	7.275	99	118874	4.730 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	443318	30.076 ng/u1	0.00
11) 2-Chlorophenol-d4	7.657	132	397910	21.599 ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	243365	12.147 ng/u1	0.00
21) Nitrobenzene-d5	9.304	128	256510	32.670 ng/u1	0.00
24) 2-Nitrophenol-d4	10.028	143	306459	33.492 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	581654	27.183 ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	626911	22.183 ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	2378699	32.478 ng/u1	0.00
49) Acenaphthylene-d8	14.463	160	2520787	31.152 ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	42932	3.478 ng/u1	0.00
60) Fluorene-d10	15.757	176	2134930	33.818 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	325985	24.311 ng/u1	0.00
73) Anthracene-d10	17.616	188	3829511	34.335 ng/u1	0.00
81) Pyrene-d10	19.839	212	5105128	33.573 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.998	264	5414960	35.139 ng/u1	0.00
Target Compounds					
				Qvalue	
22) Nitrobenzene	9.346	77	1486780	70.109 ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013753.D
Acq On : 03 Feb 2023 22:21
Operator : CG/JU
Sample : 01381-17
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q5

Quant Time: Feb 03 23:54:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 03 23:44:43 2023
Response via : Initial Calibration

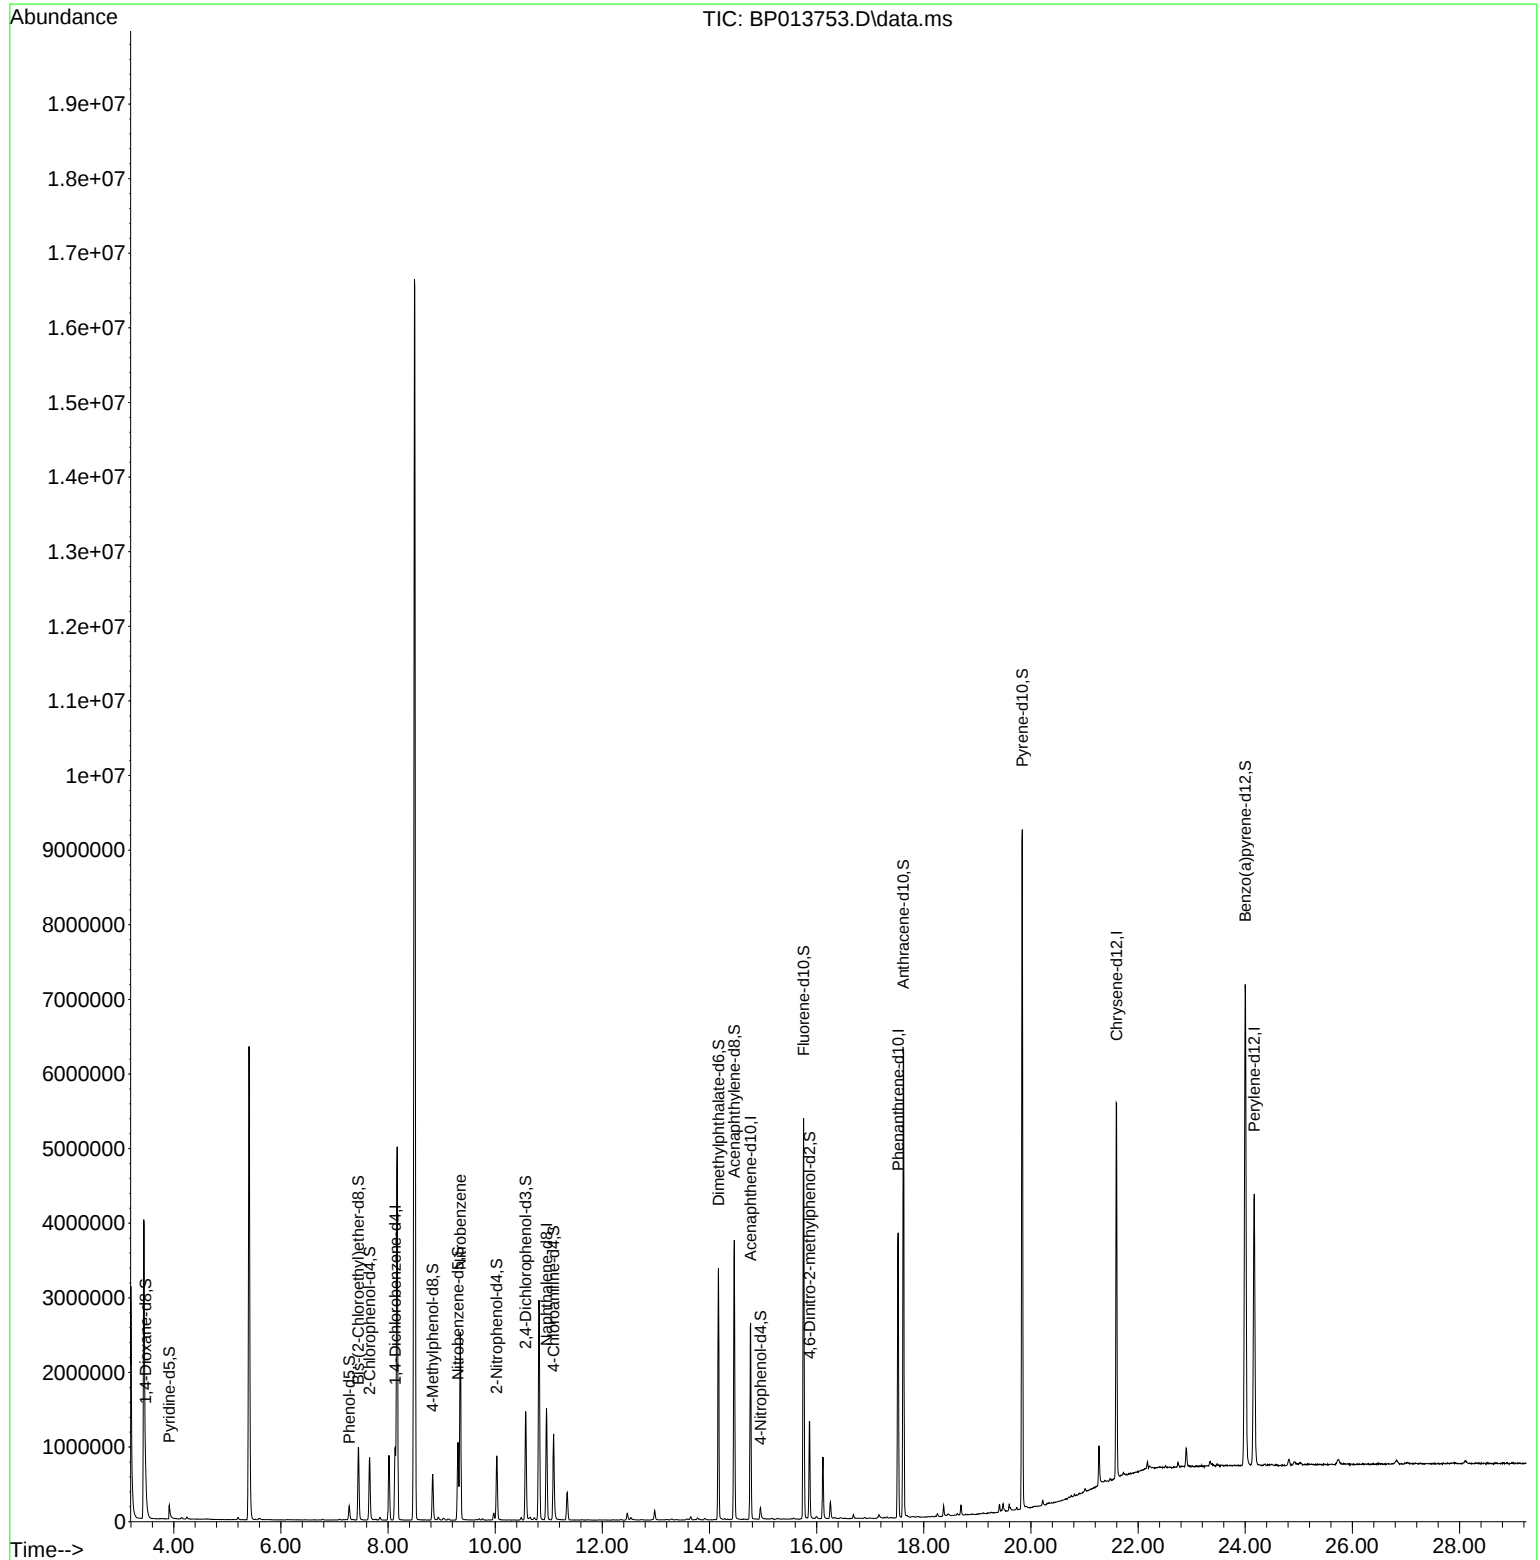

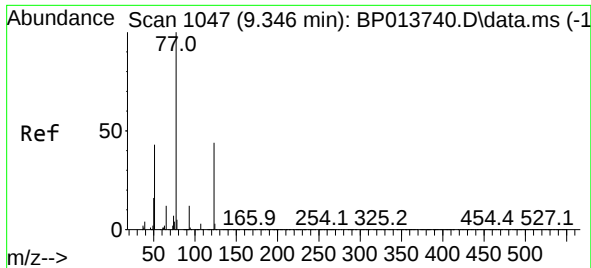

#22
 Nitrobenzene
 Concen: 70.109 ng/ul
 RT: 9.346 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: BP013753.D
 Acq: 03 Feb 2023 22:21

Instrument :
 BNA_P
 ClientSampleId :
 A44Q5

Tgt Ion: 77 Resp: 1486780

Ion	Ratio	Lower	Upper
77	100		
123	43.7	34.1	51.1
65	12.4	9.8	14.8

