

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013761.D
 Acq On : 04 Feb 2023 03:26
 Operator : CG/JU
 Sample : 01381-05
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M9

Quant Time: Feb 04 03:51:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	8.128	152	266958	20.000 ng/u1	0.00
20) Naphthalene-d8	10.957	136	1132515	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.763	164	817405	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.516	188	2000713	20.000 ng/u1	0.00
79) Chrysene-d12	21.592	240	2146656	20.000 ng/u1	0.00
88) Perylene-d12	24.162	264	2187784	20.000 ng/u1	-0.01
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.475	96	30980	4.920 ng/uL	0.00
4) Pyridine-d5	3.911	84	142545	7.890 ng/u1	0.00
7) Phenol-d5	7.275	99	128760	5.488 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	438537	31.869 ng/u1	0.00
11) 2-Chlorophenol-d4	7.657	132	393804	22.897 ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	262361	14.027 ng/u1	0.00
21) Nitrobenzene-d5	9.304	128	253621	35.105 ng/u1	0.00
24) 2-Nitrophenol-d4	10.028	143	278246	33.048 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	596768	30.310 ng/u1	0.00
31) 4-Chloroaniline-d4	11.087	131	603821	23.220 ng/u1	0.00
46) Dimethylphthalate-d6	14.163	166	2262592	35.115 ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	2449499	34.408 ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	39216	3.611 ng/u1	0.01
60) Fluorene-d10	15.757	176	2061828	37.125 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	278068	24.801 ng/u1	0.00
73) Anthracene-d10	17.616	188	3518394	37.727 ng/u1	0.00
81) Pyrene-d10	19.833	212	4535344	37.881 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.998	264	4368580	39.116 ng/u1	0.00
Target Compounds					
				Qvalue	
12) 2-Chlorophenol	7.687	128	77319	4.437 ng/u1	96
32) 4-Chloroaniline	11.110	127	36883	1.409 ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013761.D
Acq On : 04 Feb 2023 03:26
Operator : CG/JU
Sample : 01381-05
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M9

Quant Time: Feb 04 03:51:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 03 23:44:43 2023
Response via : Initial Calibration




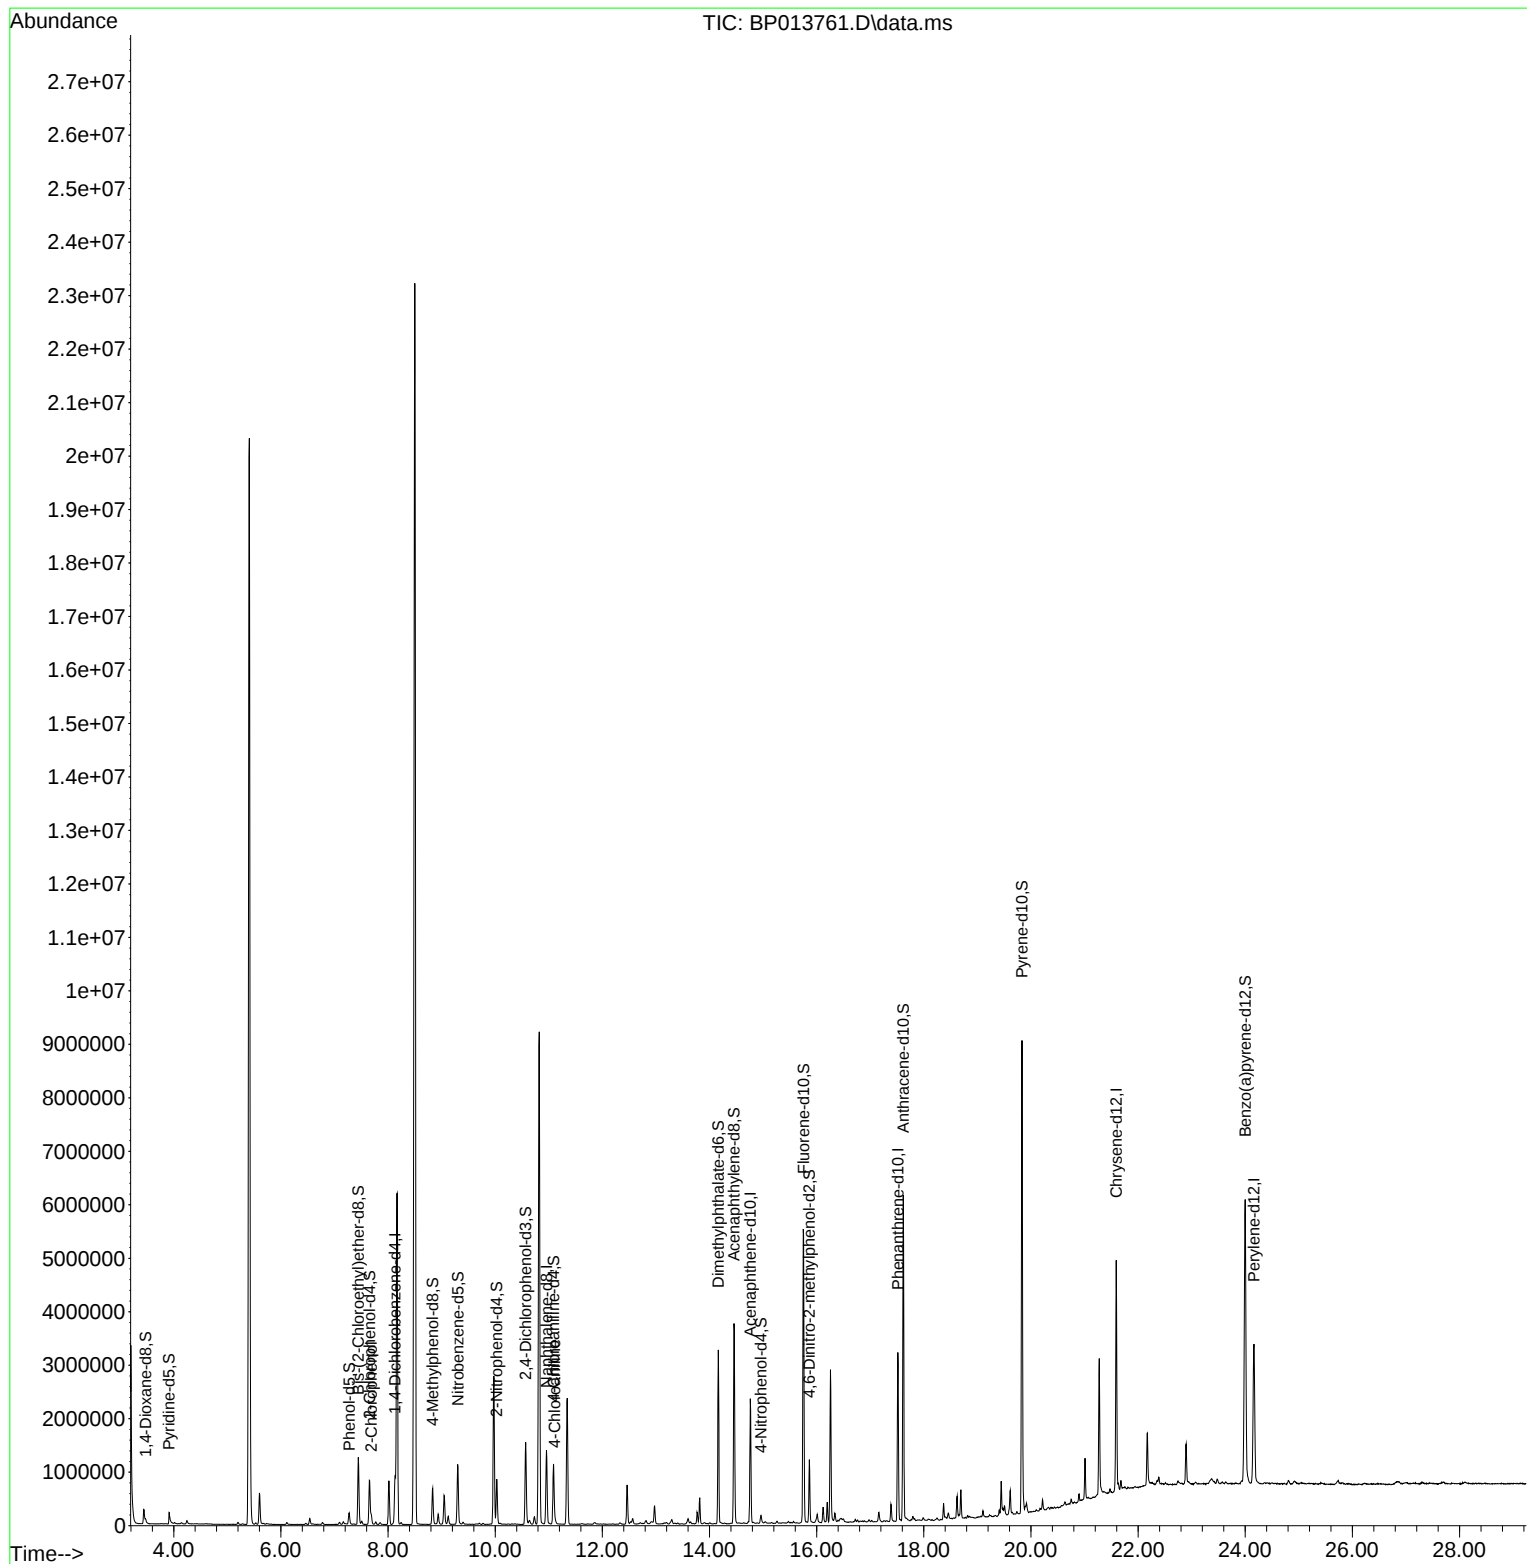


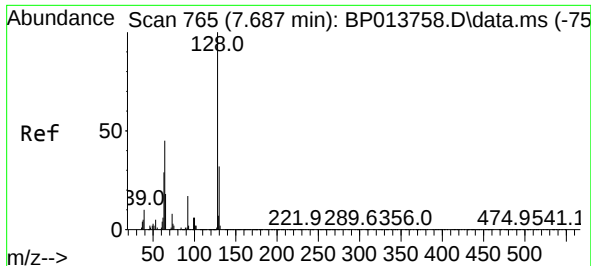

#12
2-Chlorophenol
Concen: 4.437 ng/ul
RT: 7.687 min Scan# 765
Delta R.T. -0.000 min
Lab File: BP013761.D
Acq: 04 Feb 2023 03:26

Instrument :
BNA_P
ClientSampleId :
A44M9

Tgt Ion:128 Resp: 77319
Ion Ratio Lower Upper
128 100
64 50.5 37.9 56.9
130 33.5 25.2 37.8

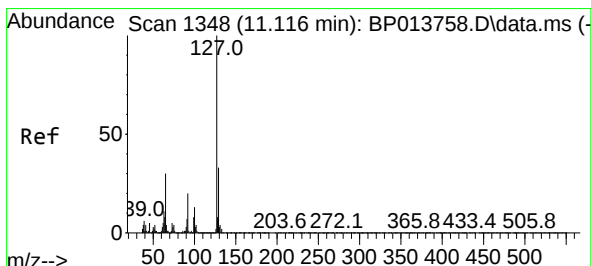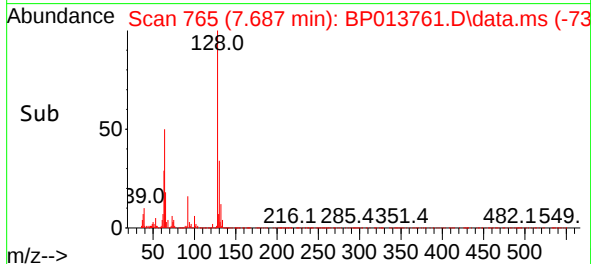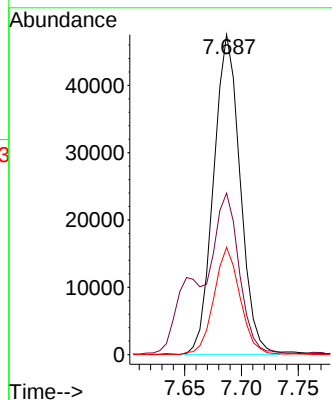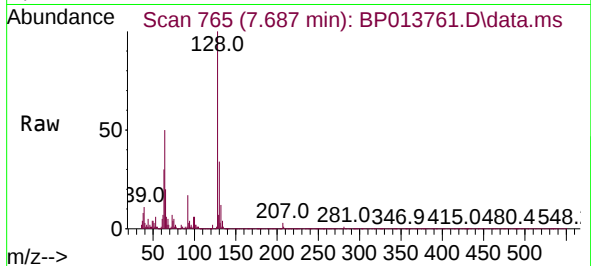

#32
4-Chloroaniline
Concen: 1.409 ng/ul
RT: 11.110 min Scan# 1347
Delta R.T. -0.006 min
Lab File: BP013761.D
Acq: 04 Feb 2023 03:26

Tgt Ion:127 Resp: 36883
Ion Ratio Lower Upper
127 100
129 33.3 26.1 39.1

