

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013762.D
 Acq On : 04 Feb 2023 04:34
 Operator : CG/JU
 Sample : 01314-24
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q7

Quant Time: Feb 04 05:00:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	8.128	152	237759	20.000 ng/u1	0.00
20) Naphthalene-d8	10.957	136	1054797	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.763	164	776776	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.516	188	2020747	20.000 ng/u1	0.00
79) Chrysene-d12	21.592	240	2110570	20.000 ng/u1	0.00
88) Perylene-d12	24.163	264	2126214	20.000 ng/u1	-0.01
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.476	96	29749	5.305 ng/uL	0.00
4) Pyridine-d5	3.911	84	214803	13.350 ng/u1	0.00
7) Phenol-d5	7.275	99	160722	7.691 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	414611	33.830 ng/u1	0.00
11) 2-Chlorophenol-d4	7.652	132	408786	26.687 ng/u1	0.00
15) 4-Methylphenol-d8	8.834	113	300403	18.033 ng/u1	0.00
21) Nitrobenzene-d5	9.305	128	247061	36.717 ng/u1	0.00
24) 2-Nitrophenol-d4	10.028	143	299712	38.220 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	608399	33.177 ng/u1	0.00
31) 4-Chloroaniline-d4	11.087	131	550100	22.713 ng/u1	0.00
46) Dimethylphthalate-d6	14.163	166	2244763	36.661 ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	2352930	34.781 ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	50587	4.902 ng/u1	0.00
60) Fluorene-d10	15.757	176	2103663	39.859 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	132107	11.666 ng/u1	0.00
73) Anthracene-d10	17.616	188	3625147	38.486 ng/u1	0.00
81) Pyrene-d10	19.833	212	4723885	40.130 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.992	264	4309671	39.706 ng/u1	-0.01
Target Compounds					
				Qvalue	
22) Nitrobenzene	9.346	77	693769	38.173 ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013762.D
Acq On : 04 Feb 2023 04:34
Operator : CG/JU
Sample : 01314-24
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q7

Quant Time: Feb 04 05:00:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 03 23:44:43 2023
Response via : Initial Calibration

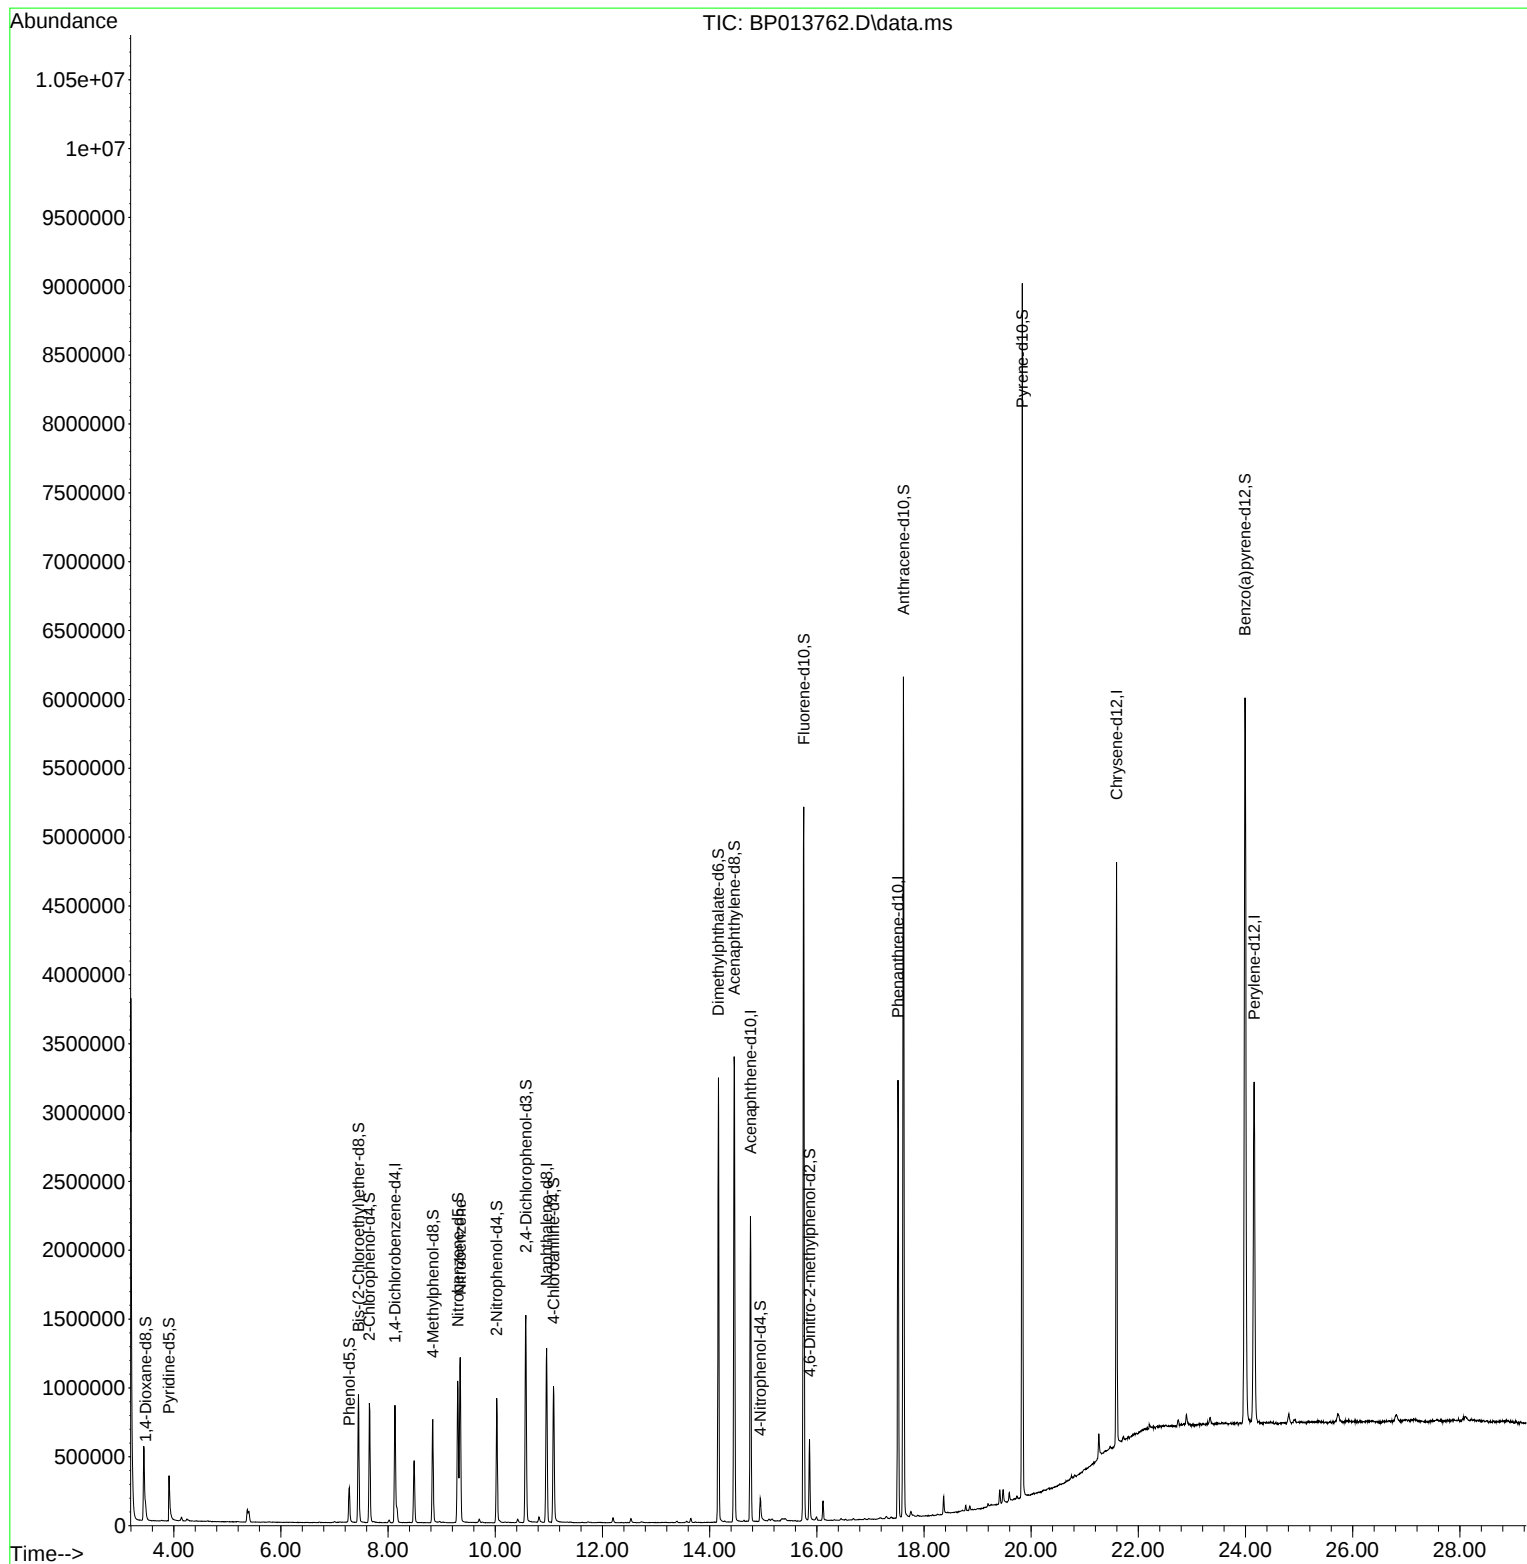

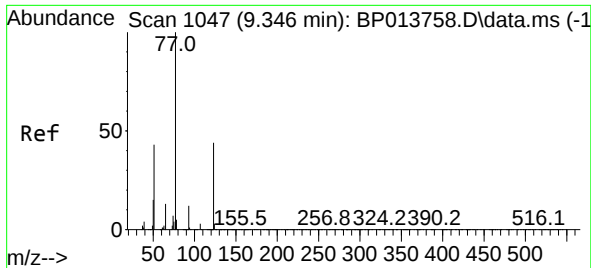

#22
 Nitrobenzene
 Concen: 38.173 ng/ul
 RT: 9.346 min Scan# 10
 Delta R.T. 0.000 min
 Lab File: BP013762.D
 Acq: 04 Feb 2023 04:34

Instrument :
 BNA_P
 ClientSampleId :
 A44Q7

Tgt Ion: 77 Resp: 693769
 Ion Ratio Lower Upper
 77 100
 123 43.6 34.1 51.1
 65 12.2 9.8 14.8

