

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013702.D
 Acq On : 02 Feb 2023 09:54
 Operator : CG/JU
 Sample : PB150531BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK531

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.476	45	49	61	rVB	55801	85367	0.96%	0.115%
2	3.911	120	123	152	rBV	705031	1163550	13.10%	1.562%
3	4.252	176	181	187	rVB	33331	49540	0.56%	0.066%
4	7.275	688	695	708	rBV	835666	1404598	15.82%	1.885%
5	7.452	718	725	740	rVB	751814	1187932	13.38%	1.595%
6	7.658	754	760	772	rBV	822797	1375207	15.49%	1.846%
7	8.134	834	841	852	rBV	752047	1224876	13.79%	1.644%
8	8.840	952	961	975	rBV	1094696	1824565	20.55%	2.449%
9	9.311	1033	1041	1054	rBV	721554	1200338	13.52%	1.611%
10	10.034	1156	1164	1173	rBV	617855	1028455	11.58%	1.380%
11	10.575	1248	1256	1270	rBV	1155641	1928859	21.72%	2.589%
12	10.963	1313	1322	1332	rBV	1148762	1947350	21.93%	2.614%
13	11.099	1337	1345	1364	rBV	1126298	2044527	23.03%	2.744%
14	12.540	1581	1590	1600	rBV2	21222	44820	0.50%	0.060%
15	14.169	1859	1867	1883	rBV	2461710	3553994	40.03%	4.770%
16	14.469	1911	1918	1927	rBV	2715798	4149930	46.74%	5.570%
17	14.775	1962	1970	1978	rBV	2083695	3159279	35.58%	4.241%
18	14.951	1992	2000	2028	rBV	895500	1433289	16.14%	1.924%
19	15.763	2131	2138	2150	rBV	3888814	5481863	61.74%	7.358%
20	15.869	2150	2156	2167	rVV	777979	1081260	12.18%	1.451%
21	16.004	2174	2179	2188	rVB2	18807	30197	0.34%	0.041%
22	17.522	2431	2437	2447	rBV	2984842	4347505	48.96%	5.836%
23	17.628	2448	2455	2464	rBV	4566252	6546680	73.73%	8.788%
24	19.422	2756	2760	2764	rVB	58427	75167	0.85%	0.101%
25	19.486	2767	2771	2777	rVV	53878	80735	0.91%	0.108%
26	19.839	2825	2831	2844	rBV	6528801	8270924	93.15%	11.102%
27	21.598	3125	3130	3140	rBV	3881610	5373585	60.52%	7.213%
28	24.010	3532	3540	3556	rVB2	4159477	8879357	100.00%	11.919%
29	24.174	3561	3568	3582	rVB2	2532432	5525876	62.23%	7.417%




Sum of corrected areas: 74499625

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013702.D
Acq On : 02 Feb 2023 09:54
Operator : CG/JU
Sample : PB150531BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK531

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

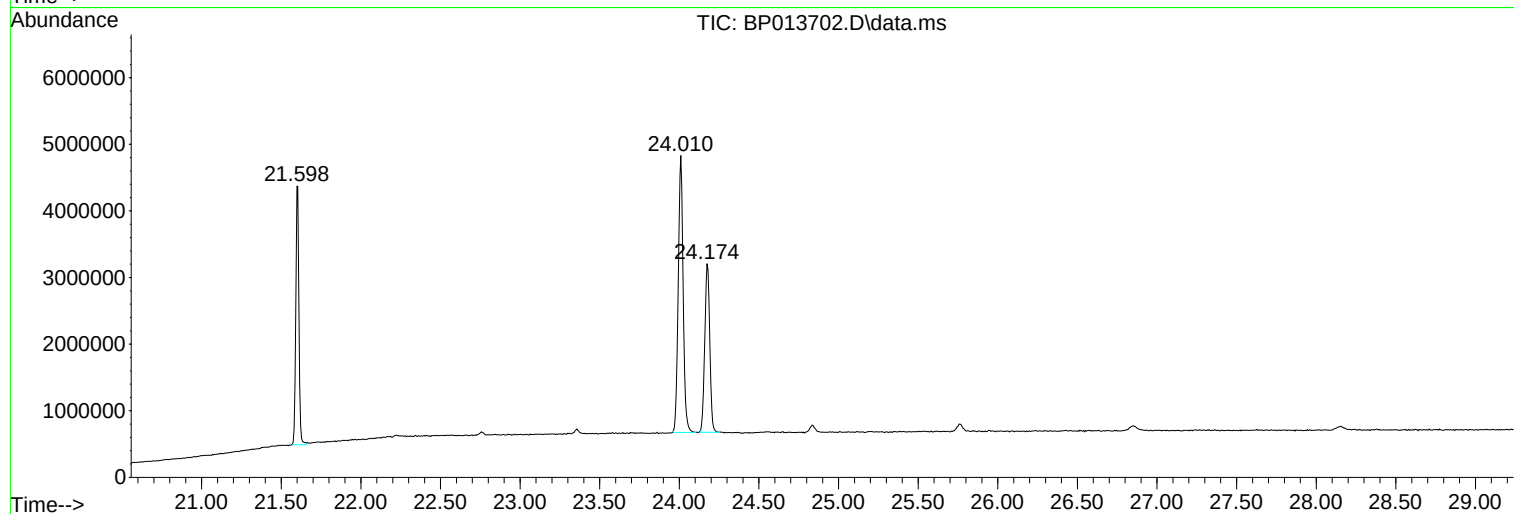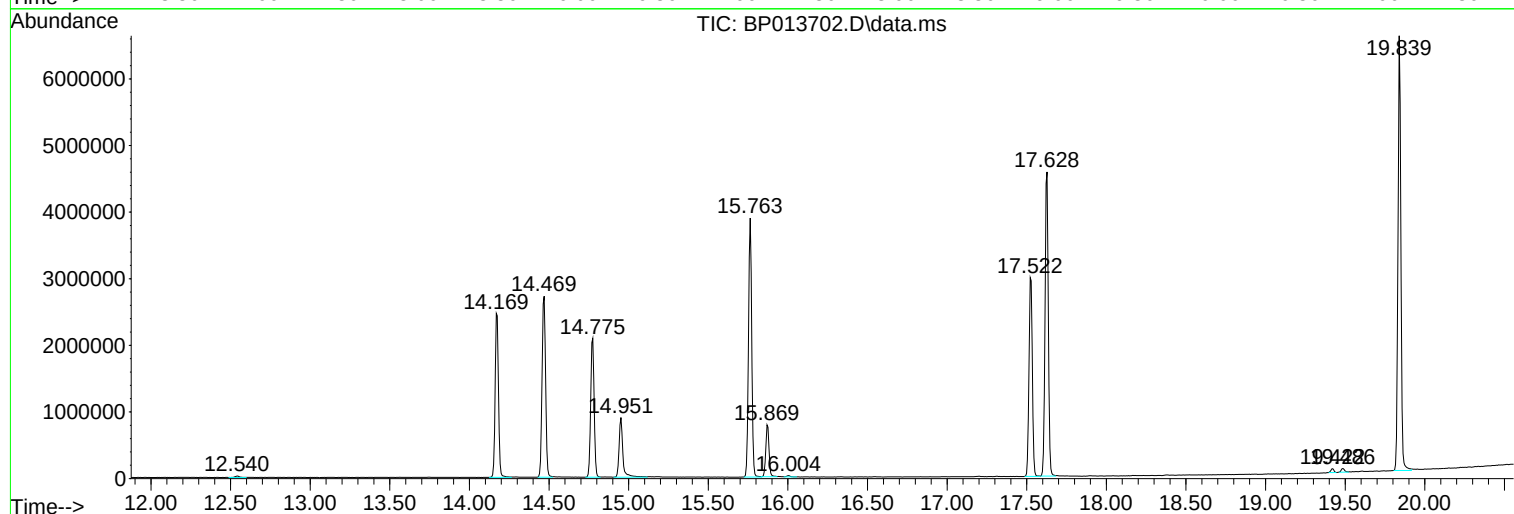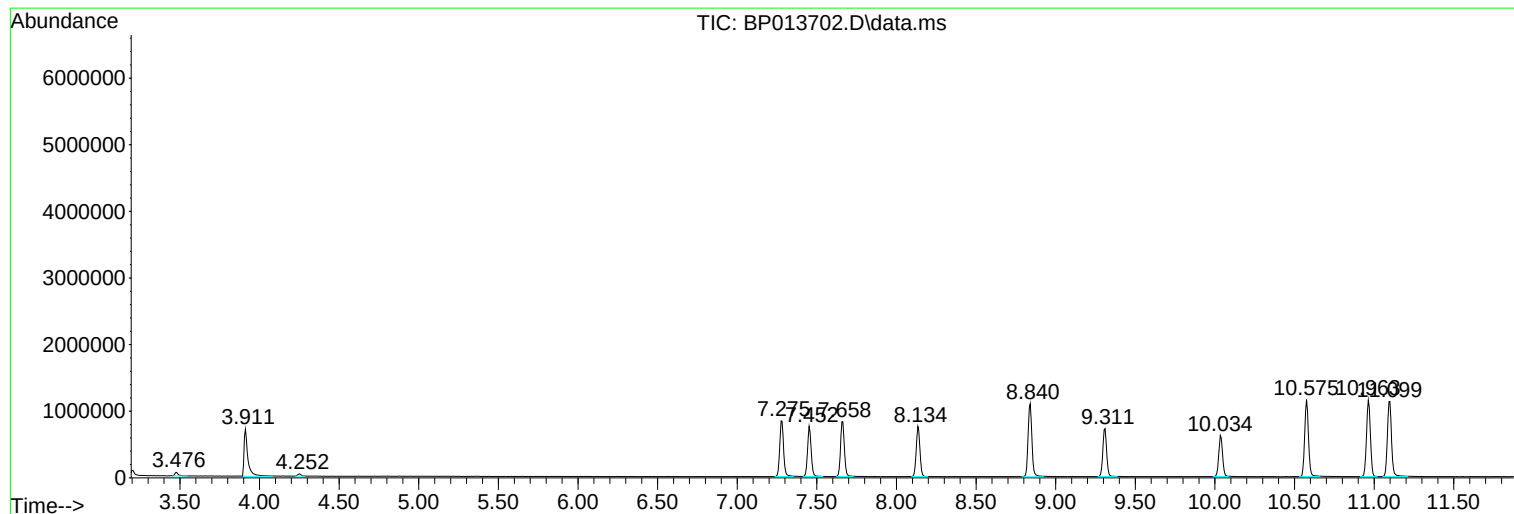

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013702.D
Acq On : 02 Feb 2023 09:54
Operator : CG/JU
Sample : PB150531BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK531

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013702.D
Acq On : 02 Feb 2023 09:54
Operator : CG/JU
Sample : PB150531BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK531

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc