

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013708.D
 Acq On : 02 Feb 2023 14:19
 Operator : CG/JU
 Sample : 01314-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.446	39	44	60	rVB	1197439	1950784	18.65%	2.242%
2	3.916	121	124	137	rBV	237645	386065	3.69%	0.444%
3	4.146	158	163	171	rBV	22573	37919	0.36%	0.044%
4	4.251	175	181	189	rVB	17191	27760	0.27%	0.032%
5	5.204	337	343	349	rBV	28852	48401	0.46%	0.056%
6	5.410	372	378	384	rBV	43886	70958	0.68%	0.082%
7	7.281	687	696	707	rBV	176033	302263	2.89%	0.347%
8	7.451	718	725	738	rBV	852235	1339794	12.81%	1.539%
9	7.663	752	761	771	rBV	714561	1173541	11.22%	1.348%
10	8.022	817	822	827	rVB4	7365	12390	0.12%	0.014%
11	8.134	832	841	854	rBV	915920	1528490	14.61%	1.756%
12	8.492	894	902	911	rBV	190403	310875	2.97%	0.357%
13	8.839	954	961	973	rBV	592267	1003109	9.59%	1.153%
14	8.939	976	978	988	rVB10	6429	13662	0.13%	0.016%
15	9.310	1033	1041	1046	rBV	869068	1498045	14.32%	1.721%
16	9.351	1046	1048	1055	rVB	109919	141608	1.35%	0.163%
17	9.710	1103	1109	1115	rVB2	15136	25220	0.24%	0.029%
18	10.034	1157	1164	1180	rVB	722700	1198671	11.46%	1.377%
19	10.575	1248	1256	1269	rBV	1250173	2101131	20.08%	2.414%
20	10.822	1291	1298	1303	rBV2	11484	21799	0.21%	0.025%
21	10.869	1303	1306	1312	rVB7	6640	12789	0.12%	0.015%
22	10.963	1314	1322	1330	rBV	1443295	2379510	22.74%	2.734%
23	11.098	1336	1345	1365	rBV	1089511	1963599	18.77%	2.256%
24	11.957	1484	1491	1497	rBV8	7432	13254	0.13%	0.015%
25	12.480	1575	1580	1585	rVV3	7151	11641	0.11%	0.013%
26	12.539	1585	1590	1599	rVB	26758	44361	0.42%	0.051%
27	12.986	1658	1666	1673	rBV3	19152	39601	0.38%	0.046%
28	13.580	1759	1767	1773	rBV7	12887	23530	0.22%	0.027%
29	13.657	1773	1780	1786	rVV3	15574	29144	0.28%	0.033%
30	13.739	1786	1794	1801	rVB8	6507	16931	0.16%	0.019%
31	13.992	1830	1837	1842	rVB10	4287	11197	0.11%	0.013%
32	14.169	1861	1867	1883	rBV	2938717	4166987	39.83%	4.788%
33	14.292	1883	1888	1893	rVB9	10592	19083	0.18%	0.022%
34	14.410	1902	1908	1911	rBV7	7805	15023	0.14%	0.017%
35	14.469	1911	1918	1930	rVV	3192150	4822668	46.09%	5.541%
36	14.645	1944	1948	1954	rVB9	6509	13022	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013708.D
 Acq On : 02 Feb 2023 14:19
 Operator : CG/JU
 Sample : 01314-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	14.769	1962	1969	1978	rBV	2537772	3786089	36.19%	4.350%
38	14.951	1994	2000	2018	rBV	135694	284210	2.72%	0.327%
39	15.163	2027	2036	2042	rBV	15377	36545	0.35%	0.042%
40	15.421	2076	2080	2082	rBV3	11805	16110	0.15%	0.019%
41	15.763	2130	2138	2150	rBV	4653509	6521368	62.33%	7.493%
42	15.869	2150	2156	2171	rVV	1060252	1505912	14.39%	1.730%
43	16.004	2173	2179	2182	rVV4	23545	46643	0.45%	0.054%
44	16.045	2182	2186	2190	rVB	38811	54421	0.52%	0.063%
45	16.121	2193	2199	2208	rVV	843112	1148013	10.97%	1.319%
46	16.351	2233	2238	2243	rBV2	25230	36486	0.35%	0.042%
47	16.692	2291	2296	2300	rBV	36934	52335	0.50%	0.060%
48	16.898	2328	2331	2341	rVB	8238	15144	0.14%	0.017%
49	17.204	2378	2383	2388	rVB9	11929	21385	0.20%	0.025%
50	17.268	2390	2394	2396	rVV5	9025	10665	0.10%	0.012%
51	17.310	2399	2401	2408	rVB3	9421	15780	0.15%	0.018%
52	17.527	2431	2438	2448	rBV	3506786	5068011	48.44%	5.823%
53	17.627	2448	2455	2464	rVV	5647129	8263961	78.99%	9.496%
54	17.698	2464	2467	2471	rVB3	32472	45291	0.43%	0.052%
55	18.168	2544	2547	2551	rBV6	11460	13961	0.13%	0.016%
56	18.374	2577	2582	2590	rBV	143917	208309	1.99%	0.239%
57	18.786	2649	2652	2656	rVB3	33766	38312	0.37%	0.044%
58	19.421	2756	2760	2764	rBV2	81674	105612	1.01%	0.121%
59	19.486	2767	2771	2779	rVB	87022	129483	1.24%	0.149%
60	19.598	2787	2790	2796	rBV2	65700	95028	0.91%	0.109%
61	19.845	2826	2832	2846	rBV	7583994	10462680	100.00%	12.022%
62	21.274	3071	3075	3082	rBV2	302256	492209	4.70%	0.566%
63	21.486	3108	3111	3121	rVB	236864	295740	2.83%	0.340%
64	21.604	3126	3131	3141	rVB	4021085	5572953	53.27%	6.404%
65	22.915	3351	3354	3360	rVB	239295	330134	3.16%	0.379%
66	24.009	3532	3540	3557	rVB2	4609389	10112785	96.66%	11.620%
67	24.180	3562	3569	3581	rVB2	2587409	5469364	52.27%	6.284%




Sum of corrected areas: 87029764

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013708.D
Acq On : 02 Feb 2023 14:19
Operator : CG/JU
Sample : 01314-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

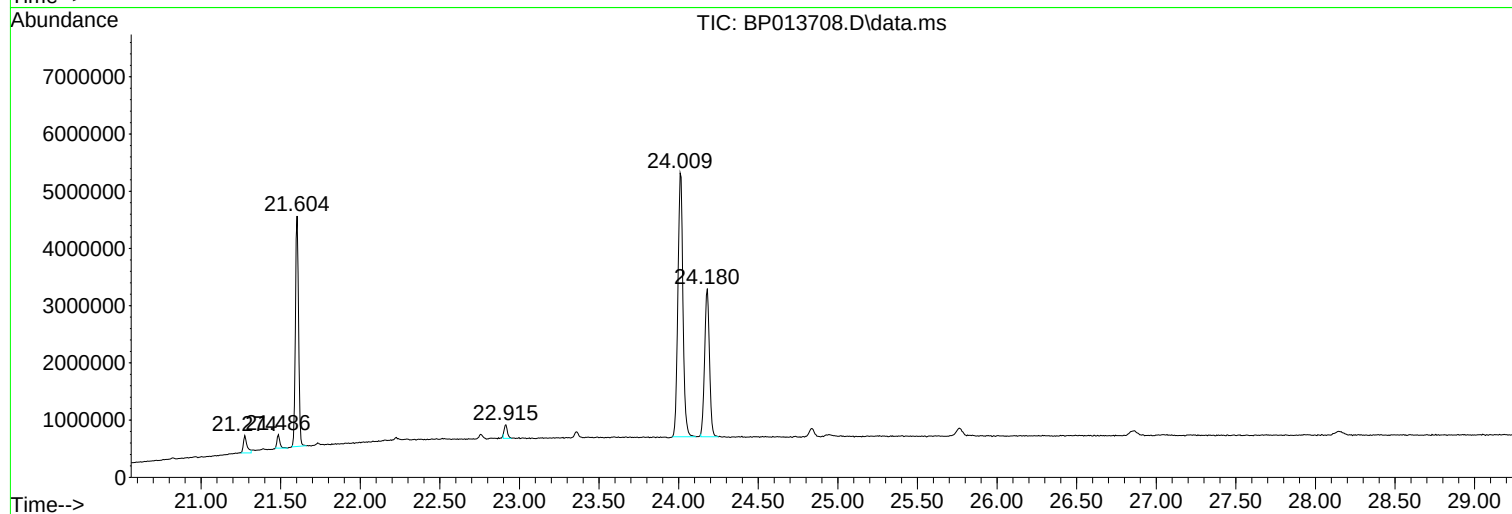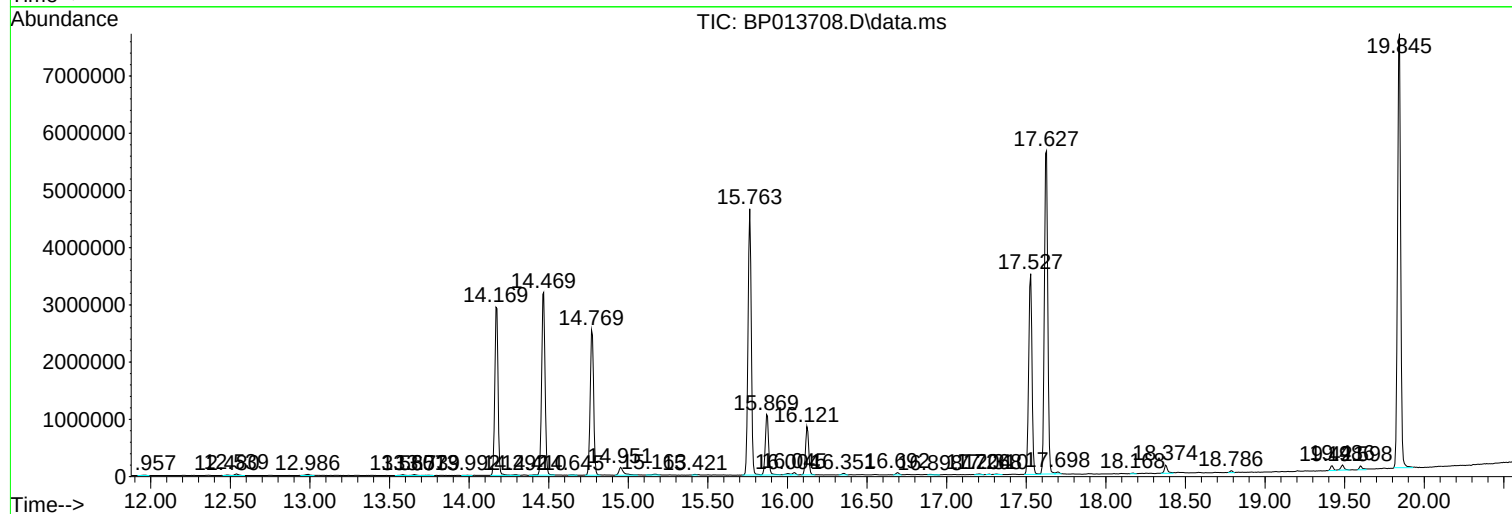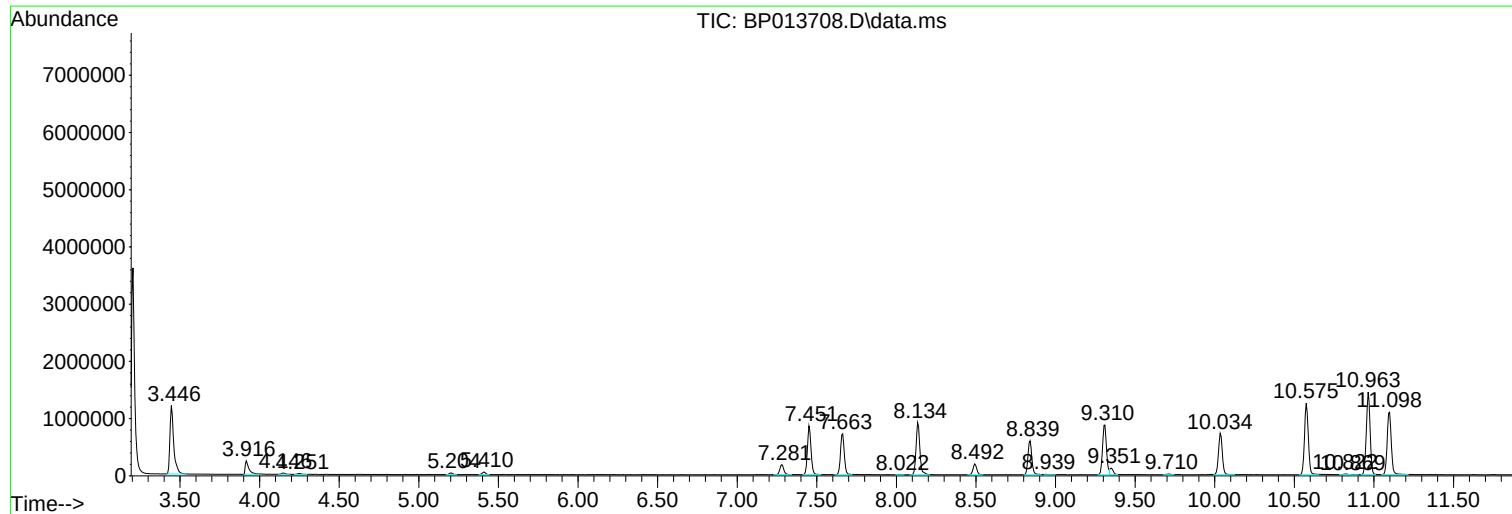

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013708.D
Acq On : 02 Feb 2023 14:19
Operator : CG/JU
Sample : 01314-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.121	6.06 ng/ul	1148010	Acenaphthene-d10	14.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	93
5			Azobenzene	182	C12H10N2	000103-33-3	64

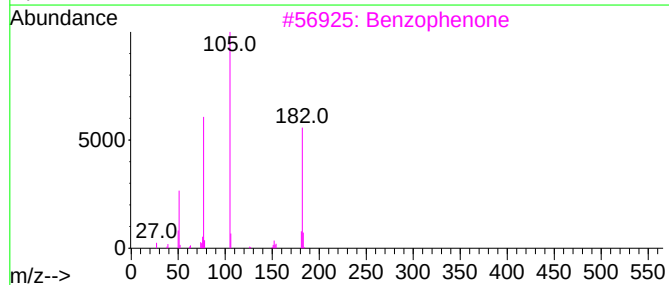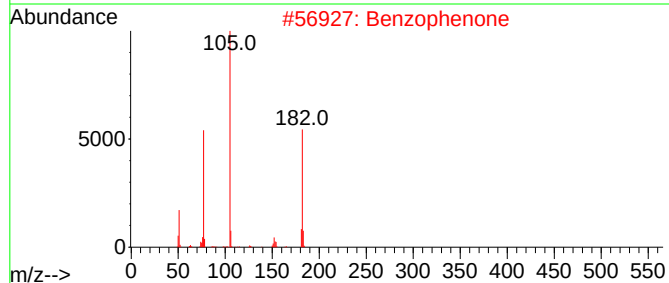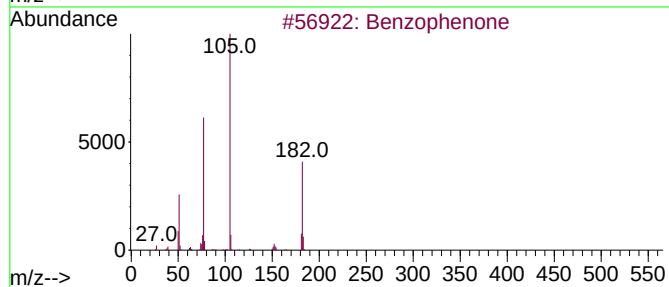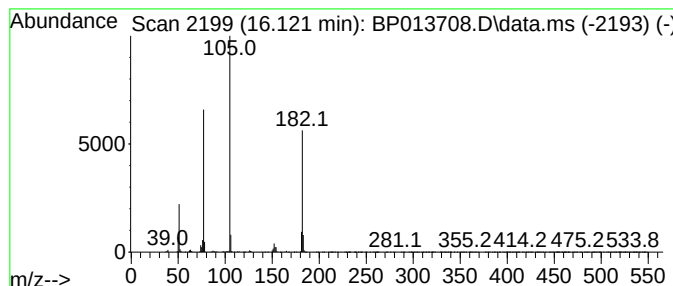

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013708.D
Acq On : 02 Feb 2023 14:19
Operator : CG/JU
Sample : 01314-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.121	6.1	ng/ul	1148010	3	14.769	3786090	20.0