

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013710.D
 Acq On : 02 Feb 2023 15:28
 Operator : CG/JU
 Sample : 01314-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.446	39	44	47	rBV	138500	192705	1.81%	0.209%
2	3.475	47	49	57	rVB	60486	80346	0.75%	0.087%
3	3.917	122	124	139	rBV	229538	375470	3.52%	0.408%
4	4.152	158	164	169	rBV	26699	43392	0.41%	0.047%
5	4.252	176	181	184	rBV	17733	28652	0.27%	0.031%
6	5.205	336	343	348	rVB3	9835	16443	0.15%	0.018%
7	5.411	369	378	392	rVB	934586	1455636	13.64%	1.581%
8	7.005	643	649	656	rVB	15851	26217	0.25%	0.028%
9	7.281	685	696	706	rBV	216521	366993	3.44%	0.398%
10	7.452	716	725	743	rBV	1489561	2372044	22.23%	2.576%
11	7.663	753	761	771	rBV	779223	1299379	12.18%	1.411%
12	8.022	815	822	830	rBV	145840	238447	2.24%	0.259%
13	8.134	833	841	845	rBV	933563	1562407	14.65%	1.696%
14	8.169	845	847	858	rVB	451336	636352	5.96%	0.691%
15	8.493	894	902	917	rBV	1583462	2602640	24.40%	2.826%
16	8.840	954	961	976	rBV	687994	1134867	10.64%	1.232%
17	8.963	979	982	989	rVV3	10470	19881	0.19%	0.022%
18	9.040	989	995	1002	rVB3	6095	12638	0.12%	0.014%
19	9.310	1033	1041	1057	rBV	949325	1625451	15.24%	1.765%
20	9.710	1105	1109	1115	rVB	38758	62014	0.58%	0.067%
21	10.034	1157	1164	1179	rBV	787822	1301426	12.20%	1.413%
22	10.575	1248	1256	1278	rBV	1335845	2274980	21.33%	2.470%
23	10.822	1292	1298	1303	rBV2	74976	123168	1.15%	0.134%
24	10.863	1303	1305	1313	rVB5	7533	11497	0.11%	0.012%
25	10.963	1315	1322	1330	rBV	1412762	2382079	22.33%	2.587%
26	11.093	1337	1344	1358	rBV	1099231	1940580	18.19%	2.107%
27	11.352	1383	1388	1394	rVB2	14047	23970	0.22%	0.026%
28	12.210	1526	1534	1540	rVB	27524	43809	0.41%	0.048%
29	12.540	1585	1590	1595	rBV	27112	44893	0.42%	0.049%
30	13.587	1761	1768	1775	rVB4	11353	20281	0.19%	0.022%
31	14.175	1861	1868	1884	rBV	3027647	4329949	40.59%	4.702%
32	14.293	1884	1888	1894	rVB9	7890	14604	0.14%	0.016%
33	14.469	1911	1918	1935	rBV	3242639	5024019	47.09%	5.455%
34	14.651	1944	1949	1952	rBV3	11832	16907	0.16%	0.018%
35	14.769	1962	1969	1978	rBV	2477772	3807692	35.69%	4.134%
36	14.951	1994	2000	2013	rBV	147317	292611	2.74%	0.318%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013710.D
 Acq On : 02 Feb 2023 15:28
 Operator : CG/JU
 Sample : 01314-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	15.169	2034	2037	2043	rVB8	11291	18989	0.18%	0.021%
38	15.763	2129	2138	2151	rBV	4726190	6758813	63.36%	7.339%
39	15.869	2151	2156	2175	rVB	1056214	1485526	13.92%	1.613%
40	16.004	2175	2179	2182	rBV2	20959	28926	0.27%	0.031%
41	16.122	2193	2199	2211	rVB	218468	324610	3.04%	0.352%
42	16.357	2231	2239	2242	rBV7	6657	14251	0.13%	0.015%
43	16.457	2252	2256	2263	rBV6	11234	22331	0.21%	0.024%
44	16.557	2267	2273	2277	rVB7	5967	12215	0.11%	0.013%
45	16.692	2291	2296	2300	rBV	25630	36372	0.34%	0.039%
46	17.198	2378	2382	2388	rVB9	7859	16405	0.15%	0.018%
47	17.304	2398	2400	2407	rVB3	7160	11617	0.11%	0.013%
48	17.528	2431	2438	2448	rBV	3537454	5064908	47.48%	5.500%
49	17.628	2448	2455	2466	rBV	5677038	8105013	75.97%	8.801%
50	18.375	2578	2582	2588	rBV	159010	208124	1.95%	0.226%
51	18.704	2634	2638	2643	rBV3	19017	32723	0.31%	0.036%
52	18.786	2649	2652	2656	rVB2	49744	54769	0.51%	0.059%
53	19.204	2720	2723	2726	rBV4	25943	34161	0.32%	0.037%
54	19.422	2756	2760	2765	rVB2	76706	103097	0.97%	0.112%
55	19.486	2767	2771	2775	rVV	86307	119351	1.12%	0.130%
56	19.598	2787	2790	2796	rBV3	74643	104224	0.98%	0.113%
57	19.845	2826	2832	2847	rBV	8017056	10668130	100.00%	11.584%
58	21.275	3071	3075	3084	rBV2	295317	511541	4.80%	0.555%
59	21.604	3126	3131	3138	rBV	4309834	5780845	54.19%	6.277%
60	22.916	3351	3354	3365	rVB2	313335	493339	4.62%	0.536%
61	24.016	3533	3541	3554	rVB2	4731575	10405787	97.54%	11.299%
62	24.180	3562	3569	3581	rVB2	2688639	5875826	55.08%	6.380%




Sum of corrected areas: 92096332

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013710.D
Acq On : 02 Feb 2023 15:28
Operator : CG/JU
Sample : 01314-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

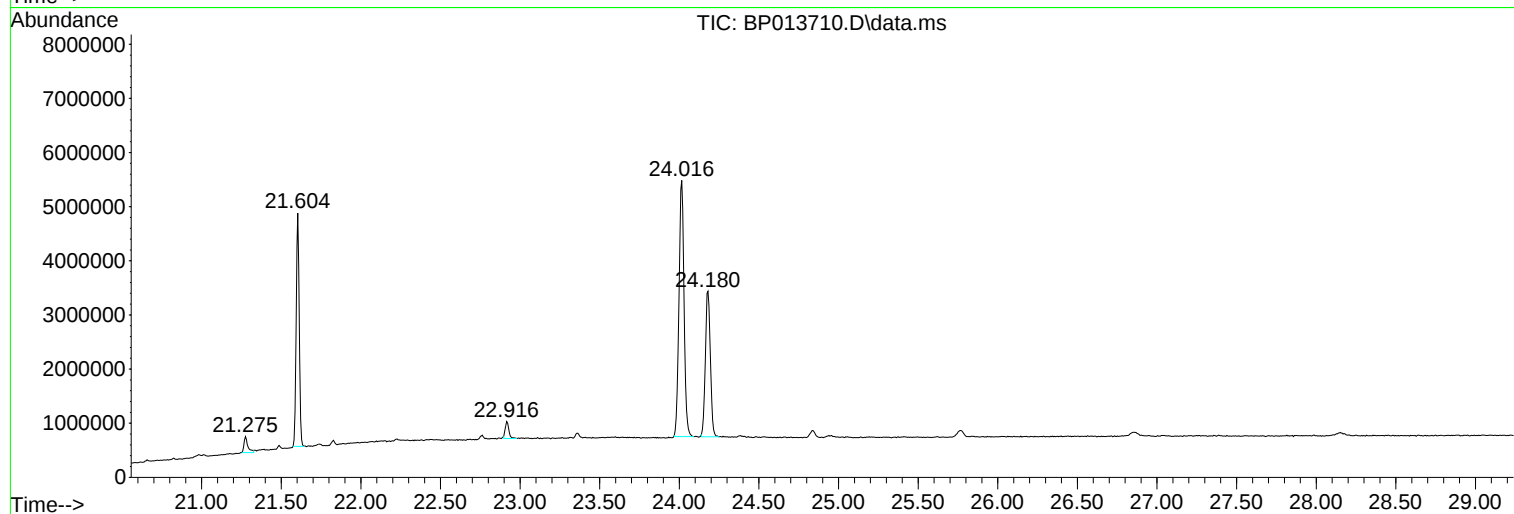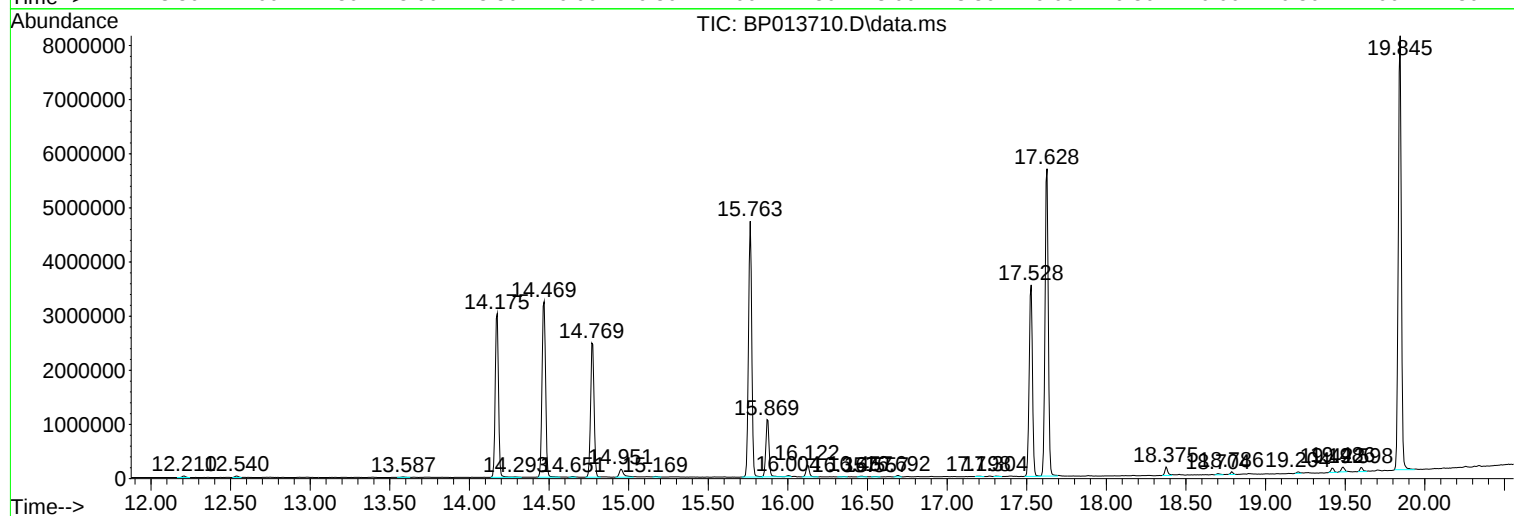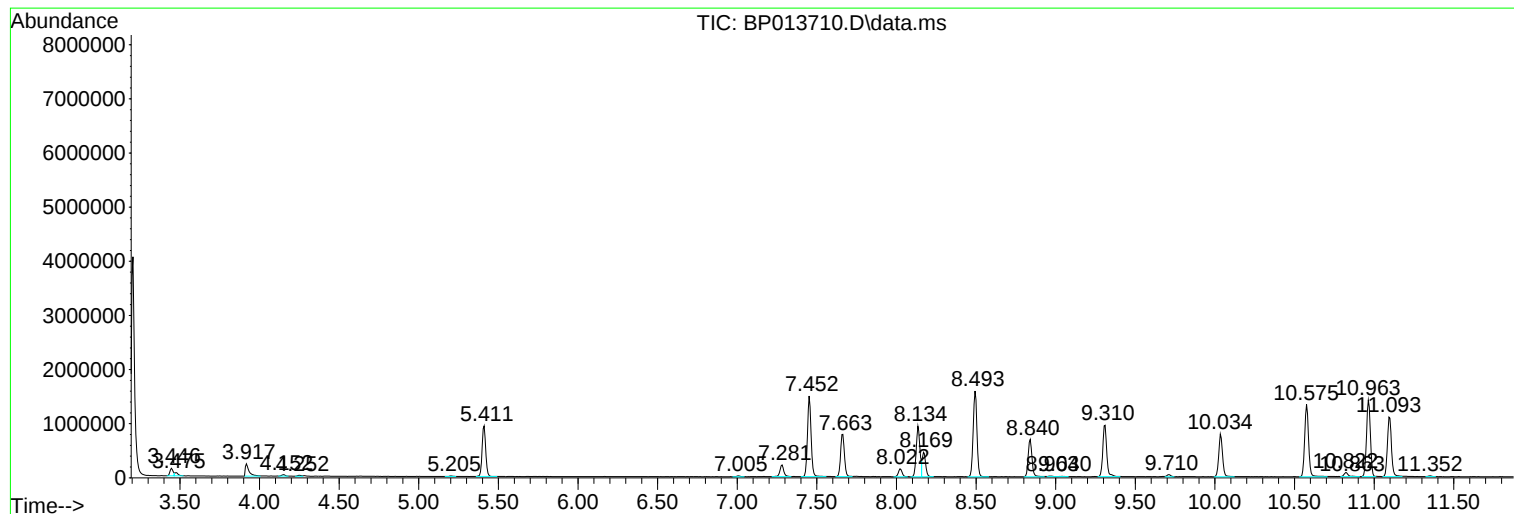

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013710.D
Acq On : 02 Feb 2023 15:28
Operator : CG/JU
Sample : 01314-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013710.D
Acq On : 02 Feb 2023 15:28
Operator : CG/JU
Sample : 01314-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc