

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013715.D
 Acq On : 02 Feb 2023 18:20
 Operator : CG/JU
 Sample : PB150546BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK546

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	57	rVB	58060	86203	0.92%	0.102%
2	3.911	120	123	147	rBV	836966	1346687	14.42%	1.586%
3	4.246	177	180	190	rVB	17403	30276	0.32%	0.036%
4	7.281	689	696	716	rBV	995473	1650644	17.67%	1.944%
5	7.452	719	725	737	rVV	874102	1360148	14.56%	1.602%
6	7.658	754	760	774	rBV	974577	1622756	17.37%	1.911%
7	8.134	834	841	852	rBB	955595	1542515	16.51%	1.817%
8	8.840	952	961	977	rBV	1272635	2146861	22.98%	2.529%
9	9.305	1030	1040	1054	rBV	876799	1489823	15.95%	1.755%
10	10.034	1155	1164	1176	rBV	764167	1252937	13.41%	1.476%
11	10.575	1248	1256	1276	rBV	1322075	2275074	24.36%	2.680%
12	10.963	1313	1322	1332	rBV	1446891	2437219	26.09%	2.871%
13	11.093	1335	1344	1363	rBV	1272375	2315412	24.79%	2.727%
14	12.540	1584	1590	1601	rBV2	23413	44472	0.48%	0.052%
15	14.175	1861	1868	1880	rBV	2678738	3929985	42.07%	4.629%
16	14.469	1910	1918	1929	rBV	3076403	4658360	49.87%	5.487%
17	14.775	1962	1970	1978	rBV	2620992	3932219	42.10%	4.631%
18	14.951	1994	2000	2018	rBV	1052846	1648457	17.65%	1.942%
19	15.175	2035	2038	2043	rVB6	7468	10882	0.12%	0.013%
20	15.763	2130	2138	2150	rBV	4476481	6231264	66.71%	7.339%
21	15.869	2150	2156	2173	rVB	1013755	1416211	15.16%	1.668%
22	16.004	2175	2179	2183	rVV2	18531	25330	0.27%	0.030%
23	16.751	2301	2306	2311	rBV9	4307	9427	0.10%	0.011%
24	17.204	2379	2383	2388	rVB8	7029	12112	0.13%	0.014%
25	17.310	2399	2401	2410	rVB3	7979	13967	0.15%	0.016%
26	17.528	2431	2438	2448	rBV	3655261	5288911	56.62%	6.229%
27	17.622	2448	2454	2474	rVB2	4830835	7125439	76.28%	8.392%
28	19.422	2756	2760	2765	rVB2	64896	85454	0.91%	0.101%
29	19.486	2767	2771	2777	rVV	67963	95227	1.02%	0.112%
30	19.845	2825	2832	2847	rBV	6649878	9340801	100.00%	11.002%
31	21.604	3125	3131	3139	rBV	4707164	6404960	68.57%	7.544%
32	24.010	3533	3540	3556	rVB2	4122726	9005759	96.41%	10.607%
33	24.180	3562	3569	3579	rVB2	2890573	6068205	64.96%	7.147%




Sum of corrected areas: 84903997

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013715.D
Acq On : 02 Feb 2023 18:20
Operator : CG/JU
Sample : PB150546BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

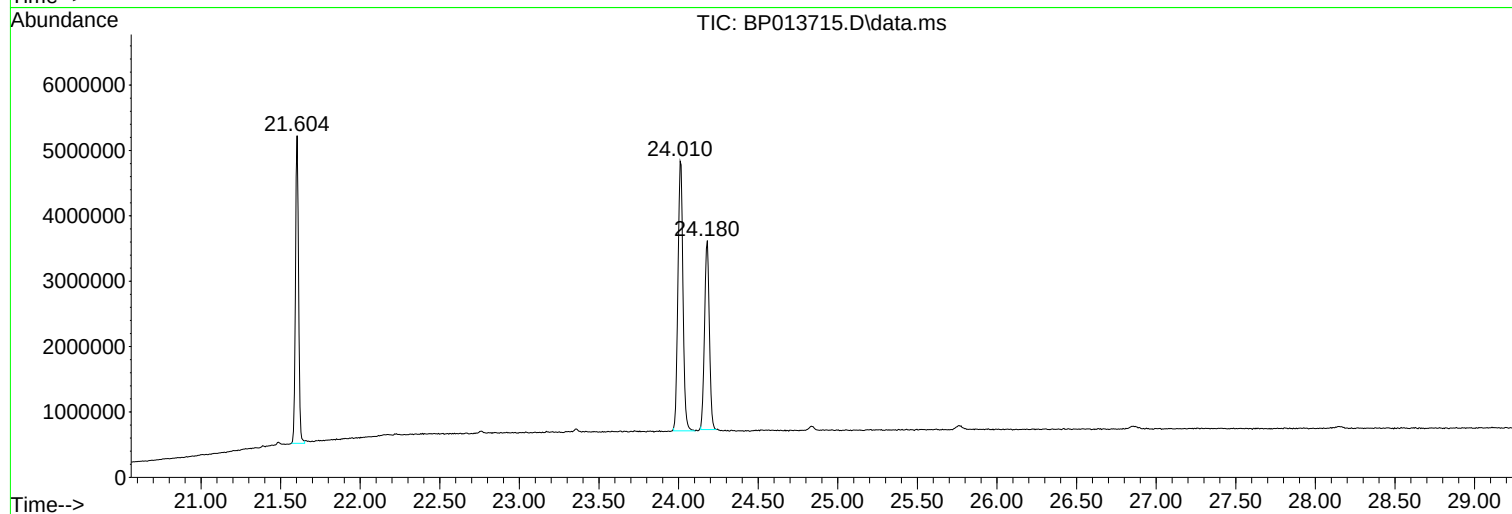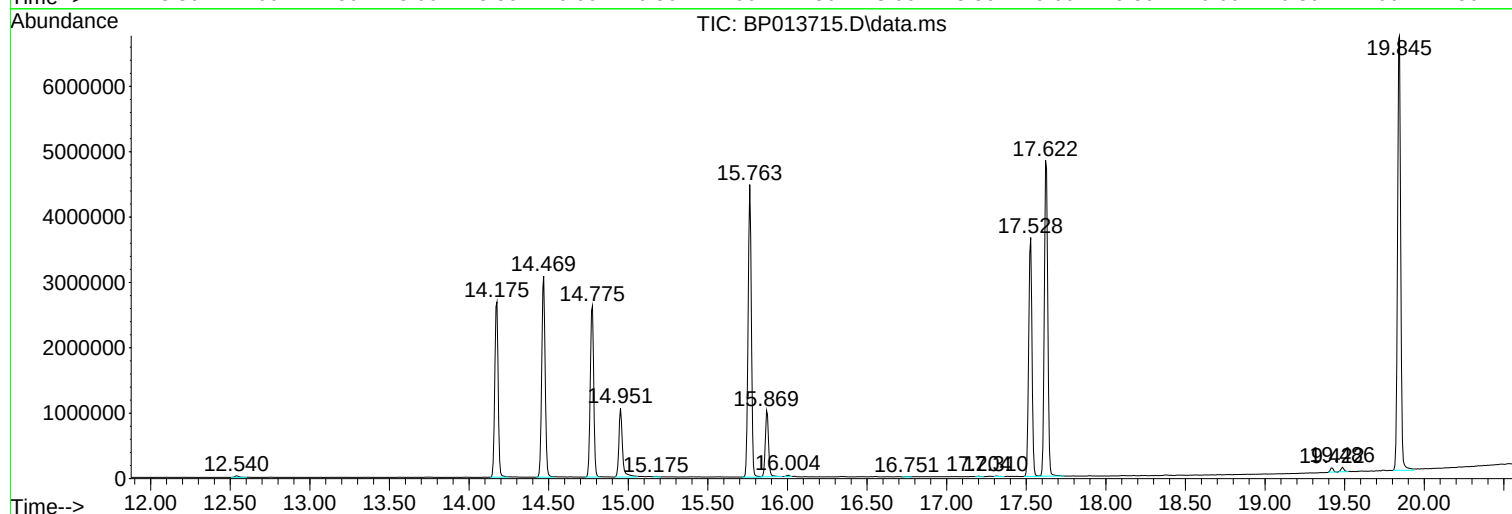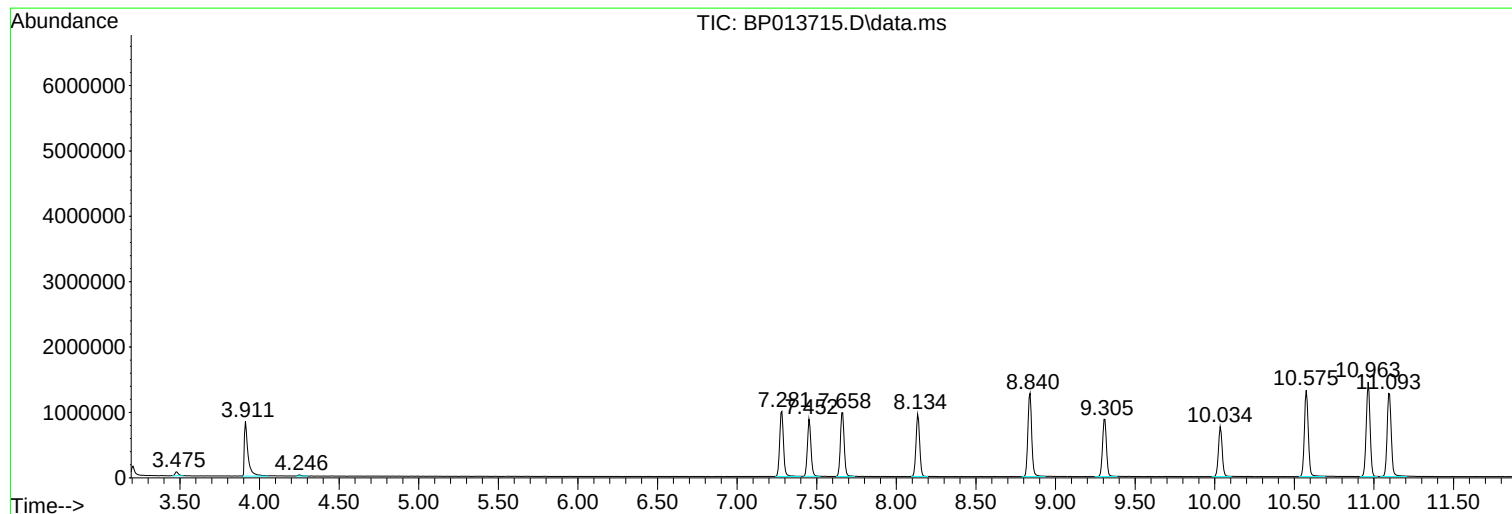

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013715.D
Acq On : 02 Feb 2023 18:20
Operator : CG/JU
Sample : PB150546BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013715.D
Acq On : 02 Feb 2023 18:20
Operator : CG/JU
Sample : PB150546BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc