

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013720.D
 Acq On : 02 Feb 2023 21:12
 Operator : CG/JU
 Sample : 01314-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.446	38	44	66	rVB	767873	1345885	4.88%	1.059%
2	3.917	121	124	140	rBV	239373	403627	1.46%	0.317%
3	4.152	158	164	171	rVB2	24086	40851	0.15%	0.032%
4	4.252	176	181	186	rVB	23227	34911	0.13%	0.027%
5	5.205	336	343	354	rBV	22555	41449	0.15%	0.033%
6	5.405	369	377	390	rVB	375653	619093	2.24%	0.487%
7	6.775	604	610	619	rBV3	13939	30927	0.11%	0.024%
8	7.281	687	696	706	rBV	189408	323191	1.17%	0.254%
9	7.452	718	725	734	rBV	961725	1501246	5.44%	1.181%
10	7.657	753	760	771	rBV	770976	1267168	4.59%	0.997%
11	8.022	814	822	830	rBV	338614	545574	1.98%	0.429%
12	8.134	834	841	843	rBV	1025508	1561489	5.66%	1.228%
13	8.169	843	847	856	rVB	2903387	4691364	17.00%	3.690%
14	8.499	893	903	914	rBV	15771297	27600448	100.00%	21.708%
15	8.834	953	960	972	rBV	593060	1008928	3.66%	0.794%
16	8.940	974	978	987	rVB	27407	51400	0.19%	0.040%
17	9.304	1032	1040	1044	rBV	941667	1573832	5.70%	1.238%
18	9.351	1044	1048	1057	rVB	544679	897837	3.25%	0.706%
19	9.640	1092	1097	1104	rBV6	17033	36924	0.13%	0.029%
20	9.710	1104	1109	1115	rVB2	22593	35858	0.13%	0.028%
21	10.034	1158	1164	1177	rVB	740381	1214340	4.40%	0.955%
22	10.575	1247	1256	1266	rBV	1295860	2156853	7.81%	1.696%
23	10.822	1291	1298	1313	rVB	307491	513216	1.86%	0.404%
24	10.963	1313	1322	1330	rBV	1517855	2536144	9.19%	1.995%
25	11.093	1336	1344	1361	rBV	1069913	1889233	6.84%	1.486%
26	11.346	1381	1387	1394	rVB	55131	96055	0.35%	0.076%
27	12.469	1571	1578	1585	rBV	98054	163357	0.59%	0.128%
28	12.534	1585	1589	1597	rVB2	26276	46722	0.17%	0.037%
29	13.581	1759	1767	1772	rBV3	21315	37008	0.13%	0.029%
30	13.657	1772	1780	1787	rVB2	67440	113809	0.41%	0.090%
31	13.851	1807	1813	1820	rVB6	17459	31102	0.11%	0.024%
32	14.169	1860	1867	1882	rBV	3229420	4520825	16.38%	3.556%
33	14.345	1893	1897	1902	rBV	22334	31610	0.11%	0.025%
34	14.463	1910	1917	1929	rBV	3364762	5067754	18.36%	3.986%
35	14.769	1963	1969	1976	rBV	2780681	4006259	14.52%	3.151%
36	14.951	1995	2000	2006	rBV2	162567	274502	0.99%	0.216%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013720.D
 Acq On : 02 Feb 2023 21:12
 Operator : CG/JU
 Sample : 01314-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	15.257	2047	2052	2062	rBV2	27287	54838	0.20%	0.043%
38	15.763	2130	2138	2145	rBV	4899428	7098018	25.72%	5.583%
39	15.828	2145	2149	2151	rVV	111822	165146	0.60%	0.130%
40	15.869	2151	2156	2168	rVB	1184838	1606643	5.82%	1.264%
41	15.998	2173	2178	2183	rVV2	24622	40669	0.15%	0.032%
42	16.122	2191	2199	2212	rBV	1569276	2111815	7.65%	1.661%
43	16.345	2232	2237	2243	rBV	44263	73443	0.27%	0.058%
44	16.463	2251	2257	2263	rBV9	10024	29495	0.11%	0.023%
45	16.522	2264	2267	2280	rVB5	25162	64311	0.23%	0.051%
46	16.686	2291	2295	2308	rVB	138132	206858	0.75%	0.163%
47	17.310	2398	2401	2411	rVB4	22841	38442	0.14%	0.030%
48	17.522	2431	2437	2445	rBV	3651225	5316908	19.26%	4.182%
49	17.622	2448	2454	2465	rBV	5816143	8561335	31.02%	6.734%
50	18.375	2578	2582	2591	rBV	197510	278156	1.01%	0.219%
51	18.698	2634	2637	2644	rVB	43167	64636	0.23%	0.051%
52	18.786	2649	2652	2656	rVV	59863	63903	0.23%	0.050%
53	19.110	2704	2707	2711	rBV	71022	90413	0.33%	0.071%
54	19.204	2720	2723	2728	rBV7	30448	50258	0.18%	0.040%
55	19.422	2756	2760	2763	rBV2	87541	115257	0.42%	0.091%
56	19.480	2766	2770	2780	rVB2	145273	253410	0.92%	0.199%
57	19.598	2787	2790	2798	rBV4	77034	115905	0.42%	0.091%
58	19.839	2825	2831	2845	rBV	8056585	11153031	40.41%	8.772%
59	21.274	3071	3075	3084	rBV2	461682	734409	2.66%	0.578%
60	21.604	3125	3131	3137	rBV	4486047	6036863	21.87%	4.748%
61	24.010	3533	3540	3555	rVB2	5008314	10712155	38.81%	8.425%
62	24.174	3561	3568	3581	rVB2	2653128	5797173	21.00%	4.560%




Sum of corrected areas: 127144281

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013720.D
Acq On : 02 Feb 2023 21:12
Operator : CG/JU
Sample : 01314-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

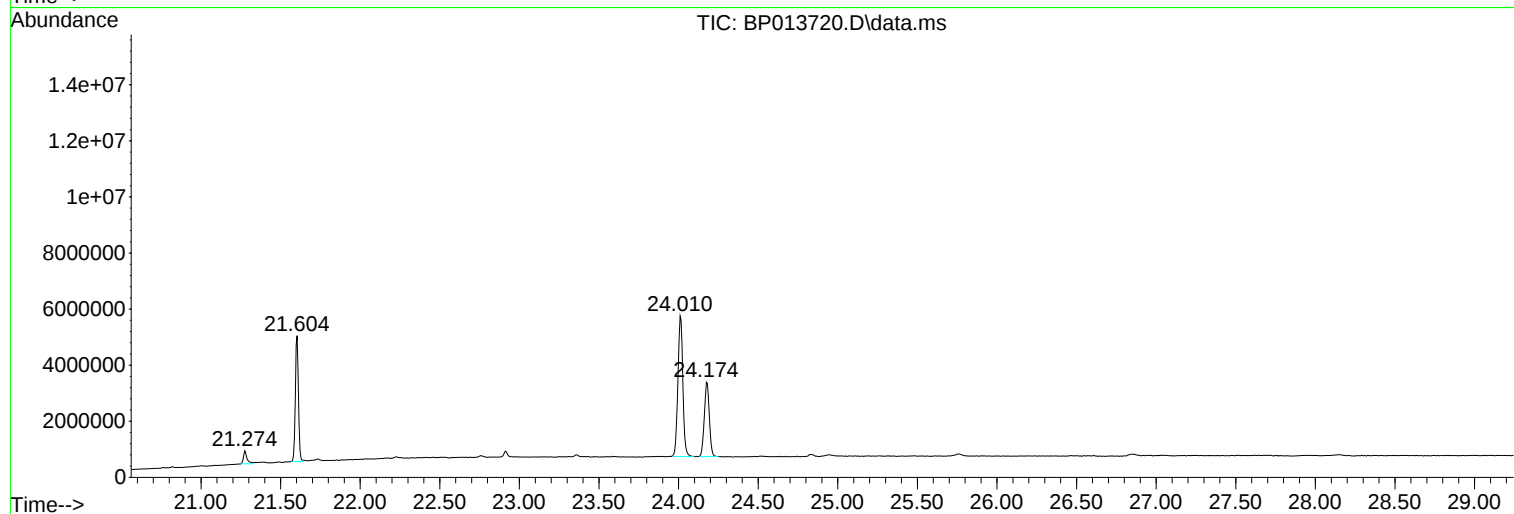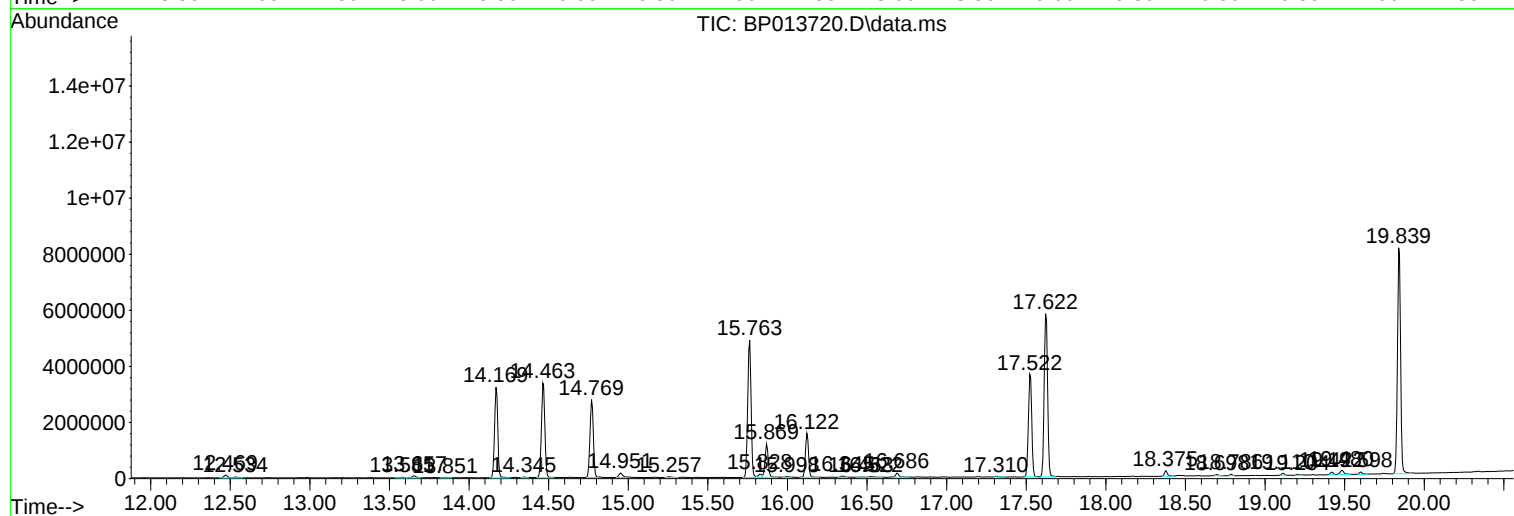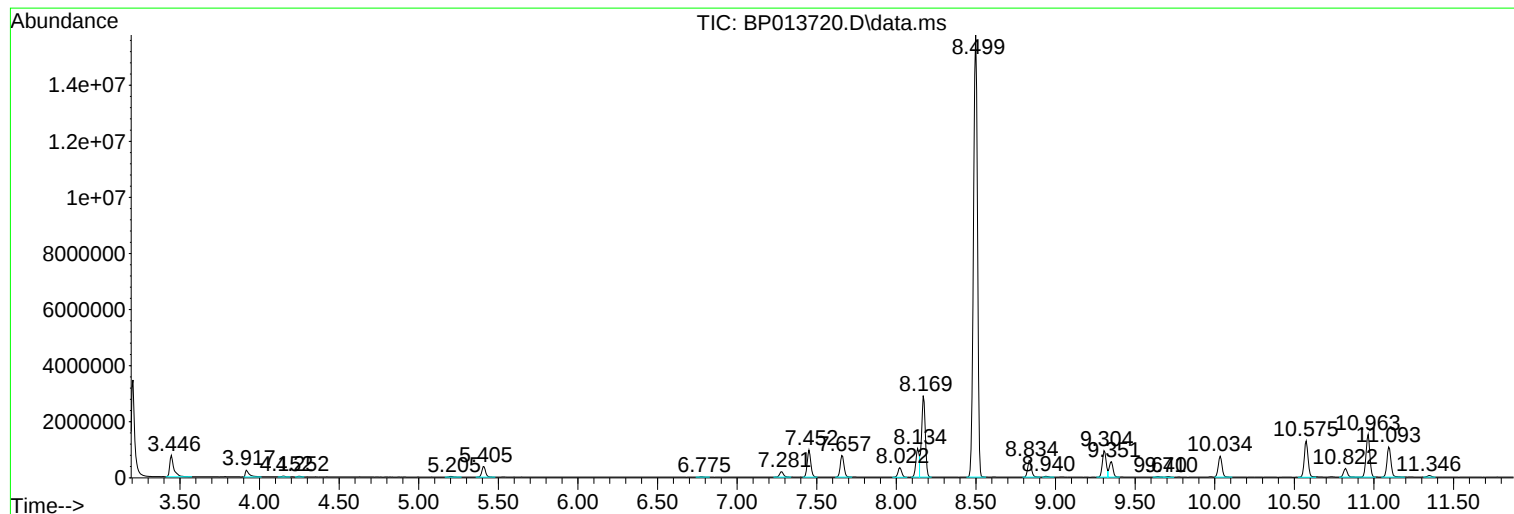

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013720.D
Acq On : 02 Feb 2023 21:12
Operator : CG/JU
Sample : 01314-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Benzophenone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.122	10.54 ng/ul	2111820	Acenaphthene-d10	14.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	93
5			Benzophenone	182	C13H10O	000119-61-9	90

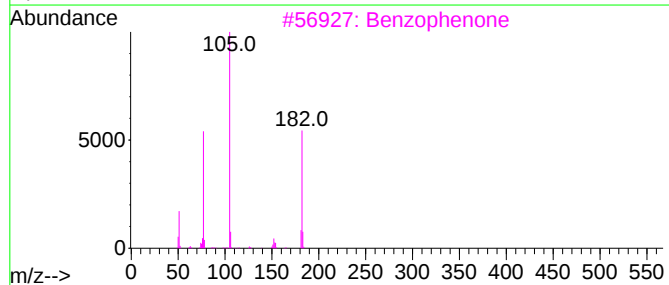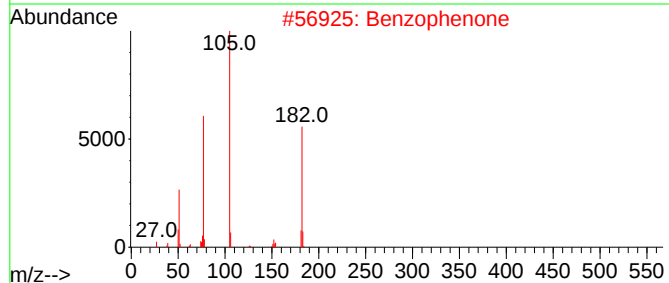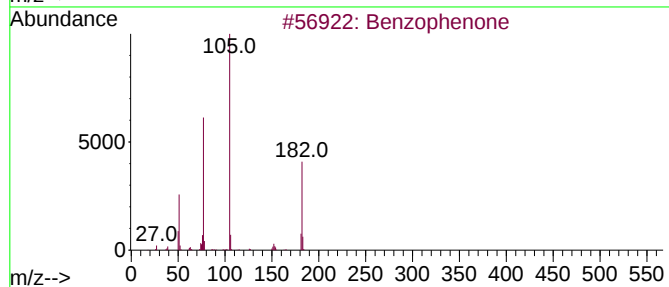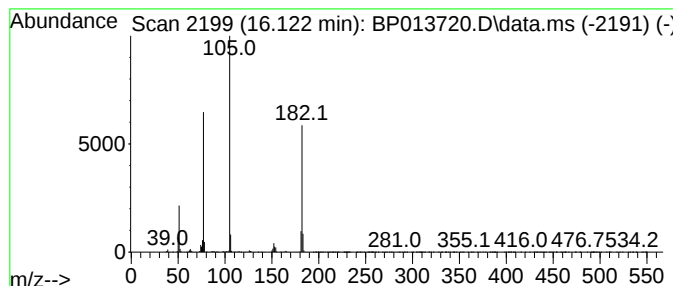

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013720.D
Acq On : 02 Feb 2023 21:12
Operator : CG/JU
Sample : 01314-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Dichloroacetic acid, heptad... Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.274	2.43 ng/ul	734409	Chrysene-d12	21.604

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	93
2			Cyclopentadecane	210	C15H30	000295-48-7	93
3			1-Heptacosanol	396	C27H56O	002004-39-9	91
4			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
5			1-Nonadecene	266	C19H38	018435-45-5	87

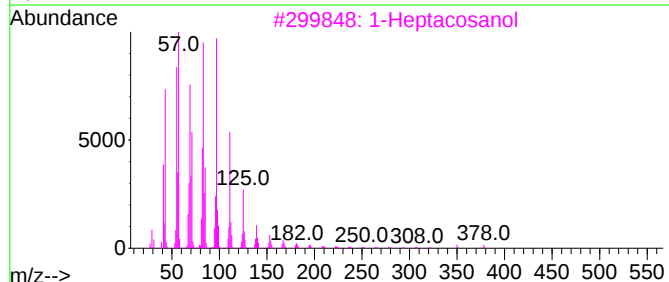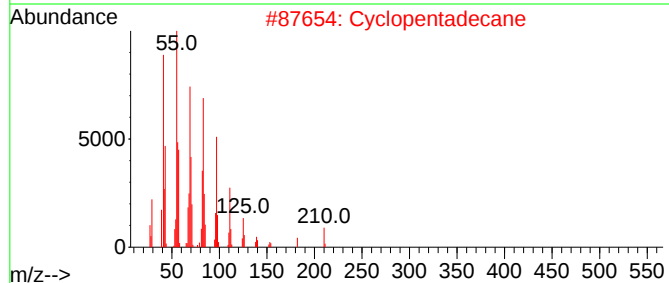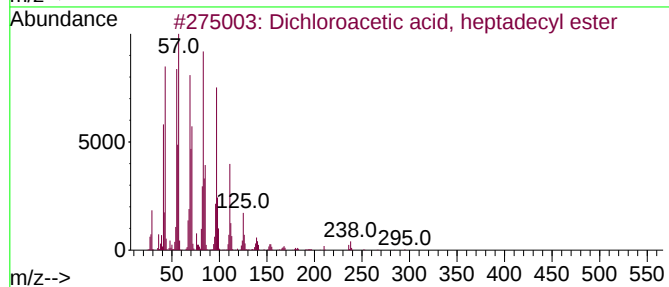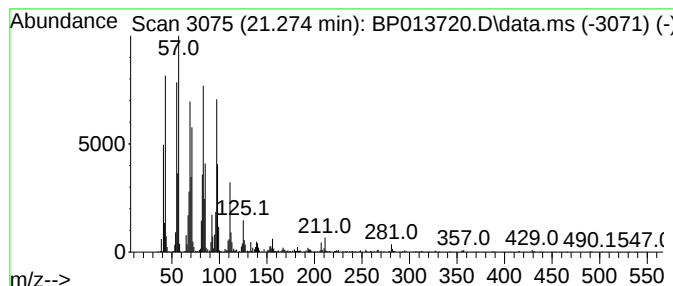

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013720.D
Acq On : 02 Feb 2023 21:12
Operator : CG/JU
Sample : 01314-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.122	10.5	ng/ul	2111820	3	14.769	4006260	20.0
Dichloroacetic ...	21.274	2.4	ng/ul	734409	5	21.604	6036860	20.0