

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013726.D
 Acq On : 03 Feb 2023 00:37
 Operator : CG/JU
 Sample : 01314-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	60	rVB	64516	99991	0.71%	0.092%
2	3.917	121	124	137	rBV	182808	304647	2.17%	0.281%
3	4.146	158	163	170	rBV2	33314	51951	0.37%	0.048%
4	4.246	176	180	185	rBV	33399	49459	0.35%	0.046%
5	5.199	338	342	350	rVB4	9875	18101	0.13%	0.017%
6	6.022	478	482	490	rBV2	10257	17851	0.13%	0.016%
7	6.093	490	494	502	rVV5	8563	16011	0.11%	0.015%
8	7.275	687	695	710	rVB	272541	462038	3.30%	0.427%
9	7.452	718	725	738	rBV	1224390	1951046	13.92%	1.802%
10	7.658	752	760	771	rBV	1060658	1737161	12.40%	1.605%
11	8.134	831	841	854	rBV	1167637	1886952	13.47%	1.743%
12	8.834	953	960	973	rBV	855811	1435210	10.24%	1.326%
13	9.304	1033	1040	1051	rBV	1353434	2195980	15.67%	2.029%
14	9.710	1103	1109	1113	rVB2	12880	21140	0.15%	0.020%
15	10.034	1156	1164	1183	rBV	1063936	1752008	12.50%	1.618%
16	10.569	1248	1255	1274	rBV	1684630	2917780	20.82%	2.695%
17	10.963	1314	1322	1336	rBV	1716958	2915268	20.81%	2.693%
18	11.093	1336	1344	1360	rBV	1404798	2435312	17.38%	2.250%
19	12.204	1528	1533	1534	rBV2	18545	22880	0.16%	0.021%
20	12.228	1534	1537	1546	rVB3	23123	47479	0.34%	0.044%
21	12.534	1583	1589	1601	rBV3	35841	62455	0.45%	0.058%
22	14.169	1860	1867	1883	rBV	3947389	5468107	39.03%	5.051%
23	14.463	1910	1917	1932	rVB	4384231	6608591	47.16%	6.105%
24	14.769	1957	1969	1977	rBV	3213031	4818261	34.39%	4.451%
25	14.839	1977	1981	1988	rVB3	26953	48385	0.35%	0.045%
26	14.951	1994	2000	2016	rBV	165894	331207	2.36%	0.306%
27	15.175	2033	2038	2044	rVB8	15648	28048	0.20%	0.026%
28	15.434	2078	2082	2089	rVB3	11084	20172	0.14%	0.019%
29	15.763	2126	2138	2150	rBV	6141931	8975083	64.05%	8.291%
30	15.869	2150	2156	2167	rVV	1537132	2041207	14.57%	1.886%
31	15.998	2174	2178	2185	rVB	28731	43487	0.31%	0.040%
32	16.545	2266	2271	2278	rVB10	9029	18384	0.13%	0.017%
33	17.104	2361	2366	2370	rBV3	14312	20427	0.15%	0.019%
34	17.198	2378	2382	2388	rVB8	10478	17000	0.12%	0.016%
35	17.522	2431	2437	2447	rBV	4308965	6097812	43.52%	5.633%
36	17.622	2447	2454	2471	rVV2	7440881	11035263	78.76%	10.194%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013726.D
 Acq On : 03 Feb 2023 00:37
 Operator : CG/JU
 Sample : 01314-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44K0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	18.169	2542	2547	2553	rBV	287895	358677	2.56%	0.331%
38	18.375	2578	2582	2588	rBV	65571	88099	0.63%	0.081%
39	19.416	2755	2759	2764	rBV	107692	147541	1.05%	0.136%
40	19.486	2767	2771	2777	rVB	104758	147137	1.05%	0.136%
41	19.598	2787	2790	2797	rBV3	42238	59796	0.43%	0.055%
42	19.839	2825	2831	2843	rBV	10404959	14011678	100.00%	12.943%
43	21.598	3125	3130	3140	rBV	5112938	7248498	51.73%	6.696%
44	24.010	3532	3540	3551	rVB2	6358269	13321153	95.07%	12.305%
45	24.174	3561	3568	3580	rVB2	3180346	6899233	49.24%	6.373%




Sum of corrected areas: 108253966

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013726.D
Acq On : 03 Feb 2023 00:37
Operator : CG/JU
Sample : 01314-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

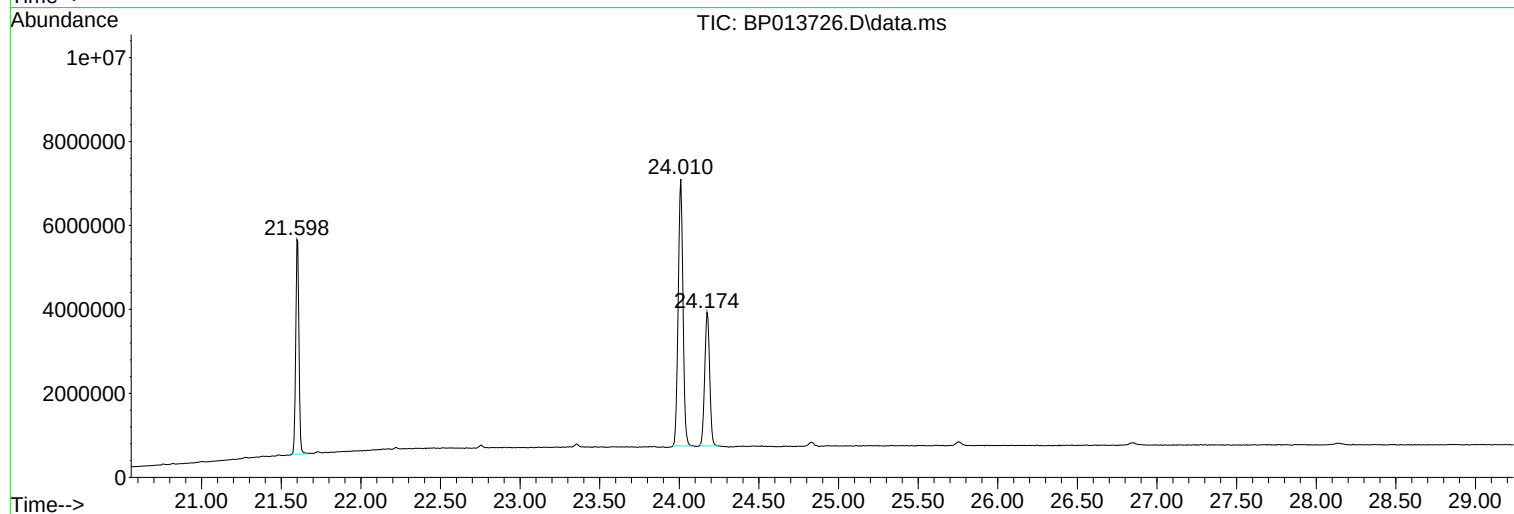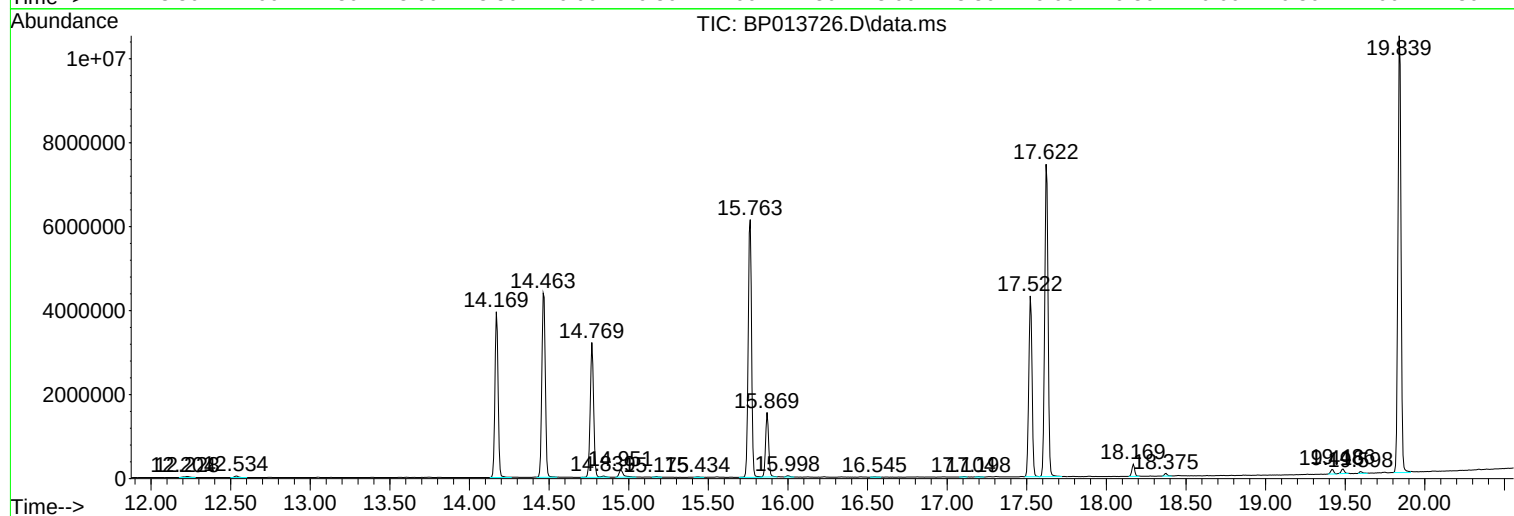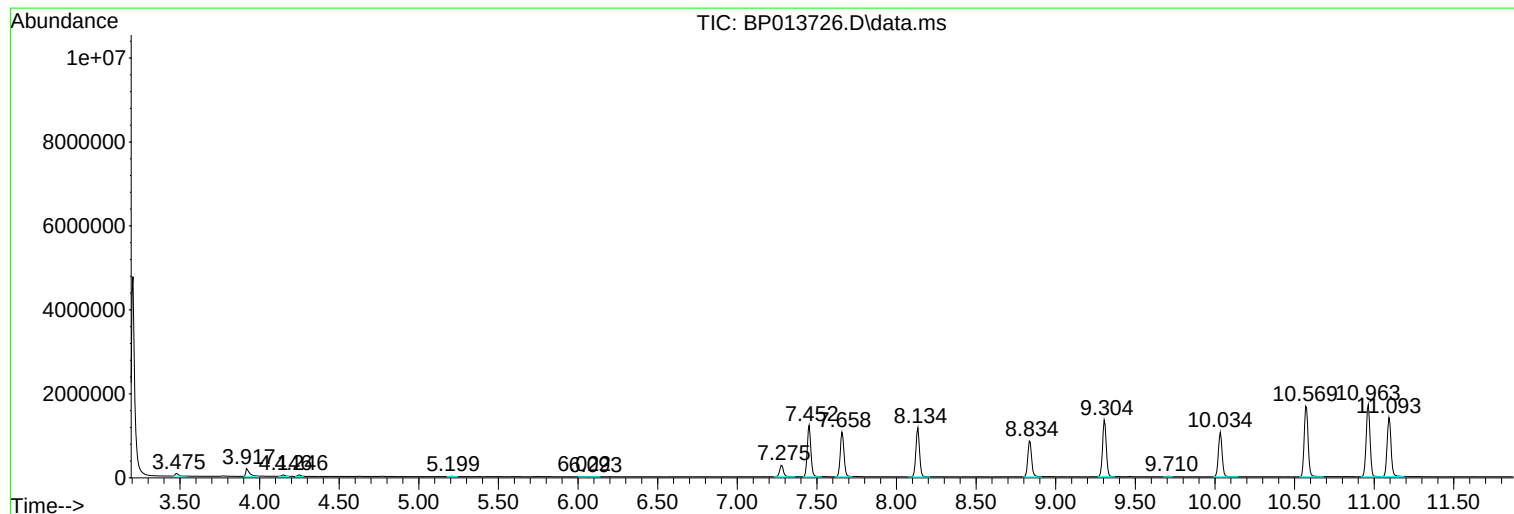

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013726.D
Acq On : 03 Feb 2023 00:37
Operator : CG/JU
Sample : 01314-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013726.D
Acq On : 03 Feb 2023 00:37
Operator : CG/JU
Sample : 01314-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------