

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013732.D
 Acq On : 03 Feb 2023 09:31
 Operator : CG/JU
 Sample : PB150529BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK529

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.481	44	50	61	rVB	51384	84229	0.85%	0.110%
2	3.916	121	124	145	rBV	630038	1153380	11.65%	1.500%
3	4.252	177	181	188	rBV	13935	20709	0.21%	0.027%
4	7.287	687	697	710	rBV	838135	1373690	13.87%	1.786%
5	7.457	719	726	740	rVB	763584	1198149	12.10%	1.558%
6	7.663	754	761	774	rBV	809871	1360254	13.73%	1.769%
7	8.140	835	842	853	rBV	789571	1279108	12.91%	1.663%
8	8.846	955	962	982	rBV	1101197	1801083	18.18%	2.342%
9	9.316	1032	1042	1050	rBV	752917	1225943	12.38%	1.594%
10	10.046	1157	1166	1174	rBV	613013	1026664	10.37%	1.335%
11	10.581	1247	1257	1272	rBV	1158749	1982262	20.01%	2.578%
12	10.969	1315	1323	1335	rBV	1226645	2056042	20.76%	2.674%
13	11.104	1338	1346	1361	rBV	1188789	2041789	20.62%	2.655%
14	12.545	1586	1591	1598	rBV	21944	39348	0.40%	0.051%
15	13.939	1818	1828	1829	rBV10	6282	13941	0.14%	0.018%
16	14.181	1862	1869	1882	rVB	2489577	3348329	33.81%	4.354%
17	14.475	1911	1919	1929	rBV	2639674	3950759	39.89%	5.138%
18	14.781	1964	1971	1979	rVB	2251009	3306522	33.38%	4.300%
19	14.957	1993	2001	2024	rBV	753140	1280264	12.93%	1.665%
20	15.504	2090	2094	2096	rBV5	7079	10535	0.11%	0.014%
21	15.692	2120	2126	2127	rBV6	19011	29201	0.29%	0.038%
22	15.769	2133	2139	2150	rVB	3753998	5497858	55.51%	7.150%
23	15.881	2152	2158	2174	rVV	790334	1079842	10.90%	1.404%
24	16.010	2176	2180	2186	rVB2	17362	27340	0.28%	0.036%
25	16.145	2196	2203	2211	rVB5	10603	26681	0.27%	0.035%
26	16.798	2308	2314	2319	rBV5	12737	24179	0.24%	0.031%
27	16.980	2341	2345	2352	rVB3	34513	57217	0.58%	0.074%
28	17.210	2381	2384	2390	rVB7	6273	10422	0.11%	0.014%
29	17.351	2404	2408	2412	rVB4	14403	20726	0.21%	0.027%
30	17.533	2432	2439	2449	rBV	3222306	4595467	46.40%	5.976%
31	17.633	2450	2456	2470	rVV	4545855	6461285	65.24%	8.403%
32	17.904	2499	2502	2507	rVB4	13760	19999	0.20%	0.026%
33	18.057	2524	2528	2532	rVB2	27350	32491	0.33%	0.042%
34	18.169	2545	2547	2553	rVB7	10838	18365	0.19%	0.024%
35	18.386	2579	2584	2589	rBV5	39094	67408	0.68%	0.088%
36	18.475	2595	2599	2602	rBV6	9497	13414	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013732.D
 Acq On : 03 Feb 2023 09:31
 Operator : CG/JU
 Sample : PB150529BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK529

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	18.963	2679	2682	2686	rVB3	26947	32092	0.32%	0.042%
38	19.427	2758	2761	2768	rVB2	61201	80687	0.81%	0.105%
39	19.498	2769	2773	2777	rBV2	61240	83916	0.85%	0.109%
40	19.727	2809	2812	2815	rBV4	31852	36834	0.37%	0.048%
41	19.851	2827	2833	2849	rBV	6340013	9904320	100.00%	12.880%
42	21.616	3127	3133	3143	rVB	4282070	5793866	58.50%	7.535%
43	24.027	3535	3543	3560	rBV2	4123906	8694022	87.78%	11.306%
44	24.192	3564	3571	3584	rVB2	2645390	5735048	57.90%	7.458%




Sum of corrected areas: 76895680

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013732.D
Acq On : 03 Feb 2023 09:31
Operator : CG/JU
Sample : PB150529BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK529

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

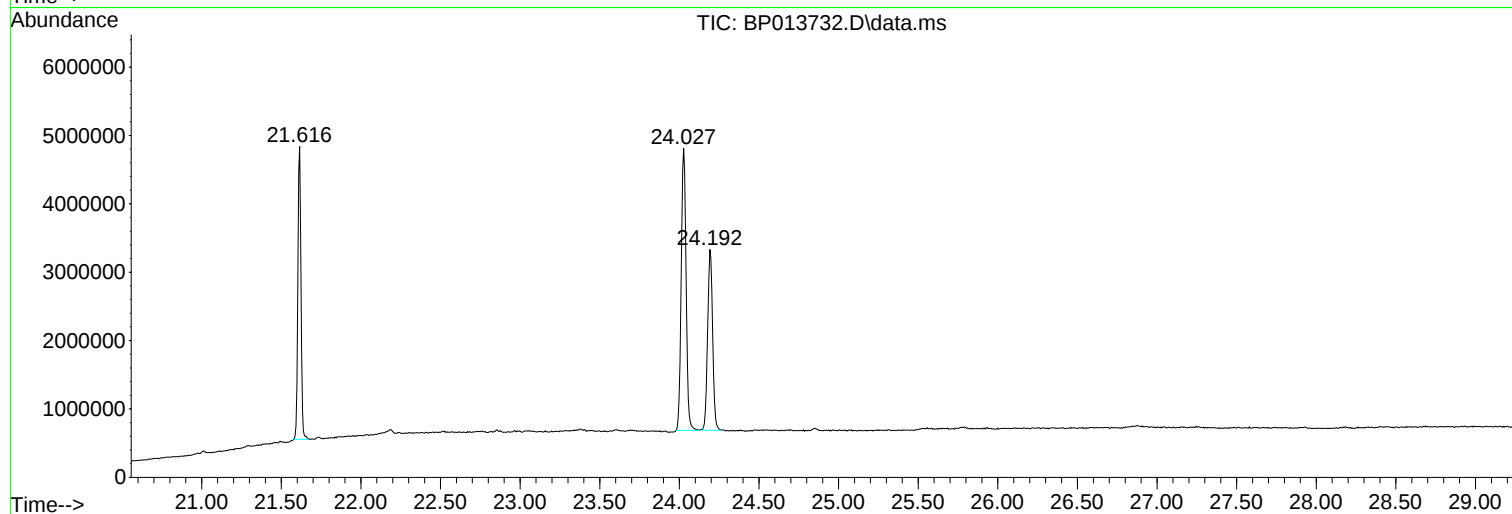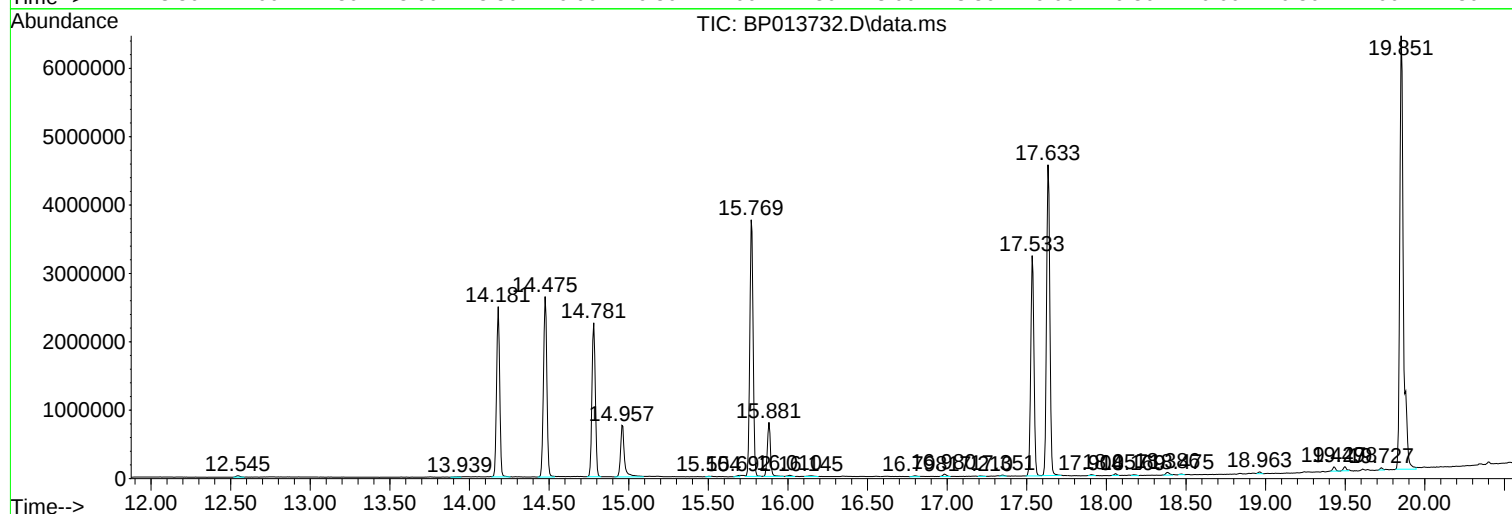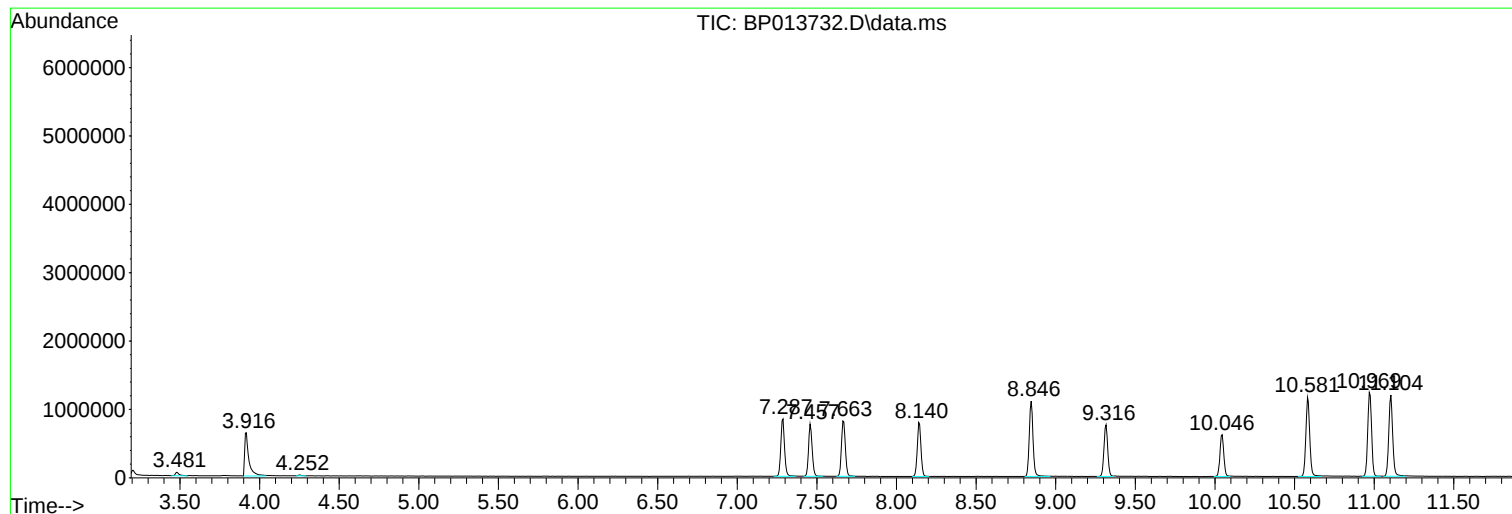

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013732.D
Acq On : 03 Feb 2023 09:31
Operator : CG/JU
Sample : PB150529BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK529

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013732.D
Acq On : 03 Feb 2023 09:31
Operator : CG/JU
Sample : PB150529BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK529

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc