

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013735.D
 Acq On : 03 Feb 2023 12:01
 Operator : CG/JU
 Sample : 01316-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44H8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.481	46	50	61	rVB	39843	66608	0.53%	0.080%
2	3.917	122	124	143	rBV	196917	378066	3.00%	0.452%
3	4.158	160	165	172	rVB2	17905	32669	0.26%	0.039%
4	4.252	175	181	186	rBV2	13862	25165	0.20%	0.030%
5	5.205	338	343	353	rVB2	16690	29806	0.24%	0.036%
6	7.287	690	697	710	rVB	204485	349172	2.77%	0.418%
7	7.458	719	726	741	rBV	818818	1310460	10.39%	1.568%
8	7.669	755	762	774	rBV	706593	1199365	9.51%	1.435%
9	8.140	834	842	853	rBV	709192	1181081	9.37%	1.413%
10	8.846	954	962	982	rBV	654349	1107990	8.79%	1.326%
11	9.316	1035	1042	1054	rBV	816500	1398152	11.09%	1.673%
12	9.716	1104	1110	1115	rVV2	15839	23892	0.19%	0.029%
13	10.046	1156	1166	1177	rBV	650896	1123447	8.91%	1.344%
14	10.581	1249	1257	1273	rBV	1220694	2083114	16.52%	2.493%
15	10.969	1313	1323	1332	rBV	1109198	1879026	14.90%	2.249%
16	11.104	1338	1346	1366	rBV	1105128	1972940	15.65%	2.361%
17	12.551	1585	1592	1604	rBV3	26483	65045	0.52%	0.078%
18	13.592	1762	1769	1773	rBV3	17228	26427	0.21%	0.032%
19	14.181	1859	1869	1884	rBV	3073617	4101093	32.53%	4.908%
20	14.475	1911	1919	1933	rBV	3161774	4701639	37.29%	5.626%
21	14.657	1946	1950	1956	rVB5	9001	13293	0.11%	0.016%
22	14.716	1956	1960	1964	rBV	10847	16970	0.13%	0.020%
23	14.781	1964	1971	1979	rVB	1996864	2981339	23.65%	3.568%
24	14.963	1995	2002	2016	rBV2	139442	298127	2.36%	0.357%
25	15.181	2034	2039	2044	rVB9	11944	22369	0.18%	0.027%
26	15.769	2130	2139	2151	rBV	4502799	6622935	52.53%	7.925%
27	15.881	2151	2158	2170	rVV	1042472	1387081	11.00%	1.660%
28	16.010	2175	2180	2186	rVB4	21574	36787	0.29%	0.044%
29	16.134	2195	2201	2211	rVB	172473	249737	1.98%	0.299%
30	16.992	2343	2347	2352	rBV8	10112	15231	0.12%	0.018%
31	17.204	2381	2383	2390	rVB8	8685	16796	0.13%	0.020%
32	17.275	2390	2395	2399	rBV5	14807	22132	0.18%	0.026%
33	17.533	2432	2439	2449	rBV	2955520	4122529	32.70%	4.933%
34	17.633	2449	2456	2466	rVV	5884242	8299171	65.83%	9.931%
35	17.704	2466	2468	2472	rVB2	23663	31412	0.25%	0.038%
36	18.169	2544	2547	2552	rBV4	24527	35199	0.28%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013735.D
 Acq On : 03 Feb 2023 12:01
 Operator : CG/JU
 Sample : 01316-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44H8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	18.216	2552	2555	2561	rVB6	17711	20765	0.16%	0.025%
38	18.386	2579	2584	2594	rBV	192025	266202	2.11%	0.319%
39	18.463	2594	2597	2600	rVV2	11552	16361	0.13%	0.020%
40	19.210	2721	2724	2728	rBV5	45400	71049	0.56%	0.085%
41	19.427	2757	2761	2766	rBV	91457	123494	0.98%	0.148%
42	19.498	2769	2773	2782	rVB	90857	145563	1.15%	0.174%
43	19.610	2788	2792	2800	rBV	93962	135044	1.07%	0.162%
44	19.851	2827	2833	2850	rBV	8418321	11364892	90.15%	13.600%
45	21.280	3073	3076	3085	rBV2	272788	452062	3.59%	0.541%
46	21.610	3127	3132	3142	rBV	4063274	5362073	42.53%	6.417%
47	24.027	3535	3543	3556	rVB2	5986050	12607054	100.00%	15.086%
48	24.192	3564	3571	3582	rVB2	2713296	5775515	45.81%	6.911%




Sum of corrected areas: 83566339

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013735.D
Acq On : 03 Feb 2023 12:01
Operator : CG/JU
Sample : 01316-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44H8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

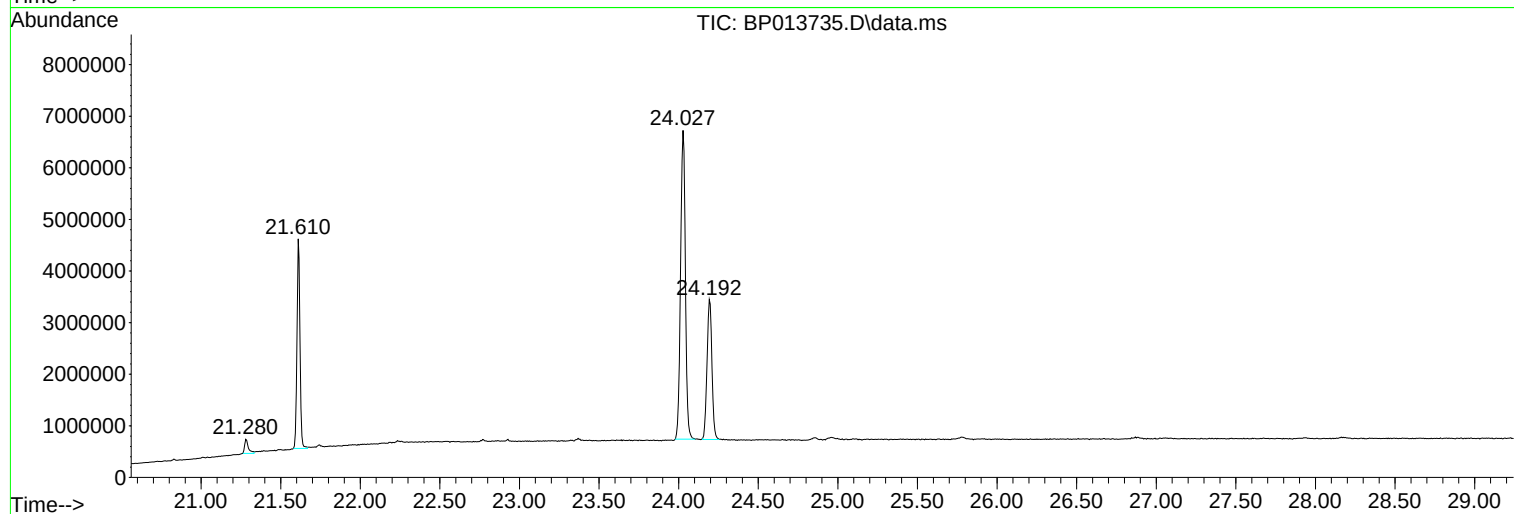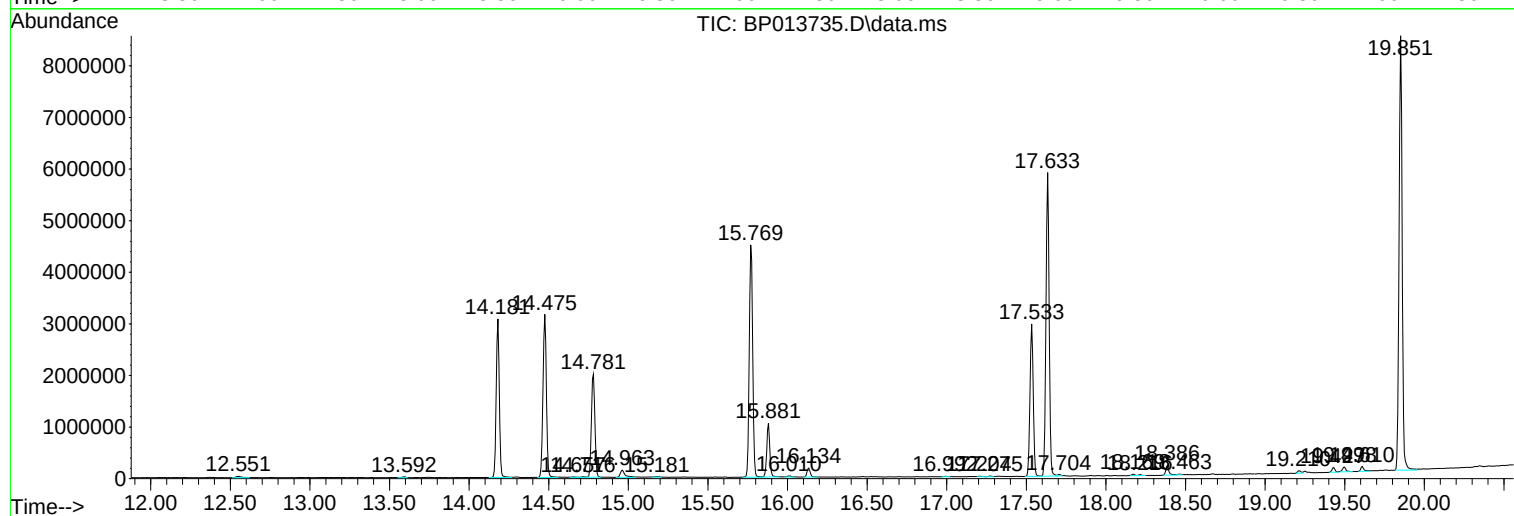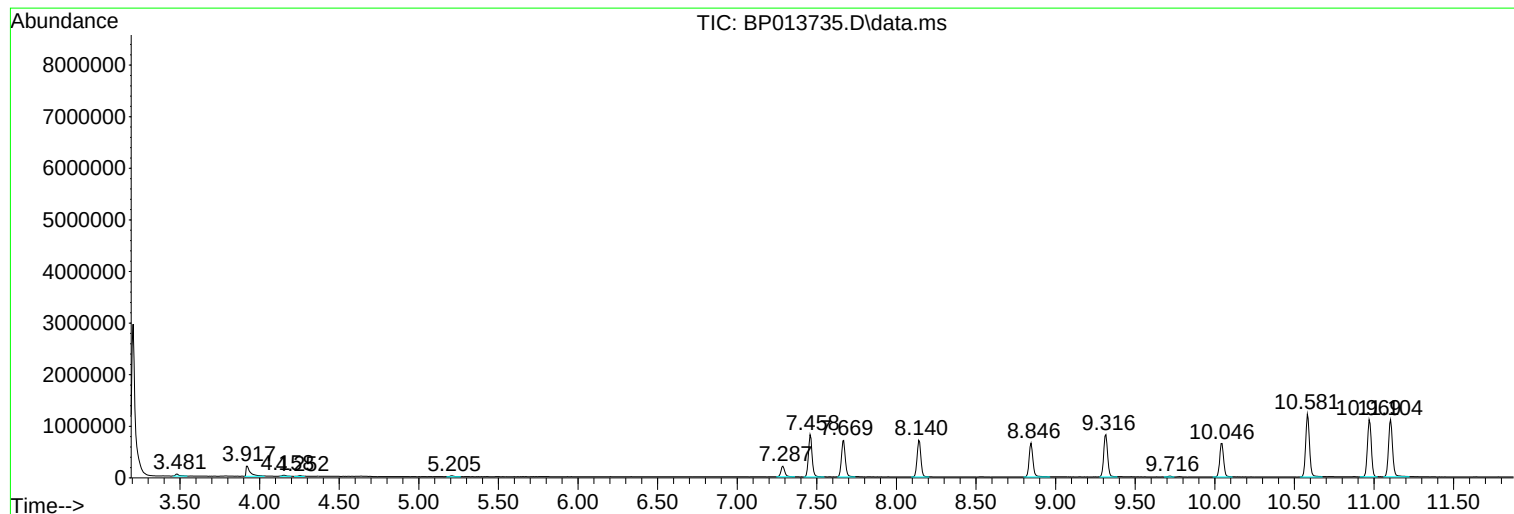

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013735.D
Acq On : 03 Feb 2023 12:01
Operator : CG/JU
Sample : 01316-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44H8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013735.D
Acq On : 03 Feb 2023 12:01
Operator : CG/JU
Sample : 01316-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44H8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------