

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013742.D
 Acq On : 03 Feb 2023 16:06
 Operator : CG/JU
 Sample : PB150621BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	56	rBV	53838	79432	0.91%	0.110%
2	3.770	96	99	104	rBV6	5128	11524	0.13%	0.016%
3	3.911	120	123	145	rBV	705730	1193815	13.74%	1.655%
4	4.252	176	181	186	rVB	10950	15606	0.18%	0.022%
5	7.281	688	696	709	rBV	895190	1469715	16.92%	2.037%
6	7.452	719	725	741	rVB	764514	1242062	14.30%	1.721%
7	7.663	752	761	775	rBV	873170	1466433	16.88%	2.032%
8	8.134	834	841	853	rBV	674915	1137766	13.10%	1.577%
9	8.840	954	961	975	rBV	1141269	1902832	21.90%	2.637%
10	9.310	1033	1041	1052	rBV	799940	1316667	15.16%	1.825%
11	10.034	1157	1164	1180	rBV	631248	1100640	12.67%	1.525%
12	10.575	1248	1256	1275	rBV	1166641	1990360	22.91%	2.759%
13	10.963	1315	1322	1337	rBV	1016545	1753952	20.19%	2.431%
14	11.099	1337	1345	1363	rBV	1161954	2055654	23.66%	2.849%
15	12.540	1585	1590	1597	rBV2	20026	37296	0.43%	0.052%
16	13.657	1773	1780	1787	rBV2	23607	42707	0.49%	0.059%
17	14.175	1860	1868	1880	rBV	2387295	3440365	39.60%	4.768%
18	14.469	1909	1918	1935	rBV	2660349	3978519	45.80%	5.514%
19	14.769	1962	1969	1979	rBV	1854598	2817761	32.44%	3.905%
20	14.951	1993	2000	2017	rBV	758681	1260932	14.51%	1.748%
21	15.763	2128	2138	2150	rBV	3771820	5474087	63.01%	7.587%
22	15.869	2150	2156	2171	rVV	825373	1194653	13.75%	1.656%
23	16.004	2175	2179	2185	rVB3	18481	30487	0.35%	0.042%
24	17.528	2431	2438	2448	rBV	2617481	3826931	44.05%	5.304%
25	17.622	2448	2454	2469	rVV	4389237	6319611	72.75%	8.759%
26	19.416	2756	2759	2766	rBV	56471	75948	0.87%	0.105%
27	19.486	2768	2771	2777	rVB	54020	74523	0.86%	0.103%
28	19.839	2825	2831	2846	rBV	6111514	8464604	97.44%	11.731%
29	21.604	3126	3131	3141	rBV	3518771	4748312	54.66%	6.581%
30	24.010	3533	3540	3552	rVB2	4194708	8687241	100.00%	12.040%
31	24.174	3562	3568	3580	rVB2	2328827	4942699	56.90%	6.850%




Sum of corrected areas: 72153134

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013742.D
Acq On : 03 Feb 2023 16:06
Operator : CG/JU
Sample : PB150621BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

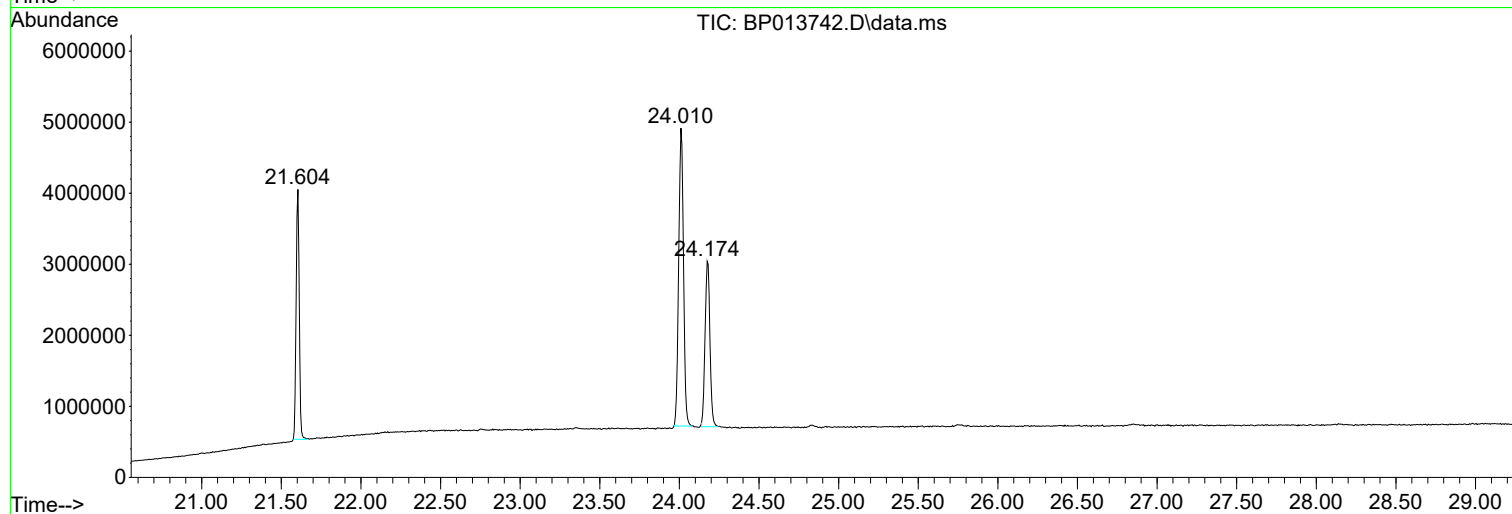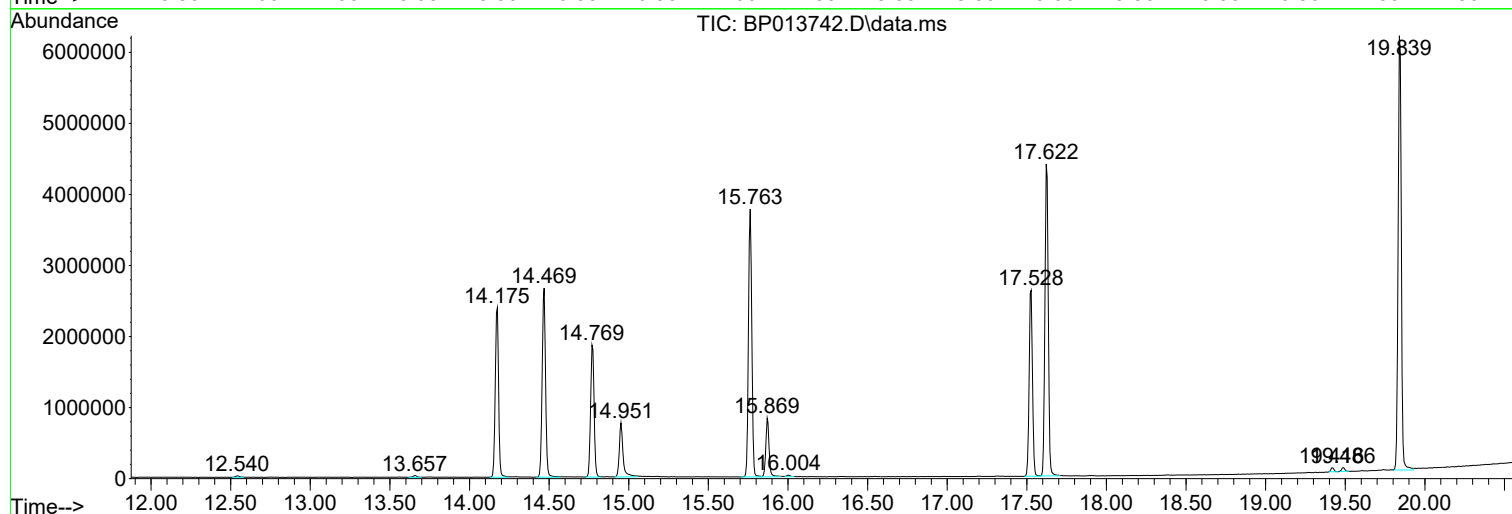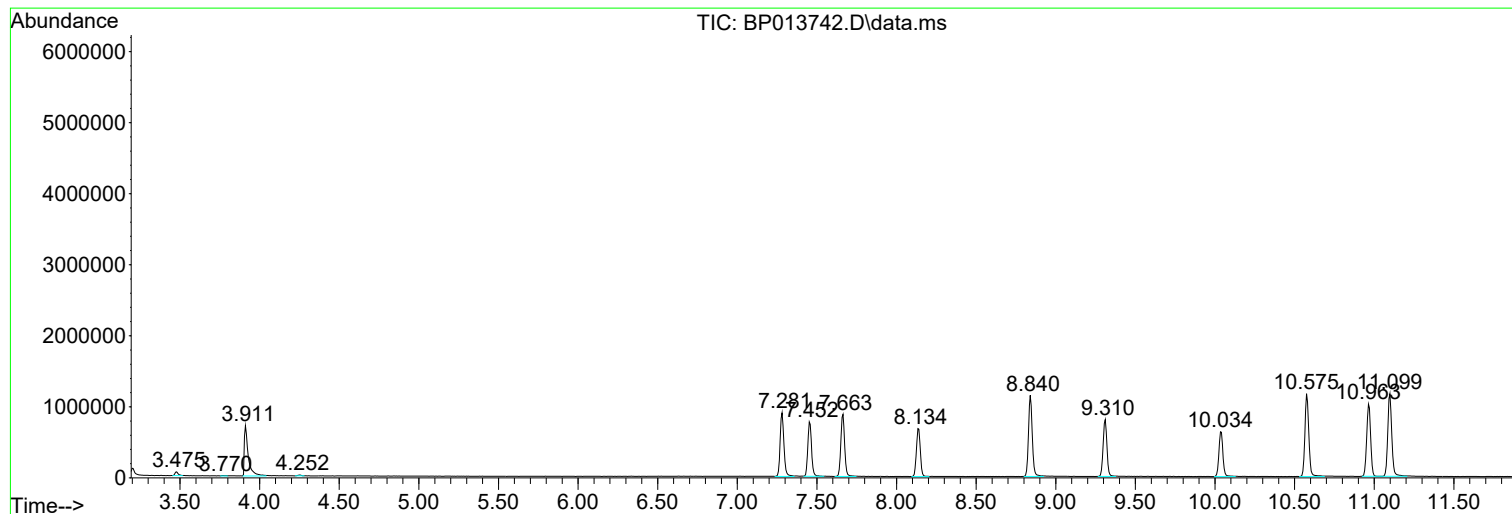

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013742.D
Acq On : 03 Feb 2023 16:06
Operator : CG/JU
Sample : PB150621BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013742.D
Acq On : 03 Feb 2023 16:06
Operator : CG/JU
Sample : PB150621BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc