

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013748.D
 Acq On : 03 Feb 2023 19:31
 Operator : CG/JU
 Sample : 01381-21
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	38	43	63	rVB	963189	1759809	14.76%	1.787%
2	3.917	122	124	137	rBV	158794	284604	2.39%	0.289%
3	4.146	158	163	168	rBV	16414	25986	0.22%	0.026%
4	4.246	176	180	187	rBV2	15492	26039	0.22%	0.026%
5	4.817	273	277	284	rVB4	8154	14319	0.12%	0.015%
6	5.199	337	342	349	rVB	40514	62929	0.53%	0.064%
7	5.405	370	377	394	rVB	1369790	2169638	18.20%	2.203%
8	7.275	689	695	705	rVB	189762	306478	2.57%	0.311%
9	7.446	718	724	739	rVB	845191	1381954	11.59%	1.403%
10	7.658	753	760	770	rBV	682293	1146909	9.62%	1.165%
11	7.852	788	793	799	rVB	10702	18765	0.16%	0.019%
12	8.017	815	821	829	rBV	266414	429677	3.60%	0.436%
13	8.128	832	840	844	rBV	731978	1294200	10.86%	1.314%
14	8.164	844	846	855	rVB	617680	904143	7.58%	0.918%
15	8.487	892	901	914	rBV	2120144	3519206	29.52%	3.573%
16	8.834	952	960	971	rBV	575281	950017	7.97%	0.965%
17	9.305	1031	1040	1043	rBV	807506	1418110	11.90%	1.440%
18	9.352	1043	1048	1064	rVB	5680653	9628603	80.77%	9.777%
19	9.705	1102	1108	1114	rVB3	14239	24585	0.21%	0.025%
20	9.775	1114	1120	1127	rBV8	8699	17859	0.15%	0.018%
21	10.028	1155	1163	1182	rBV	695716	1169416	9.81%	1.187%
22	10.487	1234	1241	1248	rBV	38395	65367	0.55%	0.066%
23	10.569	1248	1255	1268	rBV	1142374	1940002	16.27%	1.970%
24	10.816	1291	1297	1303	rBV	99573	162233	1.36%	0.165%
25	10.958	1313	1321	1330	rBV	1109861	1851658	15.53%	1.880%
26	11.093	1337	1344	1358	rBV	640738	1163421	9.76%	1.181%
27	11.346	1380	1387	1395	rVB2	26425	46904	0.39%	0.048%
28	12.087	1508	1513	1520	rBV7	15912	33858	0.28%	0.034%
29	12.475	1573	1579	1584	rBV2	11505	18330	0.15%	0.019%
30	12.534	1584	1589	1598	rVV2	23288	42998	0.36%	0.044%
31	12.728	1616	1622	1624	rBV7	5954	12875	0.11%	0.013%
32	12.981	1661	1665	1672	rVB7	6548	12915	0.11%	0.013%
33	13.593	1758	1769	1772	rBV9	13559	34767	0.29%	0.035%
34	13.646	1772	1778	1785	rVB2	38457	80788	0.68%	0.082%
35	14.169	1859	1867	1881	rBV	2573580	3663440	30.73%	3.720%
36	14.287	1884	1887	1894	rVB9	8779	14886	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013748.D
 Acq On : 03 Feb 2023 19:31
 Operator : CG/JU
 Sample : 01381-21
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	14.463	1910	1917	1929	rVV	2779439	4253206	35.68%	4.319%
38	14.763	1960	1968	1979	rBV	1857903	2882663	24.18%	2.927%
39	14.946	1993	1999	2012	rBV	158181	311405	2.61%	0.316%
40	15.163	2032	2036	2042	rVB8	14032	24704	0.21%	0.025%
41	15.493	2087	2092	2097	rBV8	7605	12284	0.10%	0.012%
42	15.757	2130	2137	2149	rBV	4373695	6220205	52.18%	6.316%
43	15.863	2149	2155	2169	rVV	1081673	1558667	13.07%	1.583%
44	15.998	2173	2178	2185	rVB2	21822	34734	0.29%	0.035%
45	16.116	2193	2198	2209	rVB	99592	148952	1.25%	0.151%
46	16.887	2326	2329	2335	rBV8	7463	12042	0.10%	0.012%
47	17.192	2379	2381	2389	rVB7	9845	14048	0.12%	0.014%
48	17.522	2430	2437	2446	rBV	2922033	4131625	34.66%	4.195%
49	17.622	2447	2454	2465	rBV	5307447	7828036	65.66%	7.948%
50	17.887	2495	2499	2503	rBV5	16257	24499	0.21%	0.025%
51	18.369	2576	2581	2589	rBV	142333	211248	1.77%	0.214%
52	18.781	2648	2651	2655	rBV	74069	78656	0.66%	0.080%
53	19.198	2717	2722	2728	rBV	199801	309885	2.60%	0.315%
54	19.416	2755	2759	2763	rVB	85715	107351	0.90%	0.109%
55	19.481	2766	2770	2774	rBV	95593	124088	1.04%	0.126%
56	19.592	2786	2789	2795	rBV	74092	106291	0.89%	0.108%
57	19.839	2825	2831	2840	rBV	7942726	10678365	89.57%	10.842%
58	21.269	3071	3074	3080	rBV	177103	222897	1.87%	0.226%
59	21.598	3125	3130	3138	rBV	4025954	5334941	44.75%	5.417%
60	22.904	3348	3352	3361	rVB	352402	551402	4.63%	0.560%
61	24.004	3531	3539	3557	rVB2	5477707	11921431	100.00%	12.105%
62	24.169	3560	3567	3577	rVB2	2669942	5685068	47.69%	5.772%




Sum of corrected areas: 98486381

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013748.D
Acq On : 03 Feb 2023 19:31
Operator : CG/JU
Sample : 01381-21
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

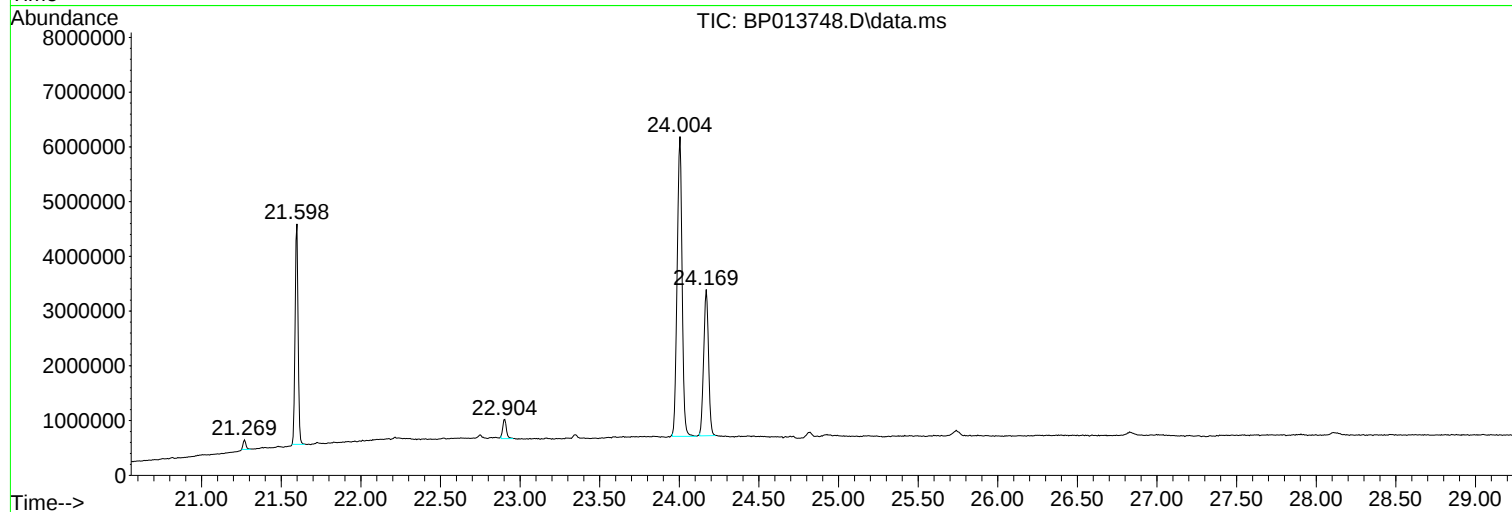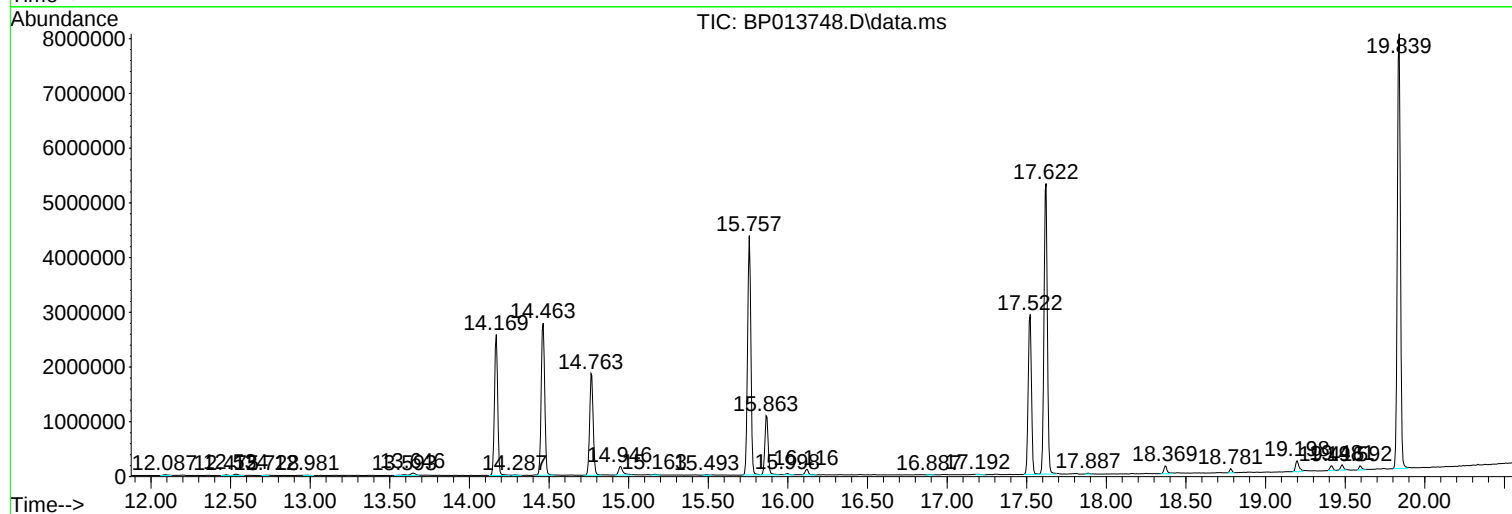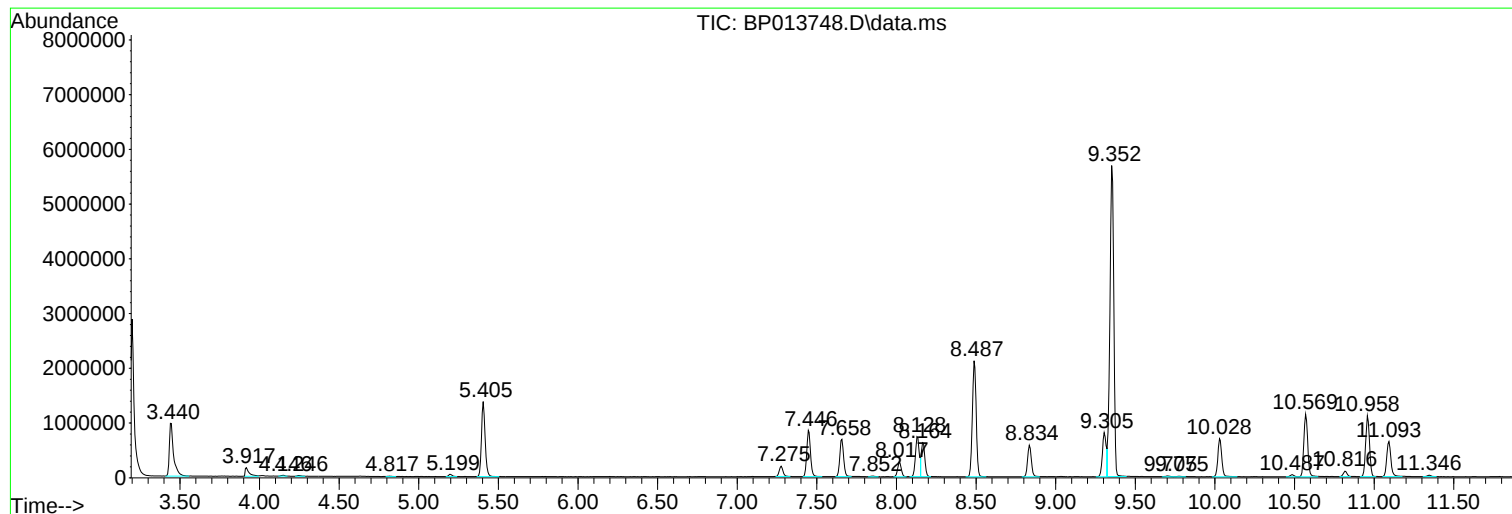

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013748.D
Acq On : 03 Feb 2023 19:31
Operator : CG/JU
Sample : 01381-21
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013748.D
Acq On : 03 Feb 2023 19:31
Operator : CG/JU
Sample : 01381-21
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc