

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013755.D
 Acq On : 03 Feb 2023 23:29
 Operator : CG/JU
 Sample : 01381-20
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.446	39	44	47	rBV	236048	360207	2.49%	0.369%
2	3.916	122	124	137	rBV	150056	270378	1.87%	0.277%
3	4.146	159	163	172	rVB	24460	40258	0.28%	0.041%
4	4.246	176	180	190	rVB	16049	31097	0.22%	0.032%
5	5.199	337	342	348	rBV	37706	58373	0.40%	0.060%
6	7.275	686	695	711	rVB	229256	383972	2.66%	0.394%
7	7.446	717	724	736	rBV	925038	1508435	10.43%	1.546%
8	7.657	752	760	769	rBV	827923	1389979	9.61%	1.425%
9	8.128	833	840	855	rBV	890520	1469736	10.17%	1.506%
10	8.493	896	902	906	rBV2	11492	22062	0.15%	0.023%
11	8.834	953	960	971	rBV	740709	1227633	8.49%	1.258%
12	9.304	1032	1040	1053	rBV	1017605	1749744	12.10%	1.793%
13	9.704	1101	1108	1113	rVB6	8607	14802	0.10%	0.015%
14	9.787	1115	1122	1127	rBV8	7572	18599	0.13%	0.019%
15	10.028	1155	1163	1179	rBV	810945	1383807	9.57%	1.418%
16	10.569	1247	1255	1276	rBV	1471356	2524373	17.46%	2.587%
17	10.957	1311	1321	1333	rBV	1399819	2341299	16.20%	2.400%
18	11.093	1336	1344	1363	rBV	721188	1307550	9.04%	1.340%
19	12.534	1582	1589	1600	rBV2	28971	52546	0.36%	0.054%
20	13.651	1774	1779	1786	rBV	34187	50332	0.35%	0.052%
21	14.169	1860	1867	1883	rBV	3479881	4946428	34.22%	5.069%
22	14.463	1909	1917	1937	rBV	3749753	5616925	38.85%	5.757%
23	14.763	1961	1968	1979	rBV	2401445	3678322	25.44%	3.770%
24	14.945	1993	1999	2011	rBV	196770	376019	2.60%	0.385%
25	15.110	2023	2027	2032	rVV7	9386	16615	0.11%	0.017%
26	15.169	2033	2037	2045	rVB10	12269	22964	0.16%	0.024%
27	15.492	2086	2092	2099	rBV	10672	19961	0.14%	0.020%
28	15.757	2130	2137	2149	rBV	5707911	8030929	55.55%	8.231%
29	15.863	2149	2155	2168	rVB	1461340	2015473	13.94%	2.066%
30	15.998	2173	2178	2184	rVB2	27678	48547	0.34%	0.050%
31	16.316	2229	2232	2239	rVB9	7608	15657	0.11%	0.016%
32	17.304	2395	2400	2409	rBV4	8546	20934	0.14%	0.021%
33	17.516	2430	2436	2446	rBV	3460141	5086470	35.18%	5.213%
34	17.616	2447	2453	2469	rVV	6806639	9835720	68.04%	10.080%
35	18.369	2577	2581	2587	rBV3	47925	72801	0.50%	0.075%
36	18.445	2590	2594	2600	rVB	67098	95983	0.66%	0.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013755.D
Acq On : 03 Feb 2023 23:29
Operator : CG/JU
Sample : 01381-20
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44N5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Title : SVOA CALIBRATION

37	19.410	2754	2758	2764	rBV2	117164	166659	1.15%	0.171%
38	19.480	2766	2770	2780	rVB	109240	173444	1.20%	0.178%
39	19.592	2786	2789	2794	rBV4	44918	54672	0.38%	0.056%
40	19.839	2824	2831	2844	rBV	9730684	13432076	92.91%	13.766%
41	21.592	3124	3129	3138	rBV	4501532	6430282	44.48%	6.590%
42	23.998	3530	3538	3556	rVB2	6675606	14456531	100.00%	14.816%
43	24.162	3559	3566	3580	rVB2	3091385	6755352	46.73%	6.923%




Sum of corrected areas: 97573946

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013755.D
Acq On : 03 Feb 2023 23:29
Operator : CG/JU
Sample : 01381-20
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

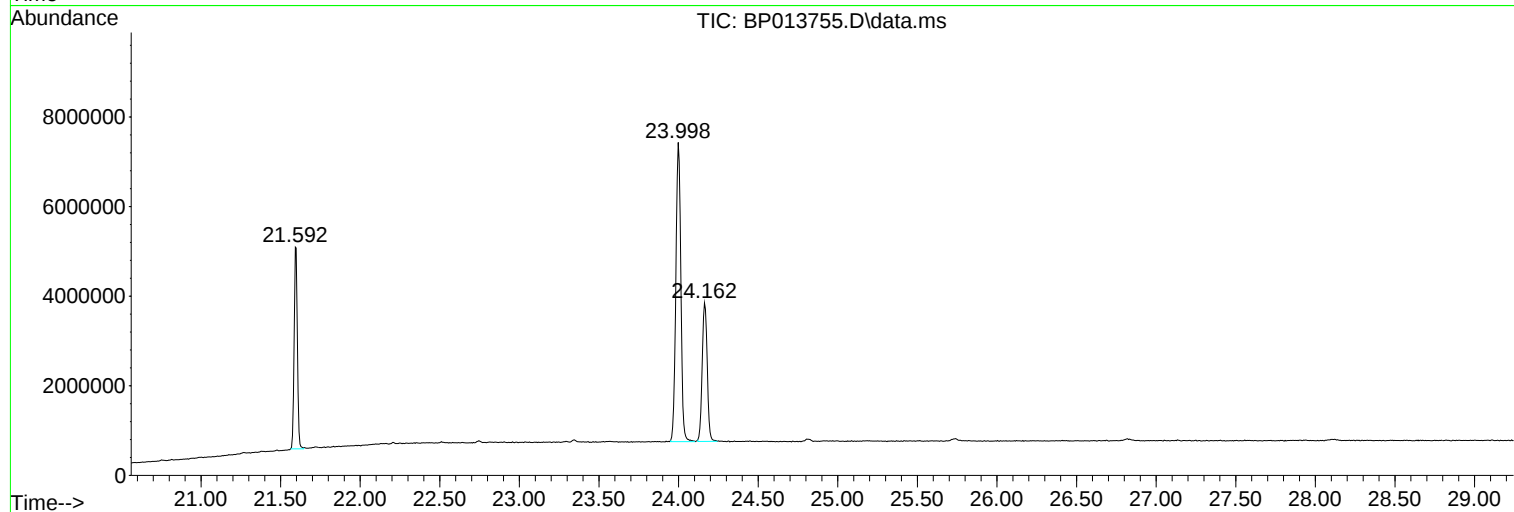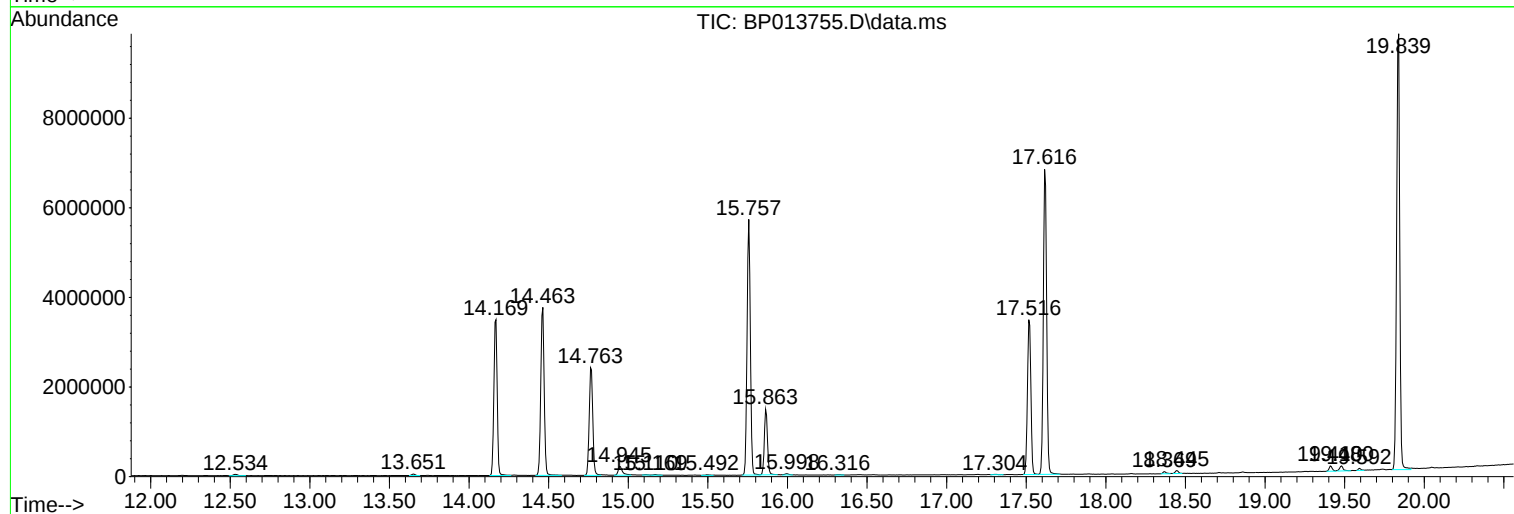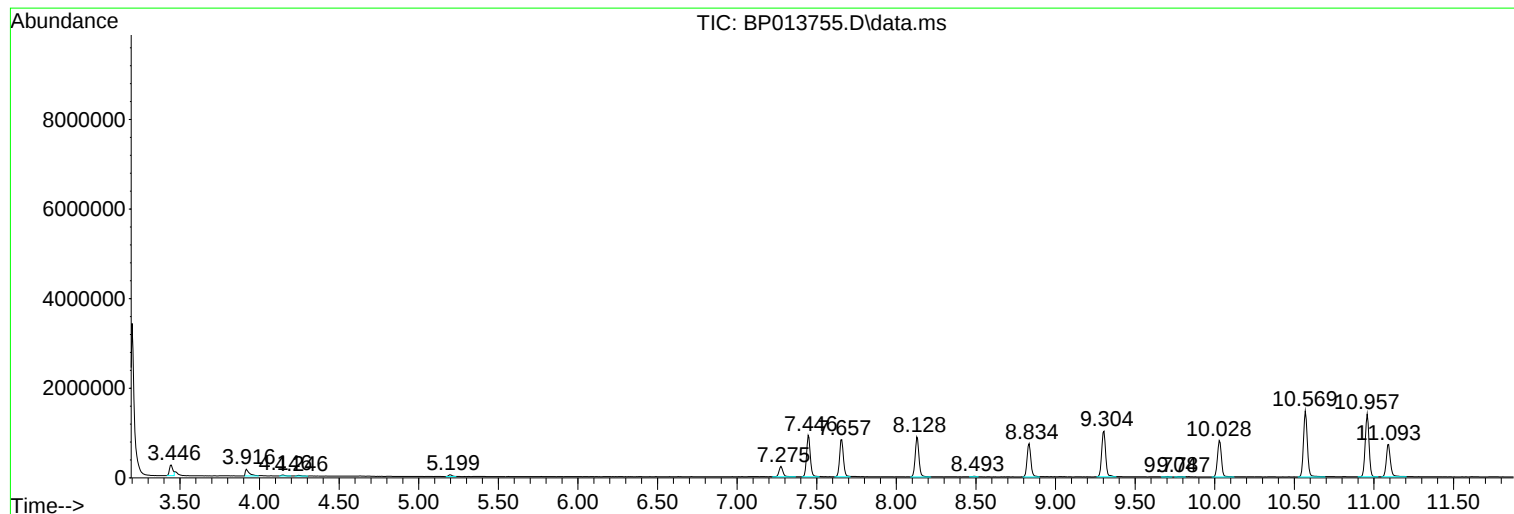

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013755.D
Acq On : 03 Feb 2023 23:29
Operator : CG/JU
Sample : 01381-20
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013755.D
Acq On : 03 Feb 2023 23:29
Operator : CG/JU
Sample : 01381-20
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc