

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013756.D
 Acq On : 04 Feb 2023 00:03
 Operator : CG/JU
 Sample : 01381-09
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	56	rBV	40915	58609	0.53%	0.070%
2	3.916	122	124	143	rBV	111438	202269	1.81%	0.243%
3	4.146	159	163	171	rVB	23545	39982	0.36%	0.048%
4	4.246	176	180	185	rVB	22068	30089	0.27%	0.036%
5	5.199	336	342	352	rBV	49565	84058	0.75%	0.101%
6	7.275	684	695	710	rVB	176002	320328	2.87%	0.384%
7	7.446	718	724	735	rBV	849009	1337070	11.98%	1.604%
8	7.657	753	760	771	rBV	715056	1194036	10.70%	1.433%
9	8.128	832	840	848	rBV	813943	1317896	11.81%	1.581%
10	8.493	891	902	905	rBV9	5880	13376	0.12%	0.016%
11	8.834	953	960	975	rBV	578984	962193	8.62%	1.154%
12	9.298	1032	1039	1051	rBV	896337	1553148	13.92%	1.864%
13	9.457	1060	1066	1071	rVB8	9705	15617	0.14%	0.019%
14	9.704	1101	1108	1113	rBV	25802	40639	0.36%	0.049%
15	10.028	1155	1163	1177	rBV	739679	1243714	11.14%	1.492%
16	10.569	1247	1255	1273	rBV	1261461	2110828	18.91%	2.533%
17	10.957	1313	1321	1328	rBV	1271694	2123790	19.03%	2.548%
18	11.092	1336	1344	1354	rBV	764680	1398524	12.53%	1.678%
19	11.734	1448	1453	1459	rBV10	5291	12012	0.11%	0.014%
20	12.198	1526	1532	1536	rBV2	38712	78331	0.70%	0.094%
21	12.534	1583	1589	1594	rVB2	26239	41937	0.38%	0.050%
22	13.045	1670	1676	1682	rBV4	10024	16057	0.14%	0.019%
23	13.651	1774	1779	1783	rVB	30726	43815	0.39%	0.053%
24	14.163	1860	1866	1881	rBV	2885676	4177963	37.43%	5.013%
25	14.457	1910	1916	1928	rVV2	3281344	4864237	43.58%	5.836%
26	14.763	1961	1968	1978	rBV	2272311	3606139	32.31%	4.327%
27	14.833	1978	1980	1993	rVB4	26255	45981	0.41%	0.055%
28	14.945	1993	1999	2015	rBV	120178	244904	2.19%	0.294%
29	15.175	2033	2038	2042	rVB8	8831	16913	0.15%	0.020%
30	15.433	2077	2082	2086	rBV3	9560	15014	0.13%	0.018%
31	15.757	2126	2137	2149	rBV	4675266	6825150	61.15%	8.189%
32	15.863	2149	2155	2173	rVV	1055527	1497923	13.42%	1.797%
33	15.992	2173	2177	2185	rVB4	21248	36282	0.33%	0.044%
34	17.098	2362	2365	2370	rVB4	8748	12258	0.11%	0.015%
35	17.192	2376	2381	2387	rBV9	9221	15474	0.14%	0.019%
36	17.304	2396	2400	2409	rBV4	8081	18231	0.16%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013756.D
 Acq On : 04 Feb 2023 00:03
 Operator : CG/JU
 Sample : 01381-09
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44K1

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	17.516	2429	2436	2446	rBV	3283411	4767318	42.71%	5.720%
38	17.616	2446	2453	2466	rBV	5635066	8179733	73.28%	9.814%
39	17.886	2497	2499	2505	rVB5	10438	14580	0.13%	0.017%
40	18.163	2541	2546	2555	rBV	219226	276602	2.48%	0.332%
41	18.369	2576	2581	2589	rBV2	75248	114488	1.03%	0.137%
42	19.410	2754	2758	2763	rBV	85344	121103	1.08%	0.145%
43	19.480	2766	2770	2774	rVV	77002	103420	0.93%	0.124%
44	19.592	2786	2789	2794	rBV4	64153	81930	0.73%	0.098%
45	19.833	2824	2830	2845	rBV	8102424	10802706	96.78%	12.962%
46	21.592	3124	3129	3138	rBV	4345701	5985252	53.62%	7.181%
47	23.998	3530	3538	3553	rVB2	5201443	11161589	100.00%	13.392%
48	24.162	3559	3566	3579	rVB2	2815418	6120932	54.84%	7.344%




Sum of corrected areas: 83344440

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013756.D
Acq On : 04 Feb 2023 00:03
Operator : CG/JU
Sample : 01381-09
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

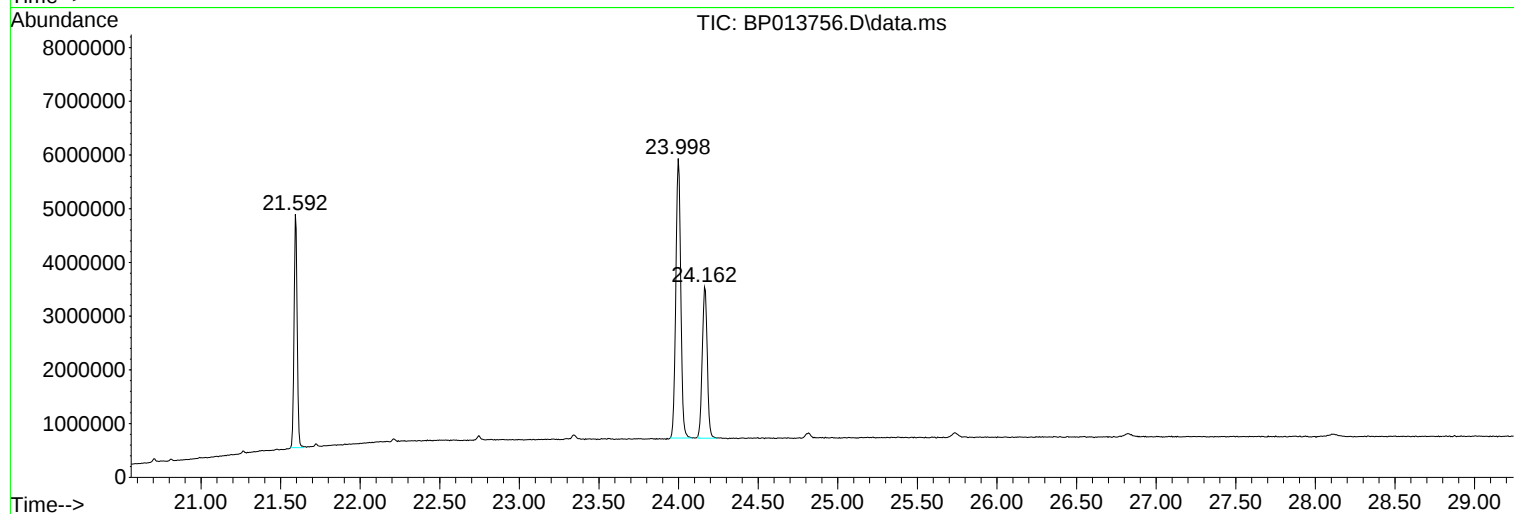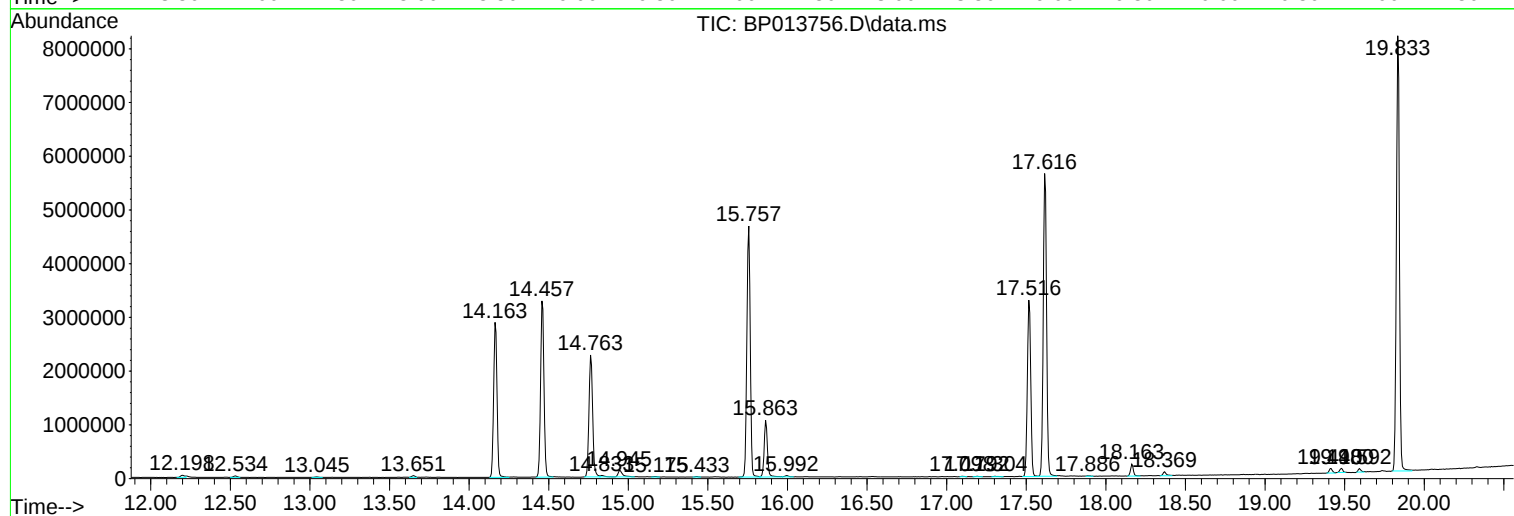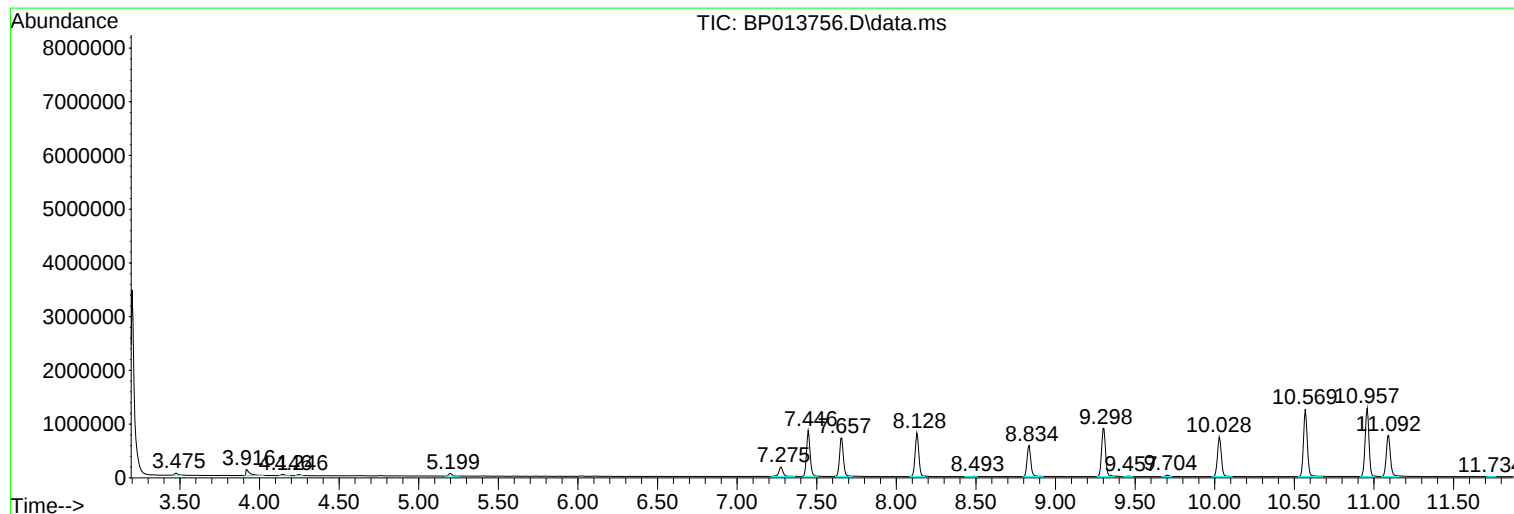

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013756.D
Acq On : 04 Feb 2023 00:03
Operator : CG/JU
Sample : 01381-09
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013756.D
Acq On : 04 Feb 2023 00:03
Operator : CG/JU
Sample : 01381-09
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc