

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013757.D
 Acq On : 04 Feb 2023 00:37
 Operator : CG/JU
 Sample : 01314-23
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	57	rVB	32497	47320	0.44%	0.059%
2	3.916	122	124	141	rBV	179101	337566	3.13%	0.418%
3	4.146	159	163	168	rVB	17342	27395	0.25%	0.034%
4	4.246	176	180	183	rBV	14648	22373	0.21%	0.028%
5	4.275	183	185	193	rVB7	8582	12967	0.12%	0.016%
6	6.999	643	648	655	rVB	12202	20748	0.19%	0.026%
7	7.275	689	695	707	rVB	151473	260292	2.41%	0.322%
8	7.446	717	724	736	rBV	744925	1220600	11.31%	1.511%
9	7.652	753	759	771	rBV	627387	1080714	10.02%	1.338%
10	8.128	832	840	850	rBV	886980	1463370	13.56%	1.812%
11	8.834	952	960	973	rBV	515938	863961	8.01%	1.070%
12	9.304	1032	1040	1052	rBV	803706	1383768	12.82%	1.713%
13	9.675	1097	1103	1104	rBV4	8272	14864	0.14%	0.018%
14	9.698	1104	1107	1113	rVV	19917	33025	0.31%	0.041%
15	10.028	1155	1163	1177	rBV	653360	1100249	10.20%	1.362%
16	10.569	1247	1255	1272	rBV	1093253	1889152	17.51%	2.339%
17	10.957	1313	1321	1330	rBV	1373944	2311401	21.42%	2.862%
18	11.093	1336	1344	1361	rBV	899213	1634629	15.15%	2.024%
19	12.534	1583	1589	1597	rBV2	21697	36132	0.33%	0.045%
20	13.581	1763	1767	1773	rVB4	8490	13259	0.12%	0.016%
21	13.651	1773	1779	1784	rBV	24343	40433	0.37%	0.050%
22	14.163	1859	1866	1881	rBV	2564383	3586944	33.24%	4.441%
23	14.281	1883	1886	1892	rVB7	6714	12211	0.11%	0.015%
24	14.392	1902	1905	1909	rBV6	11073	15711	0.15%	0.019%
25	14.463	1909	1917	1932	rVV	2827229	4269066	39.56%	5.286%
26	14.639	1944	1947	1953	rVB	11801	15840	0.15%	0.020%
27	14.710	1954	1959	1961	rBV	7926	11275	0.10%	0.014%
28	14.763	1961	1968	1979	rVV	2413763	3568303	33.07%	4.418%
29	14.945	1994	1999	2014	rBV2	85290	195955	1.82%	0.243%
30	15.386	2070	2074	2078	rBV6	13319	20074	0.19%	0.025%
31	15.757	2125	2137	2149	rBV	4271707	5990650	55.52%	7.417%
32	15.863	2149	2155	2169	rVV	939104	1302855	12.07%	1.613%
33	15.998	2173	2178	2182	rVB2	20206	32082	0.30%	0.040%
34	16.116	2192	2198	2209	rBV	139992	206116	1.91%	0.255%
35	16.686	2290	2295	2299	rBV	16994	25527	0.24%	0.032%
36	17.304	2396	2400	2405	rBV4	12282	20345	0.19%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013757.D
 Acq On : 04 Feb 2023 00:37
 Operator : CG/JU
 Sample : 01314-23
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	17.516	2430	2436	2447	rBV	3504184	5125065	47.50%	6.345%
38	17.616	2447	2453	2464	rBV	5298360	7328569	67.92%	9.074%
39	18.369	2577	2581	2587	rBV2	77612	106076	0.98%	0.131%
40	18.780	2648	2651	2654	rVB4	30178	33965	0.31%	0.042%
41	19.192	2719	2721	2724	rBV4	16792	19802	0.18%	0.025%
42	19.410	2755	2758	2763	rBV	72562	93482	0.87%	0.116%
43	19.480	2766	2770	2774	rVV	76903	100524	0.93%	0.124%
44	19.592	2786	2789	2793	rBV4	38593	47353	0.44%	0.059%
45	19.833	2824	2830	2844	rBV	7208790	9932458	92.05%	12.297%
46	21.263	3070	3073	3083	rBV3	186012	341246	3.16%	0.422%
47	21.592	3124	3129	3137	rBV	4781833	6674088	61.85%	8.263%
48	23.998	3530	3538	3553	rVB2	5051119	10790412	100.00%	13.360%
49	24.162	3559	3566	3580	rVB2	3380662	7088421	65.69%	8.776%




Sum of corrected areas: 80768633

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013757.D
Acq On : 04 Feb 2023 00:37
Operator : CG/JU
Sample : 01314-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

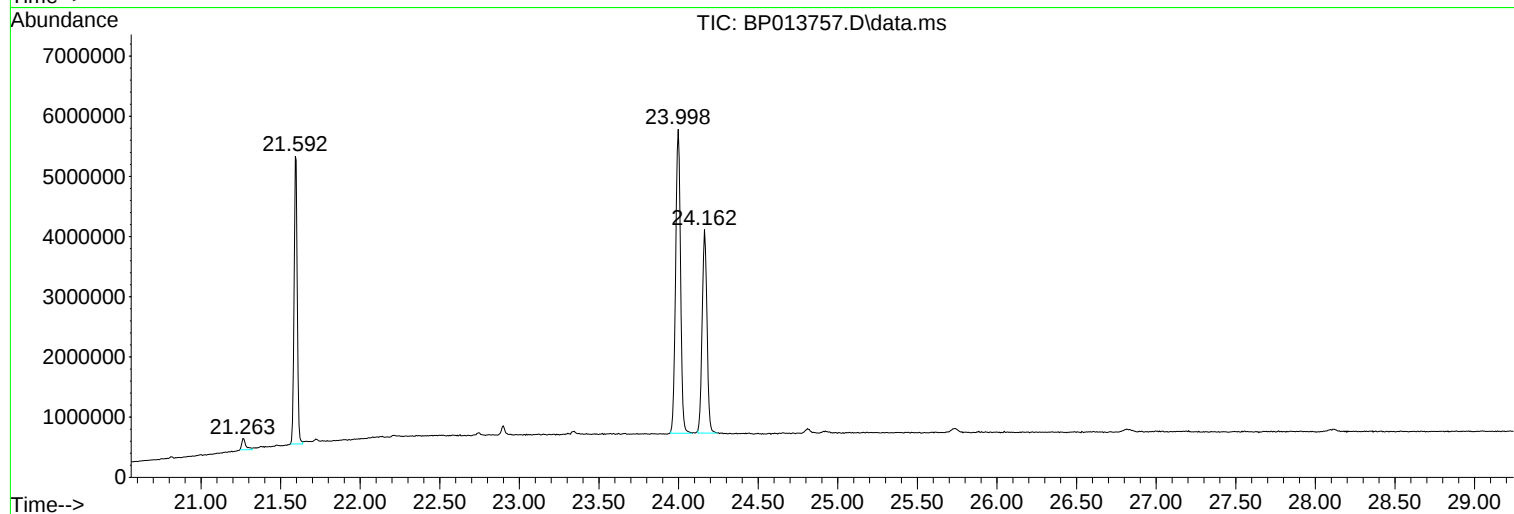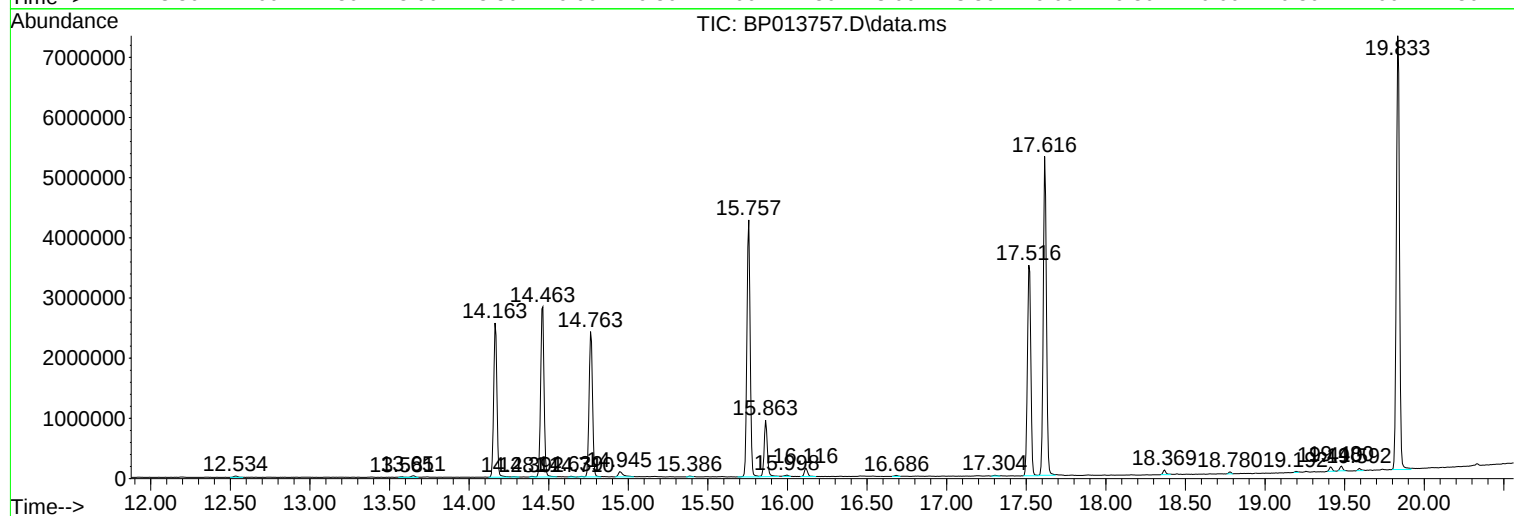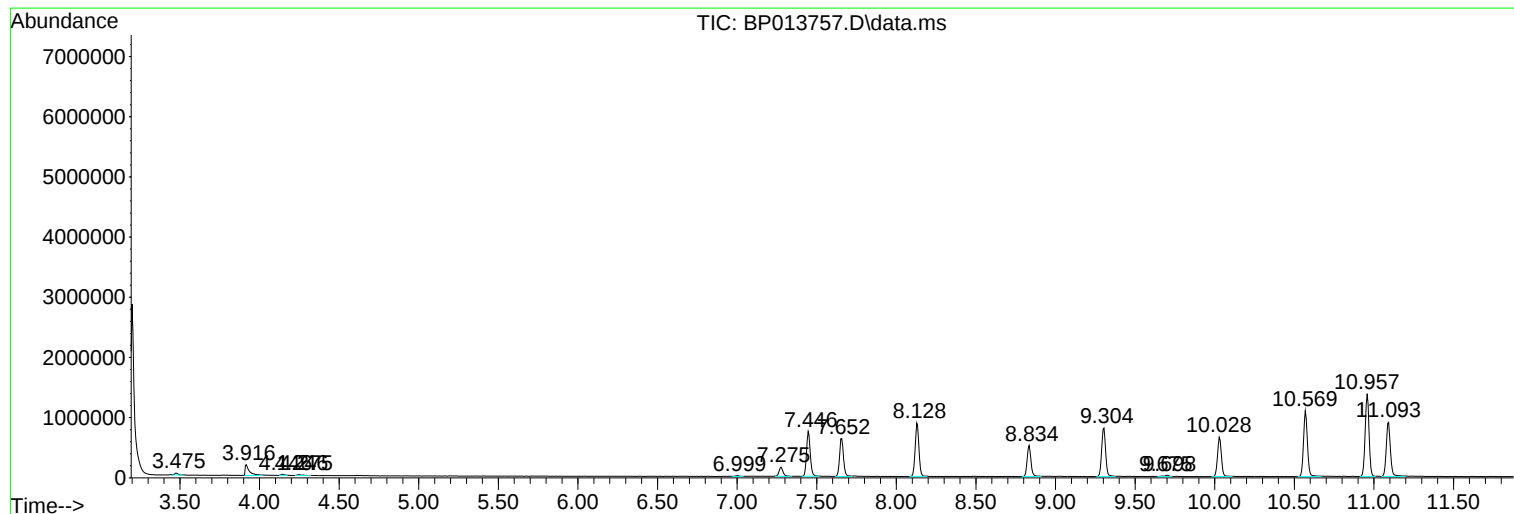

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013757.D
Acq On : 04 Feb 2023 00:37
Operator : CG/JU
Sample : 01314-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013757.D
Acq On : 04 Feb 2023 00:37
Operator : CG/JU
Sample : 01314-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc