

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013759.D
 Acq On : 04 Feb 2023 02:18
 Operator : CG/JU
 Sample : PB150620BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	56	rBV	66575	93056	0.84%	0.093%
2	3.905	119	122	149	rBV	879982	1511618	13.68%	1.514%
3	4.246	176	180	189	rVB	20755	31128	0.28%	0.031%
4	7.275	687	695	711	rBV	1143237	1851819	16.76%	1.855%
5	7.446	717	724	737	rBV	973429	1537253	13.92%	1.540%
6	7.652	751	759	773	rBV	1099509	1849832	16.75%	1.853%
7	8.128	833	840	855	rBV	1125708	1842318	16.68%	1.846%
8	8.834	951	960	974	rBV	1457430	2401741	21.74%	2.406%
9	9.304	1031	1040	1054	rBV	1045282	1750955	15.85%	1.754%
10	10.028	1154	1163	1182	rBV	895988	1482211	13.42%	1.485%
11	10.569	1248	1255	1273	rBV	1509774	2591104	23.46%	2.596%
12	10.957	1313	1321	1331	rBV	1766730	2937152	26.59%	2.943%
13	11.087	1335	1343	1359	rBV	1484217	2639253	23.89%	2.644%
14	12.534	1582	1589	1598	rBV2	26494	51122	0.46%	0.051%
15	13.651	1772	1779	1784	rBV	40043	62198	0.56%	0.062%
16	14.163	1857	1866	1881	rBV	3063982	4340141	39.29%	4.348%
17	14.457	1909	1916	1930	rBV	3455582	5217942	47.23%	5.228%
18	14.763	1961	1968	1979	rBV	3213739	4616487	41.79%	4.625%
19	14.945	1992	1999	2022	rBV	1069062	1768129	16.01%	1.771%
20	15.169	2033	2037	2045	rVB10	8867	16805	0.15%	0.017%
21	15.757	2129	2137	2149	rBV	4702176	6937814	62.80%	6.951%
22	15.863	2149	2155	2170	rVV	1132950	1543989	13.98%	1.547%
23	15.992	2173	2177	2185	rVB2	24879	43234	0.39%	0.043%
24	16.539	2264	2270	2273	rBV7	7655	12813	0.12%	0.013%
25	17.310	2396	2401	2404	rVB3	7522	12266	0.11%	0.012%
26	17.516	2429	2436	2446	rBV	4494264	6371123	57.67%	6.383%
27	17.616	2446	2453	2466	rVV	5601624	8010449	72.51%	8.026%
28	19.410	2754	2758	2763	rBV	76866	107976	0.98%	0.108%
29	19.480	2766	2770	2776	rVB	74245	105129	0.95%	0.105%
30	19.833	2824	2830	2849	rBV	7989537	10688656	96.76%	10.709%
31	21.592	3124	3129	3140	rBV	6074265	8079303	73.14%	8.095%
32	23.998	3530	3538	3551	rVB2	5168290	11046894	100.00%	11.068%
33	24.162	3559	3566	3582	rVB2	3782897	8260034	74.77%	8.276%




Sum of corrected areas: 99811944

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013759.D
Acq On : 04 Feb 2023 02:18
Operator : CG/JU
Sample : PB150620BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK620

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

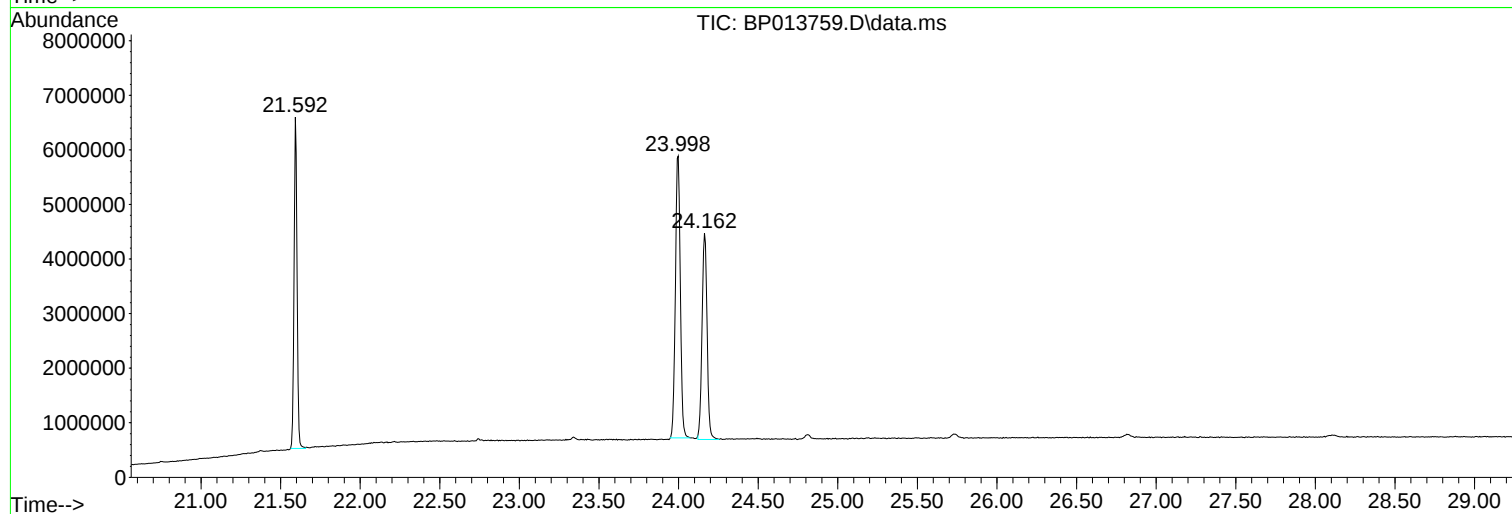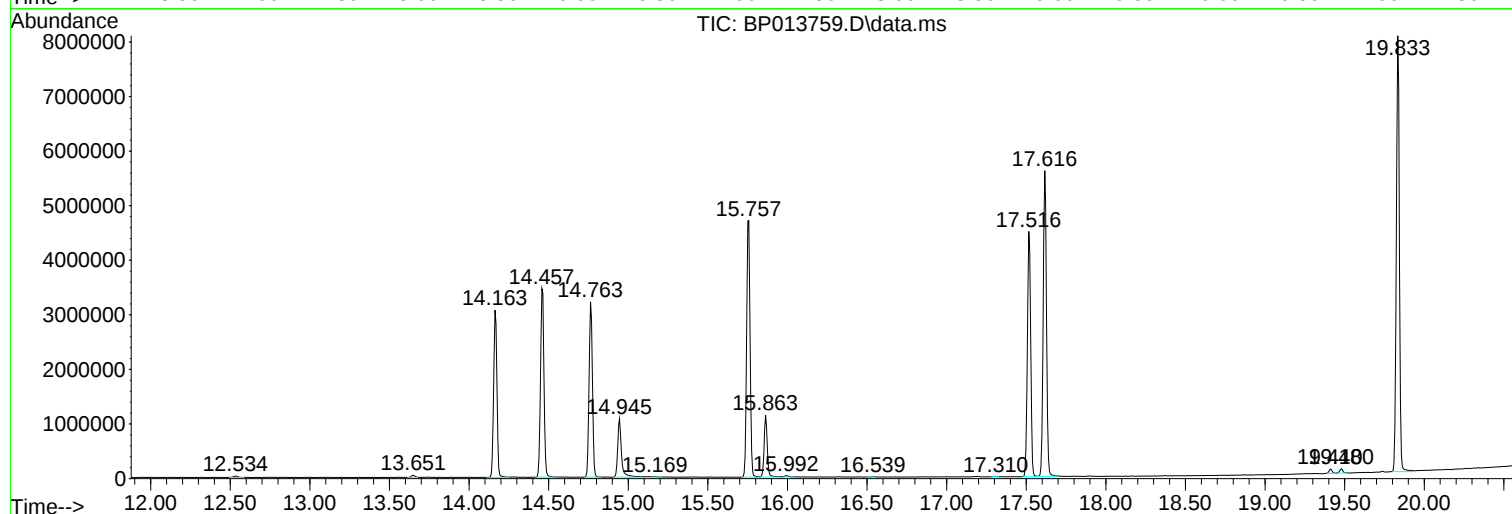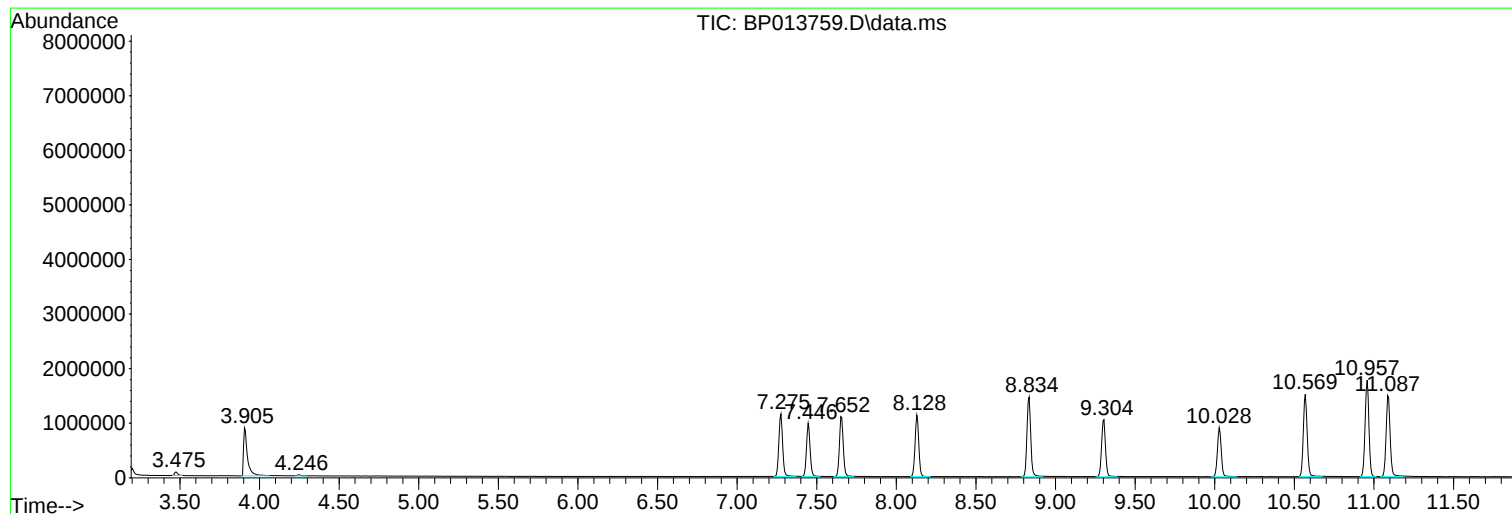

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013759.D
Acq On : 04 Feb 2023 02:18
Operator : CG/JU
Sample : PB150620BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK620

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013759.D
Acq On : 04 Feb 2023 02:18
Operator : CG/JU
Sample : PB150620BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK620

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc