

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013760.D
 Acq On : 04 Feb 2023 02:52
 Operator : CG/JU
 Sample : PB150651BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	59	rBV	66515	100973	0.90%	0.107%
2	3.905	119	122	143	rBV	877355	1526001	13.64%	1.614%
3	4.246	177	180	187	rVB	15469	21931	0.20%	0.023%
4	7.275	687	695	708	rBV	1142071	1869074	16.71%	1.977%
5	7.446	717	724	744	rVB	975187	1549058	13.85%	1.639%
6	7.652	752	759	773	rBV	1120177	1820221	16.28%	1.925%
7	8.128	833	840	852	rBV	908969	1455734	13.02%	1.540%
8	8.834	953	960	977	rBV	1488097	2455111	21.95%	2.597%
9	9.299	1032	1039	1052	rBV	1046665	1744083	15.59%	1.845%
10	10.028	1155	1163	1173	rBV	875215	1477194	13.21%	1.563%
11	10.569	1247	1255	1269	rBV	1578199	2648047	23.68%	2.801%
12	10.957	1311	1321	1330	rBV	1392780	2311676	20.67%	2.445%
13	11.087	1335	1343	1365	rBV	1533071	2713309	24.26%	2.870%
14	12.534	1581	1589	1594	rBV	28067	50280	0.45%	0.053%
15	13.651	1774	1779	1784	rBV	34001	52375	0.47%	0.055%
16	14.163	1856	1866	1878	rBV	3196222	4548542	40.67%	4.811%
17	14.457	1908	1916	1929	rBV	3491866	5383308	48.13%	5.694%
18	14.763	1961	1968	1980	rBV	2467833	3627954	32.44%	3.837%
19	14.945	1991	1999	2025	rBV	1189012	1884479	16.85%	1.993%
20	15.757	2129	2137	2149	rBV	4889359	7241006	64.74%	7.659%
21	15.863	2149	2155	2168	rVV	1184564	1597076	14.28%	1.689%
22	15.998	2173	2178	2184	rVB3	25696	45784	0.41%	0.048%
23	16.539	2266	2270	2276	rVB7	8734	12690	0.11%	0.013%
24	17.192	2377	2381	2387	rBV9	7393	12050	0.11%	0.013%
25	17.516	2429	2436	2446	rBV	3492560	4943291	44.20%	5.229%
26	17.616	2446	2453	2475	rVV2	5966439	8547972	76.43%	9.042%
27	19.410	2754	2758	2764	rBV2	82445	108544	0.97%	0.115%
28	19.480	2766	2770	2778	rVB	78207	109538	0.98%	0.116%
29	19.833	2824	2830	2846	rBV	8557554	11184148	100.00%	11.830%
30	21.592	3124	3129	3141	rBV	4600540	6227281	55.68%	6.587%
31	23.998	3530	3538	3553	rVB2	5366687	11180688	99.97%	11.826%
32	24.163	3559	3566	3580	rVB2	2948628	6090839	54.46%	6.443%




Sum of corrected areas: 94540257

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013760.D
Acq On : 04 Feb 2023 02:52
Operator : CG/JU
Sample : PB150651BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

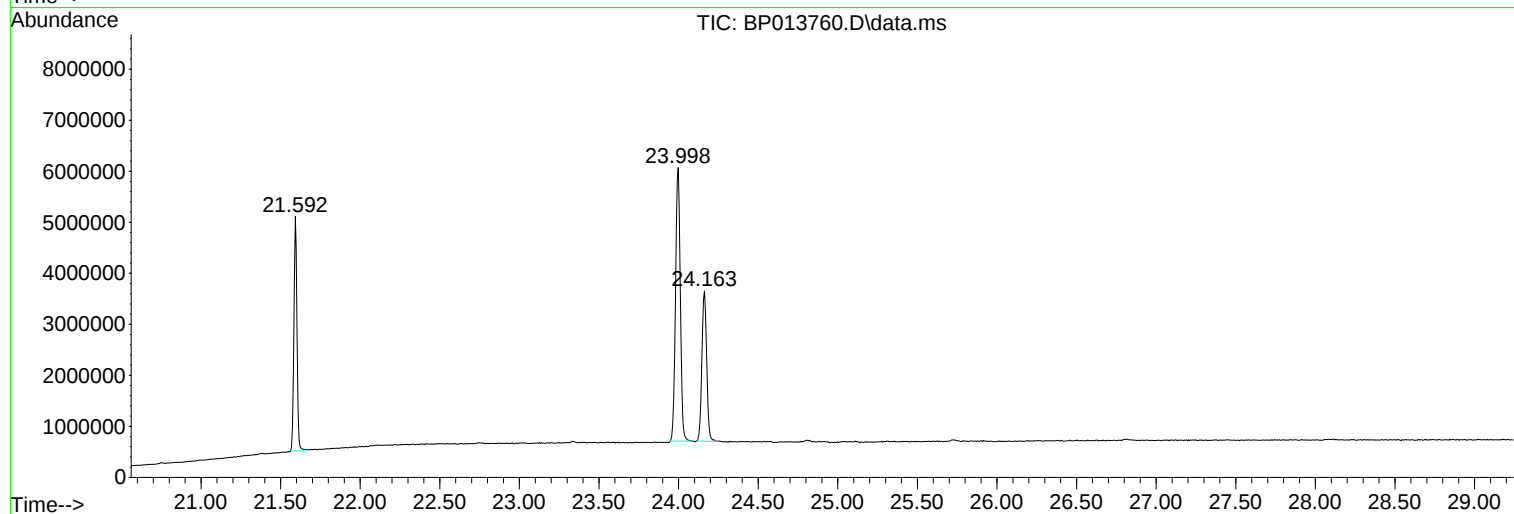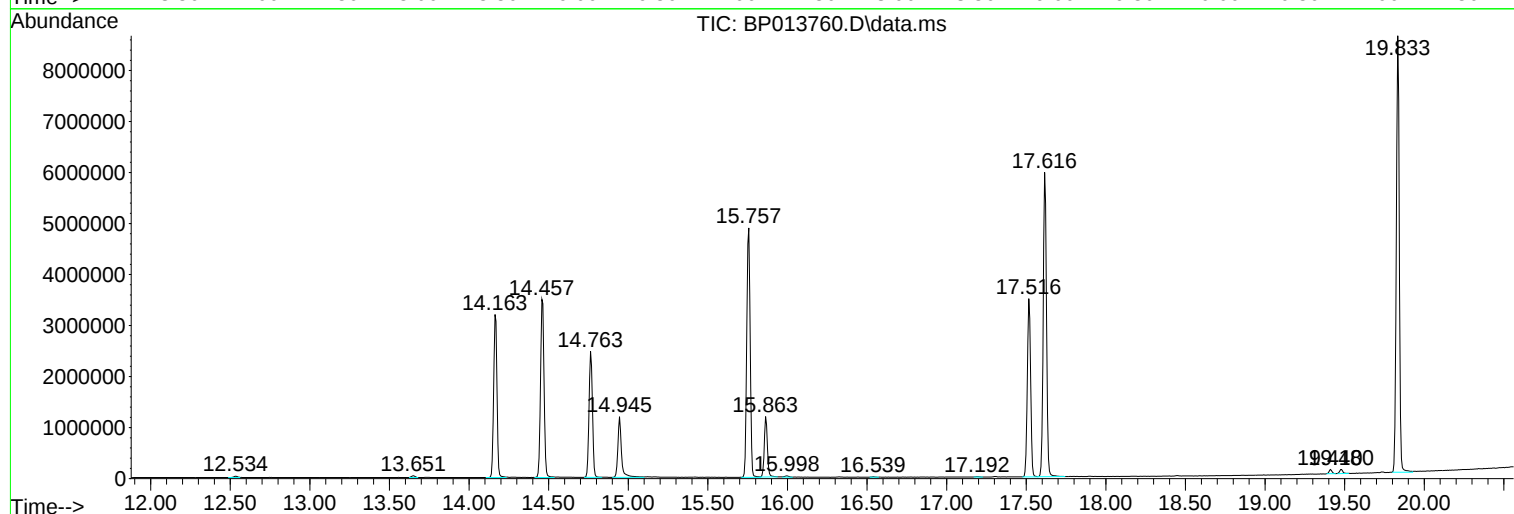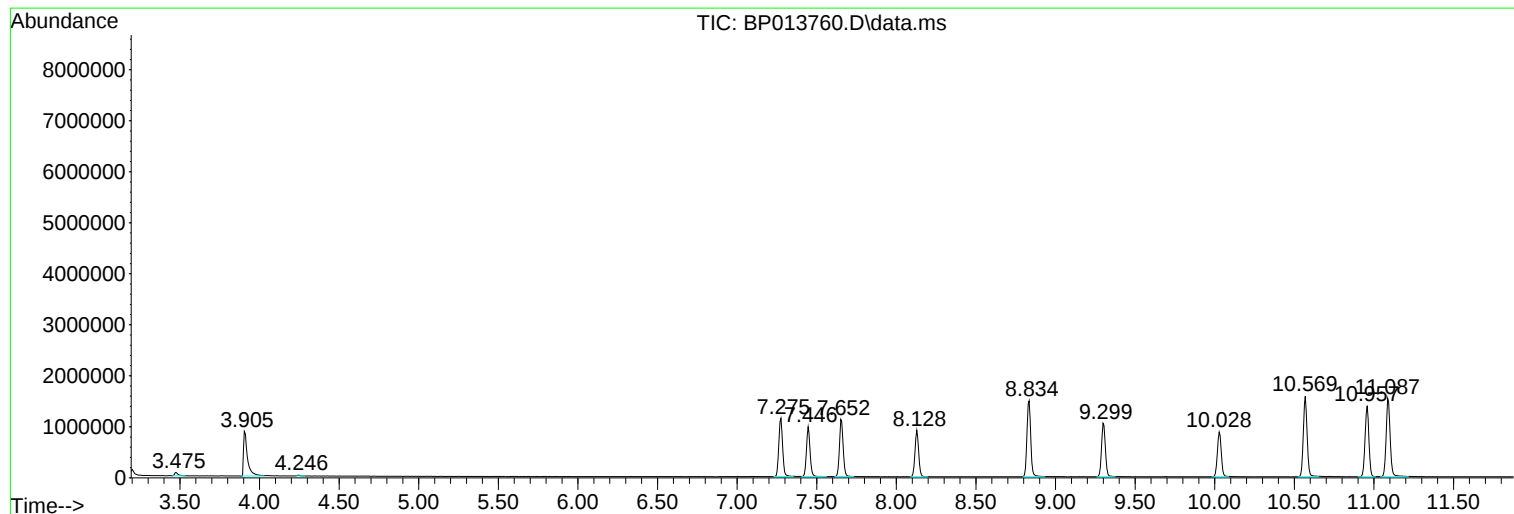

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013760.D
Acq On : 04 Feb 2023 02:52
Operator : CG/JU
Sample : PB150651BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013760.D
Acq On : 04 Feb 2023 02:52
Operator : CG/JU
Sample : PB150651BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc