

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013762.D
 Acq On : 04 Feb 2023 04:34
 Operator : CG/JU
 Sample : 01314-24
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	38	43	68	rVB2	541351	1016089	8.68%	1.119%
2	3.911	121	123	136	rBV	328891	550600	4.70%	0.606%
3	4.146	159	163	168	rVB	26335	42715	0.36%	0.047%
4	4.246	176	180	184	rBV	13635	21946	0.19%	0.024%
5	5.375	365	372	374	rBV	93488	147397	1.26%	0.162%
6	7.275	688	695	706	rVB	250333	417574	3.57%	0.460%
7	7.446	716	724	742	rBV	928352	1497271	12.79%	1.648%
8	7.652	751	759	769	rBV	867058	1416850	12.10%	1.560%
9	8.016	816	821	830	rVB2	19913	37648	0.32%	0.041%
10	8.128	833	840	853	rBV	852814	1524449	13.02%	1.678%
11	8.487	894	901	914	rVB	450913	746603	6.38%	0.822%
12	8.834	951	960	972	rBV	749716	1271754	10.86%	1.400%
13	8.963	979	982	986	rVB5	8607	12691	0.11%	0.014%
14	9.299	1032	1039	1043	rBV	1028326	1734172	14.81%	1.909%
15	9.346	1043	1047	1063	rVB	1197539	1934164	16.52%	2.129%
16	9.705	1101	1108	1114	rVV2	25671	44165	0.38%	0.049%
17	10.028	1154	1163	1171	rBV	904455	1460494	12.48%	1.608%
18	10.416	1224	1229	1239	rBV2	23738	43881	0.37%	0.048%
19	10.569	1247	1255	1265	rBV	1505749	2557665	21.85%	2.816%
20	10.816	1291	1297	1309	rBV3	39191	75775	0.65%	0.083%
21	10.957	1313	1321	1330	rBV	1265113	2134893	18.24%	2.350%
22	11.087	1336	1343	1358	rBV	988160	1764672	15.07%	1.943%
23	12.199	1526	1532	1539	rVB2	35618	58977	0.50%	0.065%
24	12.528	1582	1588	1598	rBV3	31497	61018	0.52%	0.067%
25	13.393	1728	1735	1741	rVB2	10235	20187	0.17%	0.022%
26	13.651	1773	1779	1787	rVB	30741	50174	0.43%	0.055%
27	14.163	1859	1866	1883	rBV	3228606	4518870	38.60%	4.974%
28	14.281	1883	1886	1891	rVB7	8076	13060	0.11%	0.014%
29	14.457	1909	1916	1930	rBV	3379471	5233179	44.70%	5.761%
30	14.763	1961	1968	1977	rBV	2214428	3324720	28.40%	3.660%
31	14.946	1993	1999	2016	rBV	168615	339451	2.90%	0.374%
32	15.104	2022	2026	2031	rBV7	12772	25603	0.22%	0.028%
33	15.169	2031	2037	2044	rVB10	14392	33622	0.29%	0.037%
34	15.351	2062	2068	2069	rBV3	15336	26290	0.22%	0.029%
35	15.757	2127	2137	2149	rBV	5186115	7543543	64.44%	8.304%
36	15.863	2149	2155	2164	rVV	583608	799090	6.83%	0.880%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
 Data File : BP013762.D
 Acq On : 04 Feb 2023 04:34
 Operator : CG/JU
 Sample : 01314-24
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	15.993	2173	2177	2182	rVB	24267	38885	0.33%	0.043%
38	16.116	2192	2198	2204	rBV	143399	198871	1.70%	0.219%
39	16.451	2251	2255	2262	rBV7	11050	19418	0.17%	0.021%
40	16.681	2291	2294	2298	rVB3	9302	12620	0.11%	0.014%
41	16.898	2326	2331	2333	rBV6	8469	12569	0.11%	0.014%
42	17.516	2430	2436	2446	rBV	3178689	4625121	39.51%	5.091%
43	17.616	2446	2453	2469	rVV2	6101660	8810826	75.27%	9.699%
44	17.757	2472	2477	2482	rBV4	36838	72261	0.62%	0.080%
45	18.369	2576	2581	2589	rBV	129200	194351	1.66%	0.214%
46	18.781	2647	2651	2654	rBV3	40254	46238	0.39%	0.051%
47	18.857	2661	2664	2668	rVB3	27163	33650	0.29%	0.037%
48	19.416	2755	2759	2764	rBV2	97663	125906	1.08%	0.139%
49	19.481	2766	2770	2779	rVB	90691	143786	1.23%	0.158%
50	19.592	2786	2789	2793	rBV4	59144	73380	0.63%	0.081%
51	19.833	2824	2830	2840	rBV	8817522	11706367	100.00%	12.887%
52	21.263	3070	3073	3079	rBV2	165870	237742	2.03%	0.262%
53	21.592	3124	3129	3138	rBV	4221718	5582924	47.69%	6.146%
54	23.992	3529	3537	3549	rBV2	5259941	11061958	94.50%	12.177%
55	24.163	3559	3566	3577	rVB2	2471624	5343011	45.64%	5.882%




Sum of corrected areas: 90841136

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013762.D
Acq On : 04 Feb 2023 04:34
Operator : CG/JU
Sample : 01314-24
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

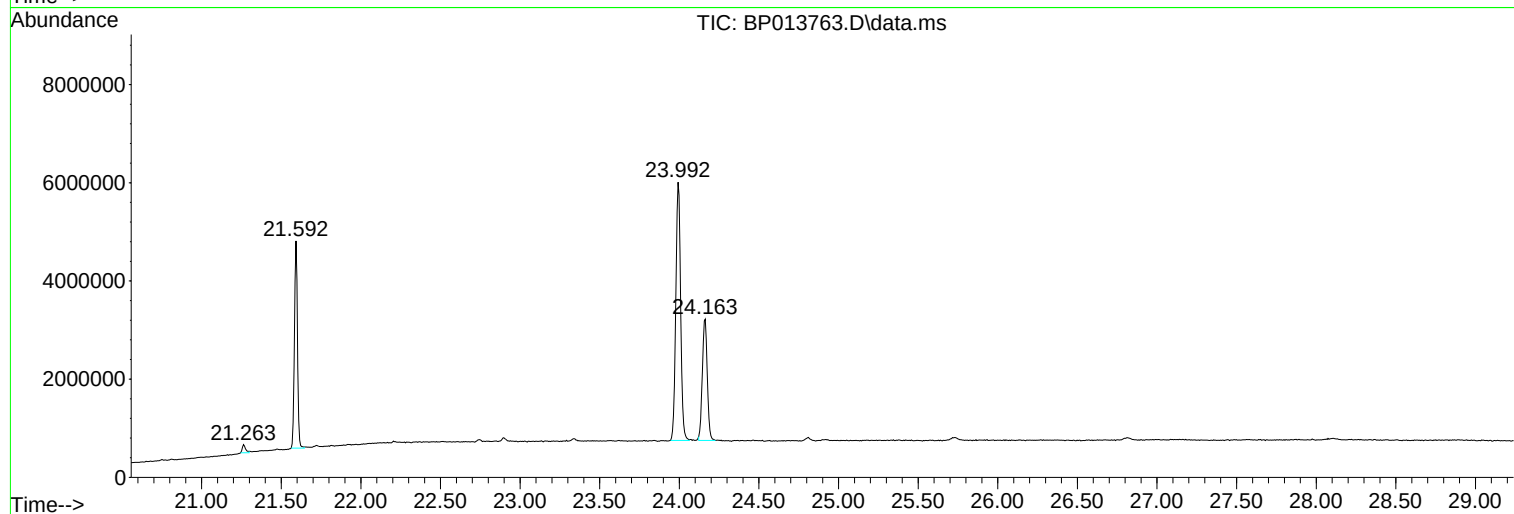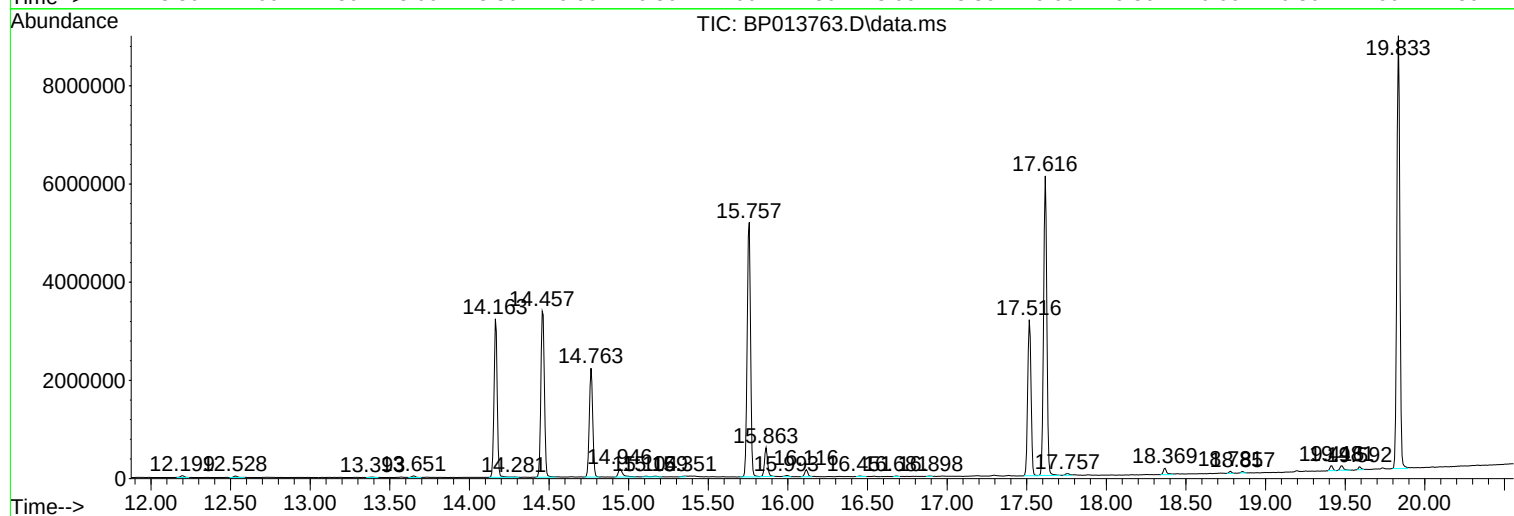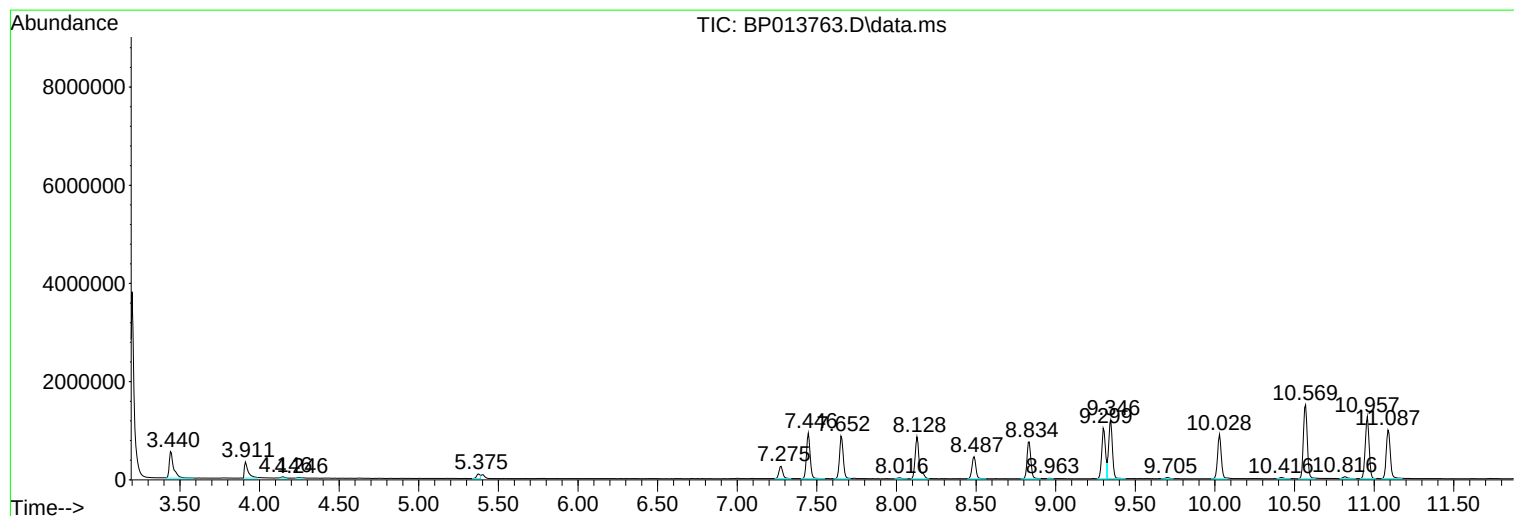

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013762.D
Acq On : 04 Feb 2023 04:34
Operator : CG/JU
Sample : 01314-24
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020223\
Data File : BP013762.D
Acq On : 04 Feb 2023 04:34
Operator : CG/JU
Sample : 01314-24
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
