

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
 Data File : BP013775.D
 Acq On : 06 Feb 2023 16:58
 Operator : CG/JU
 Sample : 01381-21DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6DL

Quant Time: Feb 06 23:56:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 23:44:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.128	152	211779	20.000	ng/ul	0.00
20) Naphthalene-d8	10.952	136	917634	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.763	164	701793	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.516	188	1791418	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1874876	20.000	ng/ul	0.00
88) Perylene-d12	24.163	264	1873218	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.476	96	3413	0.683	ng/uL	0.00
4) Pyridine-d5	3.928	84	18519	1.292	ng/ul	0.02
7) Phenol-d5	7.275	99	25466	1.368	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.446	67	82236	7.533	ng/ul	0.00
11) 2-Chlorophenol-d4	7.658	132	72509	5.314	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	47034	3.170	ng/ul	0.00
21) Nitrobenzene-d5	9.299	128	39583	6.762	ng/ul	0.00
24) 2-Nitrophenol-d4	10.028	143	44242	6.485	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	91614	5.743	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	72819	3.456	ng/ul	0.00
46) Dimethylphthalate-d6	14.163	166	420520	7.602	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	423619	6.931	ng/ul	0.00
54) 4-Nitrophenol-d4	14.928	143	8	0.001	ng/ul	-0.02
60) Fluorene-d10	15.751	176	398142	8.350	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	14410	1.435	ng/ul	0.00
73) Anthracene-d10	17.616	188	726081	8.695	ng/ul	0.00
81) Pyrene-d10	19.834	212	966947	9.247	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.992	264	813694	8.509	ng/ul	-0.01
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.340	77	794323	50.239	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013775.D
Acq On : 06 Feb 2023 16:58
Operator : CG/JU
Sample : 01381-21DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6DL

Quant Time: Feb 06 23:56:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 03 23:44:43 2023
Response via : Initial Calibration

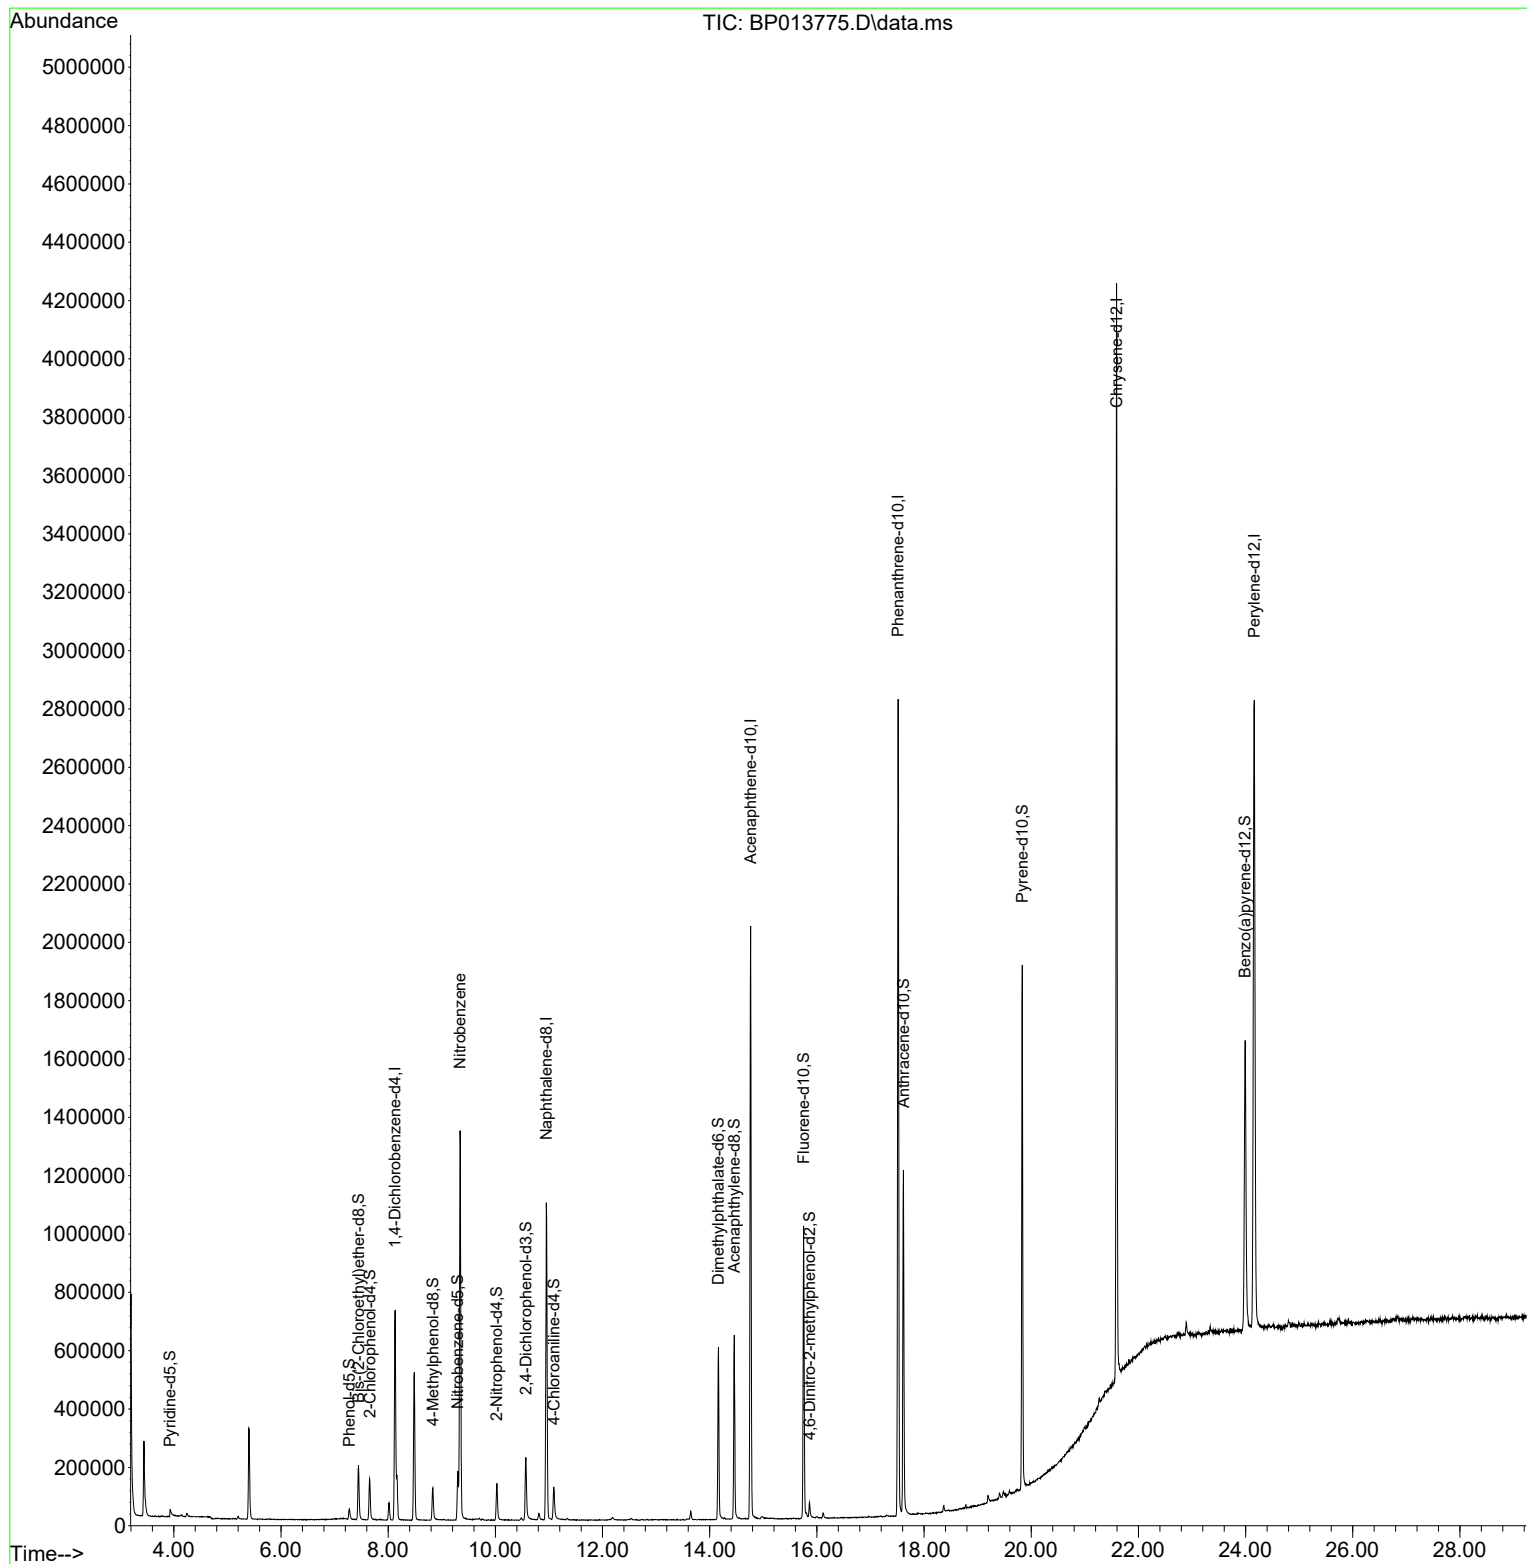

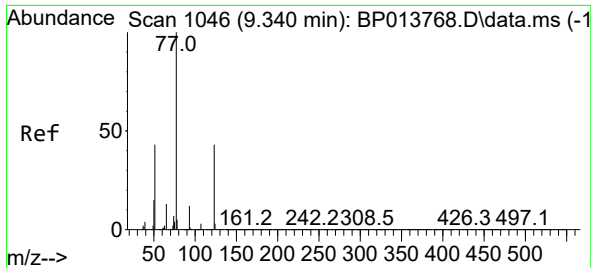

#22
 Nitrobenzene
 Concen: 50.239 ng/ul
 RT: 9.340 min Scan# 10
 Delta R.T. -0.006 min
 Lab File: BP013775.D
 Acq: 06 Feb 2023 16:58

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6DL

Tgt Ion: 77 Resp: 794323
 Ion Ratio Lower Upper
 77 100
 123 42.8 34.1 51.1
 65 12.7 9.8 14.8

