

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
 Data File : BP013771.D
 Acq On : 06 Feb 2023 13:58
 Operator : CG/JU
 Sample : 01381-22
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.446	39	44	61	rVB2	235301	441476	4.93%	0.575%
2	3.916	121	124	143	rBV	118633	216945	2.42%	0.283%
3	4.146	158	163	172	rVB2	17006	31167	0.35%	0.041%
4	4.246	176	180	186	rBV2	14807	23731	0.27%	0.031%
5	5.199	337	342	350	rBV	25936	42181	0.47%	0.055%
6	5.411	370	378	389	rBV	1629869	2650315	29.62%	3.453%
7	7.281	690	696	705	rBV	157754	259635	2.90%	0.338%
8	7.452	718	725	740	rBV	662987	1055918	11.80%	1.376%
9	7.657	753	760	771	rBV	592437	978577	10.94%	1.275%
10	8.022	816	822	830	rBV	74099	123470	1.38%	0.161%
11	8.134	832	841	844	rBV	710335	1129209	12.62%	1.471%
12	8.169	844	847	857	rVB	547859	888509	9.93%	1.158%
13	8.493	894	902	915	rBV	2437297	4050419	45.26%	5.278%
14	8.840	953	961	970	rBV	503835	843517	9.43%	1.099%
15	9.310	1033	1041	1053	rBV	682585	1173092	13.11%	1.529%
16	9.404	1053	1057	1063	rVB6	8957	15592	0.17%	0.020%
17	9.704	1104	1108	1115	rVB	16906	28694	0.32%	0.037%
18	9.775	1115	1120	1123	rBV7	7120	11110	0.12%	0.014%
19	9.981	1149	1155	1159	rBV	42758	75757	0.85%	0.099%
20	10.034	1159	1164	1173	rVB	523487	873962	9.77%	1.139%
21	10.575	1248	1256	1273	rBV	974728	1663013	18.58%	2.167%
22	10.822	1291	1298	1307	rBV	1240418	2066839	23.10%	2.693%
23	10.963	1313	1322	1330	rBV	1068596	1815045	20.28%	2.365%
24	11.098	1337	1345	1357	rBV	473604	822536	9.19%	1.072%
25	11.351	1379	1388	1395	rBV	321435	540114	6.04%	0.704%
26	12.198	1529	1532	1540	rVB7	7630	12709	0.14%	0.017%
27	12.357	1553	1559	1566	rVB8	6732	12276	0.14%	0.016%
28	12.481	1576	1580	1586	rBV5	7775	16605	0.19%	0.022%
29	12.540	1586	1590	1595	rVV3	18948	33952	0.38%	0.044%
30	12.587	1596	1598	1607	rVB10	5462	9466	0.11%	0.012%
31	12.981	1660	1665	1676	rBV	24700	46756	0.52%	0.061%
32	13.298	1713	1719	1726	rVB10	6642	16559	0.19%	0.022%
33	13.587	1760	1768	1770	rBV3	15830	25789	0.29%	0.034%
34	13.657	1776	1780	1785	rVB7	6288	10784	0.12%	0.014%
35	13.822	1802	1808	1817	rBV	43562	71048	0.79%	0.093%
36	14.169	1858	1867	1882	rBV	2195355	3065355	34.25%	3.994%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
 Data File : BP013771.D
 Acq On : 06 Feb 2023 13:58
 Operator : CG/JU
 Sample : 01381-22
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	14.292	1885	1888	1893	rVB7	7183	10661	0.12%	0.014%
38	14.469	1909	1918	1931	rBV	2382011	3514918	39.28%	4.580%
39	14.769	1962	1969	1981	rBV	1963094	2873814	32.11%	3.745%
40	14.957	1995	2001	2016	rBV2	96637	223777	2.50%	0.292%
41	15.163	2033	2036	2047	rVB8	15593	33425	0.37%	0.044%
42	15.763	2126	2138	2150	rBV	3673523	5189982	58.00%	6.763%
43	15.869	2150	2156	2169	rVB	738157	1064928	11.90%	1.388%
44	16.004	2175	2179	2188	rVB5	20085	34349	0.38%	0.045%
45	16.122	2193	2199	2211	rBV	338525	495821	5.54%	0.646%
46	16.263	2218	2223	2231	rBV2	36682	60119	0.67%	0.078%
47	16.351	2234	2238	2244	rVB5	9433	17075	0.19%	0.022%
48	16.457	2251	2256	2260	rBV7	8387	16007	0.18%	0.021%
49	16.904	2328	2332	2335	rVB5	8146	11672	0.13%	0.015%
50	17.398	2413	2416	2423	rVB5	17253	26118	0.29%	0.034%
51	17.522	2431	2437	2448	rBV	2612977	3909953	43.69%	5.095%
52	17.622	2448	2454	2465	rBV2	4471718	6553000	73.23%	8.539%
53	18.375	2578	2582	2589	rBV2	112123	150395	1.68%	0.196%
54	18.457	2593	2596	2602	rVB2	12991	25534	0.29%	0.033%
55	18.698	2634	2637	2644	rVB	40071	54170	0.61%	0.071%
56	19.422	2756	2760	2763	rBV2	62264	90439	1.01%	0.118%
57	19.457	2763	2766	2768	rVV	33179	41454	0.46%	0.054%
58	19.486	2768	2771	2775	rVB	63570	79166	0.88%	0.103%
59	19.598	2787	2790	2793	rBV3	41783	60764	0.68%	0.079%
60	19.839	2825	2831	2841	rBV	6573574	8948701	100.00%	11.661%
61	20.051	2864	2867	2872	rBV	73587	88604	0.99%	0.115%
62	21.274	3072	3075	3083	rBV3	271629	462131	5.16%	0.602%
63	21.598	3125	3130	3141	rBV	3347548	4876806	54.50%	6.355%
64	24.010	3532	3540	3555	rVB	3887983	8220695	91.86%	10.712%
65	24.174	3561	3568	3579	rVB2	2105630	4466418	49.91%	5.820%




Sum of corrected areas: 76743018

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013771.D
Acq On : 06 Feb 2023 13:58
Operator : CG/JU
Sample : 01381-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

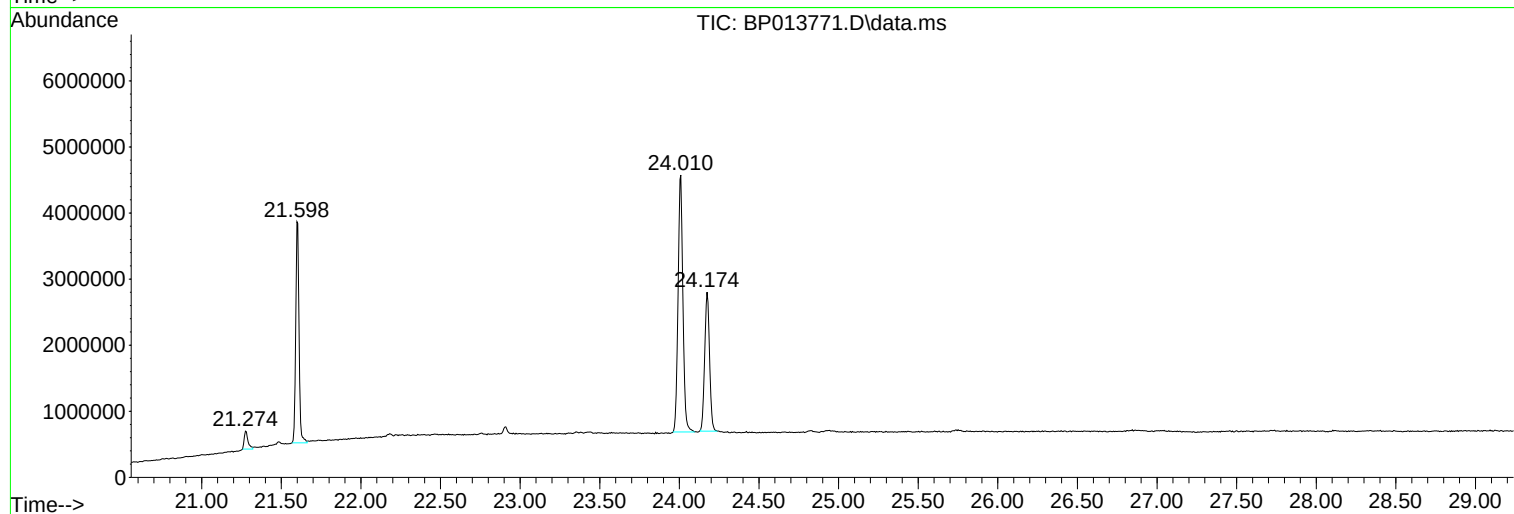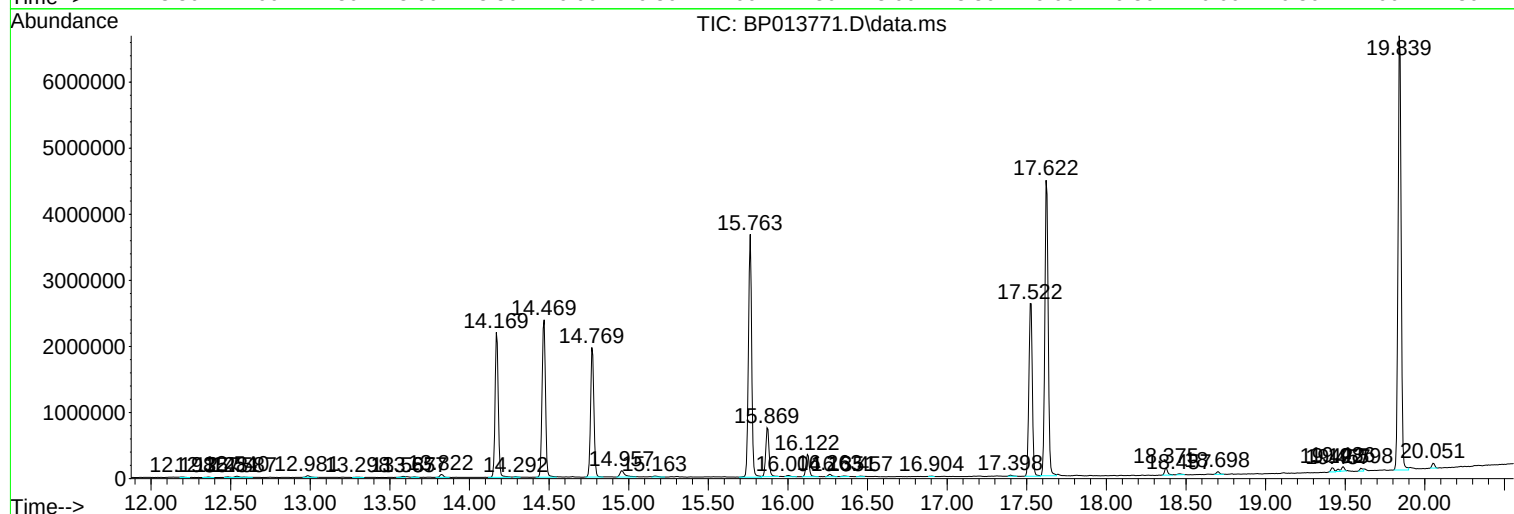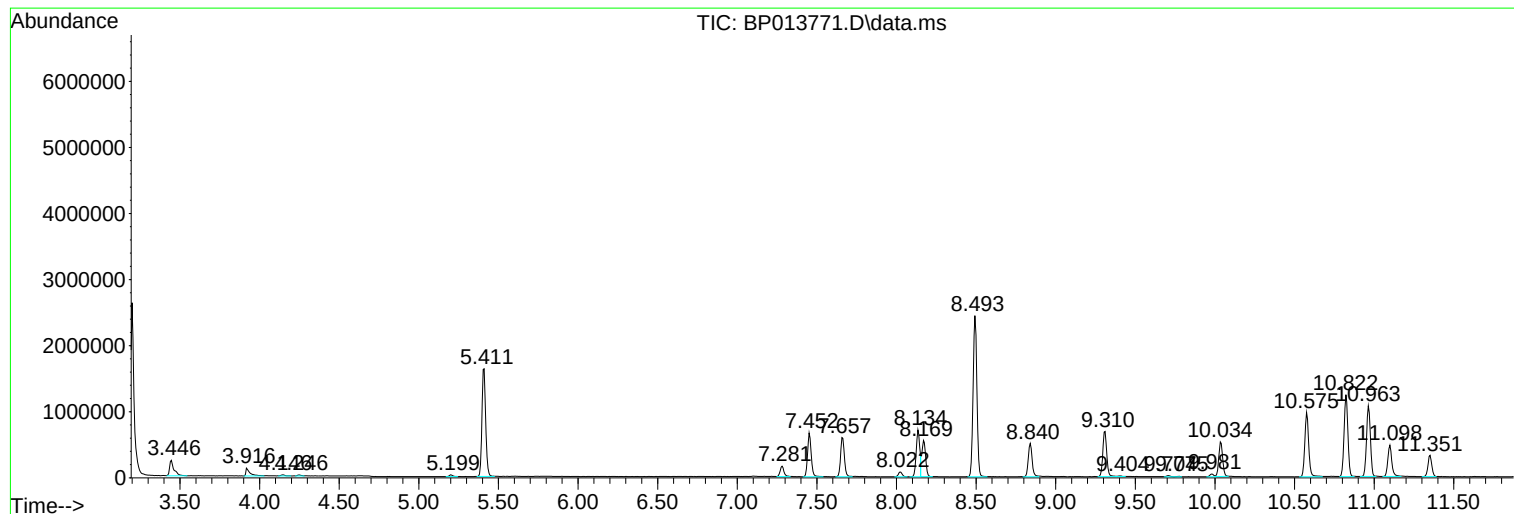

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013771.D
Acq On : 06 Feb 2023 13:58
Operator : CG/JU
Sample : 01381-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Benzene, 1,3,5-trichloro- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.822	22.77 ng/ul	2066840	Naphthalene-d8	10.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
5			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	97

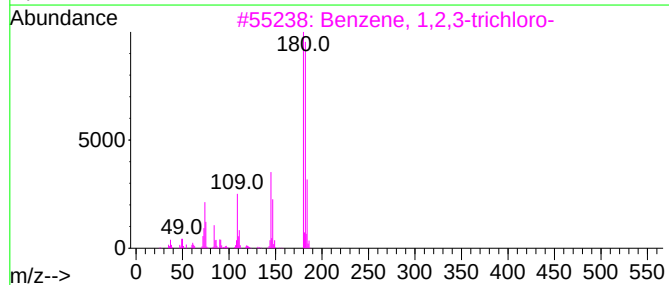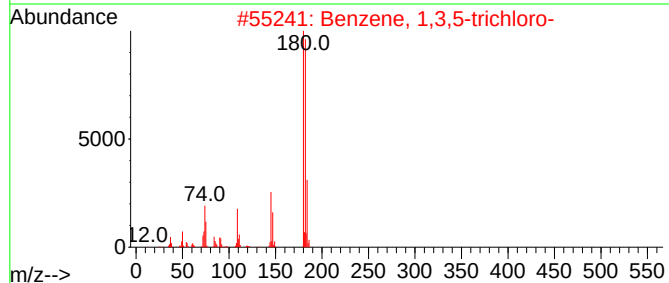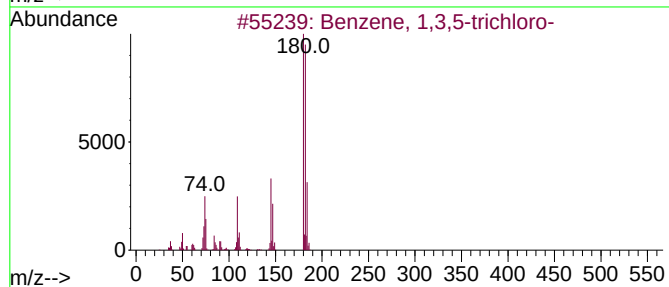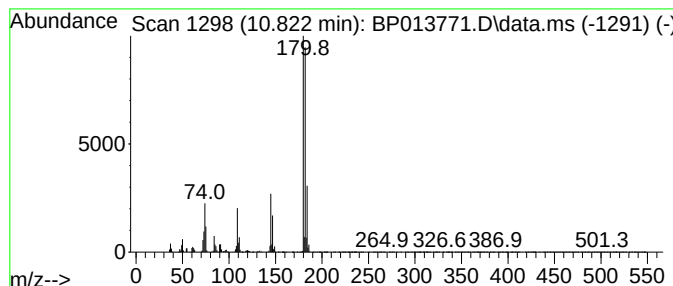

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013771.D
Acq On : 06 Feb 2023 13:58
Operator : CG/JU
Sample : 01381-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Benzophenone Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.122	3.45 ng/ul	495821	Acenaphthene-d10	14.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	93
5			1,2,4-Trioxolane, 3,3,5-triphenyl-	304	C20H16O3	023246-12-0	45

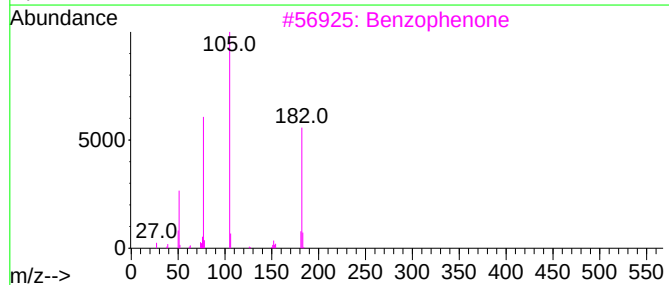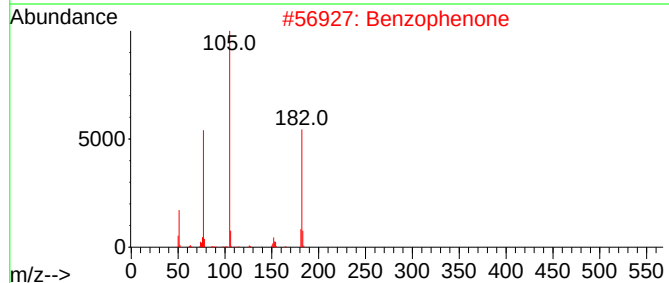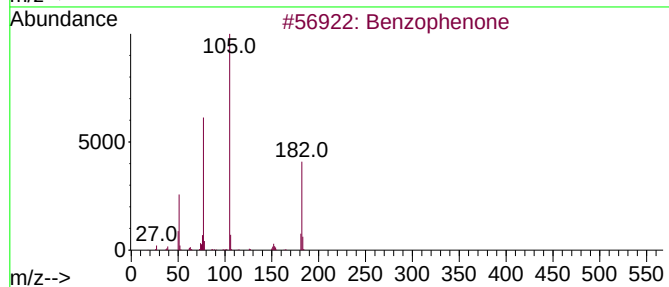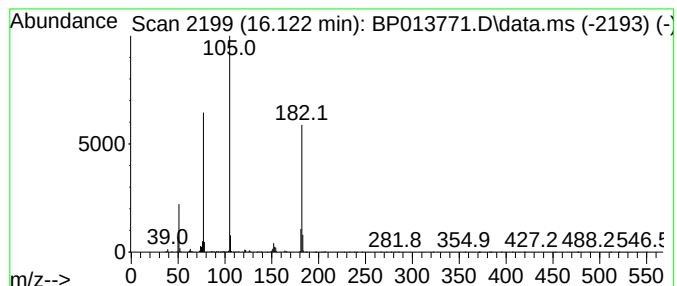

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013771.D
Acq On : 06 Feb 2023 13:58
Operator : CG/JU
Sample : 01381-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	10.822	22.8	ng/u1	2066840	2	10.963	1815050	20.0
Benzophenone	16.122	3.5	ng/u1	495821	3	14.769	2873810	20.0