

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
 Data File : BP013774.D
 Acq On : 06 Feb 2023 16:24
 Operator : CG/JU
 Sample : 01381-25
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013774.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	45	49	55	rVB	44023	59284	0.54%	0.071%
2	3.916	121	124	141	rBV	167795	329870	2.98%	0.397%
3	4.146	158	163	172	rVV3	20218	37814	0.34%	0.045%
4	4.246	176	180	188	rBV	15764	26363	0.24%	0.032%
5	5.199	337	342	353	rVB2	33710	55366	0.50%	0.067%
6	7.281	690	696	705	rVB	185309	317926	2.87%	0.382%
7	7.452	718	725	740	rBV	828613	1365373	12.33%	1.642%
8	7.657	751	760	771	rBV	742186	1234028	11.15%	1.484%
9	8.134	833	841	855	rBV	902337	1480167	13.37%	1.780%
10	8.493	897	902	911	rVB6	7186	16158	0.15%	0.019%
11	8.834	953	960	975	rBV	584912	1002007	9.05%	1.205%
12	9.304	1033	1040	1054	rBV	910978	1559746	14.09%	1.876%
13	9.404	1054	1057	1063	rVB6	6311	11652	0.11%	0.014%
14	9.704	1104	1108	1114	rVB	23732	36916	0.33%	0.044%
15	9.763	1114	1118	1128	rVB4	13979	25427	0.23%	0.031%
16	10.034	1156	1164	1184	rBV	740357	1217572	11.00%	1.465%
17	10.575	1248	1256	1272	rBV	1197429	2109452	19.05%	2.537%
18	10.816	1292	1297	1303	rBV4	10076	16817	0.15%	0.020%
19	10.963	1313	1322	1330	rBV	1345277	2279198	20.59%	2.741%
20	11.093	1337	1344	1356	rBV	1011986	1791635	16.18%	2.155%
21	12.175	1515	1528	1538	rVB4	31660	120909	1.09%	0.145%
22	12.540	1585	1590	1599	rBV	24851	44222	0.40%	0.053%
23	12.987	1659	1666	1672	rVB	5748	12220	0.11%	0.015%
24	13.398	1730	1736	1742	rVB2	6534	12469	0.11%	0.015%
25	13.581	1759	1767	1771	rBV5	14872	24444	0.22%	0.029%
26	13.651	1774	1779	1787	rVB2	23263	35414	0.32%	0.043%
27	14.169	1859	1867	1882	rBV	2915098	4054425	36.62%	4.877%
28	14.281	1883	1886	1894	rVB10	8092	16751	0.15%	0.020%
29	14.463	1910	1917	1932	rBV	3087774	4625759	41.78%	5.564%
30	14.769	1962	1969	1981	rBV	2479847	3582729	32.36%	4.309%
31	14.951	1993	2000	2013	rBV	99010	231203	2.09%	0.278%
32	15.175	2033	2038	2043	rVB8	12595	28887	0.26%	0.035%
33	15.757	2125	2137	2150	rBV	4372248	6490827	58.63%	7.807%
34	15.869	2150	2156	2167	rVB	271379	404240	3.65%	0.486%
35	15.998	2172	2178	2186	rVB4	23045	47124	0.43%	0.057%
36	16.122	2195	2199	2213	rVB	62737	97413	0.88%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
 Data File : BP013774.D
 Acq On : 06 Feb 2023 16:24
 Operator : CG/JU
 Sample : 01381-25
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

37	16.892	2327	2330	2338	rBV9	6433	14328	0.13%	0.017%
38	17.522	2431	2437	2447	rBV	3424265	4838982	43.71%	5.820%
39	17.622	2447	2454	2464	rBV2	5674507	8103729	73.20%	9.747%
40	17.892	2496	2500	2506	rVB5	14764	22394	0.20%	0.027%
41	18.375	2577	2582	2589	rBV	112120	161452	1.46%	0.194%
42	18.863	2662	2665	2670	rBV6	14213	24445	0.22%	0.029%
43	19.204	2718	2723	2730	rBV2	171559	336825	3.04%	0.405%
44	19.416	2755	2759	2764	rBV	93247	121853	1.10%	0.147%
45	19.486	2767	2771	2781	rVB	86577	153334	1.39%	0.184%
46	19.598	2787	2790	2793	rBV3	39095	47715	0.43%	0.057%
47	19.839	2825	2831	2847	rBV	8461750	11070534	100.00%	13.316%
48	21.269	3071	3074	3085	rBV3	238263	451439	4.08%	0.543%
49	21.598	3125	3130	3139	rBV	4580066	6061938	54.76%	7.291%
50	24.004	3531	3539	3552	rBV2	5204507	10993378	99.30%	13.223%
51	24.168	3560	3567	3578	rVB2	2744173	5934121	53.60%	7.138%




Sum of corrected areas: 83138274

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013774.D
Acq On : 06 Feb 2023 16:24
Operator : CG/JU
Sample : 01381-25
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44P7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

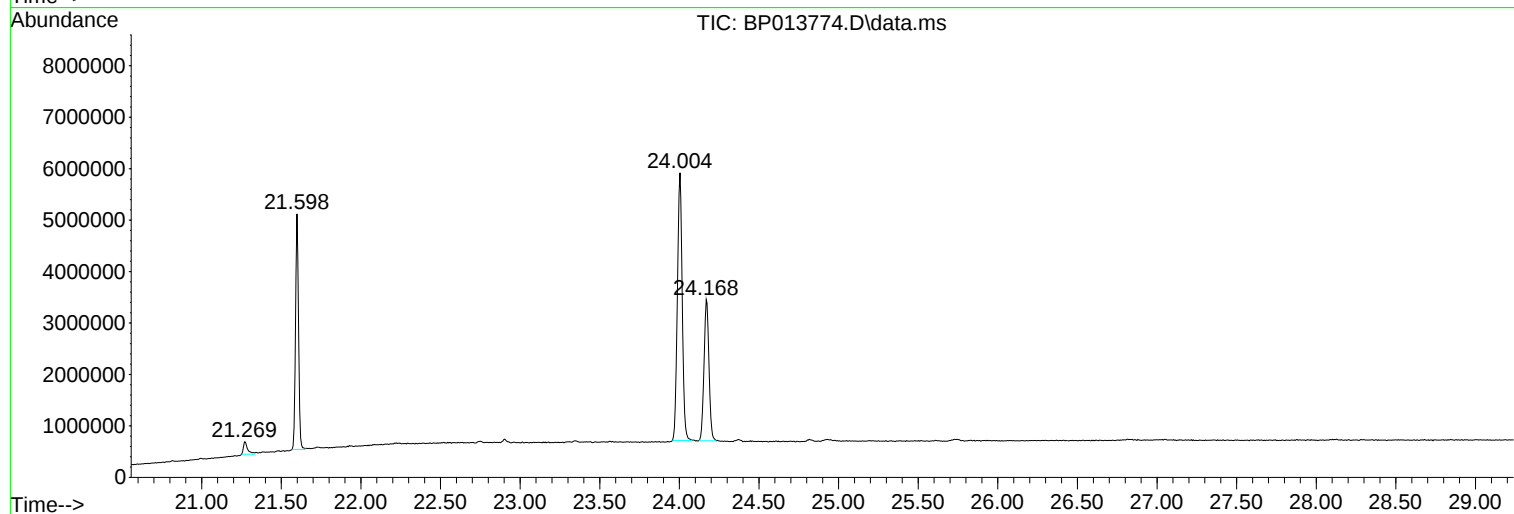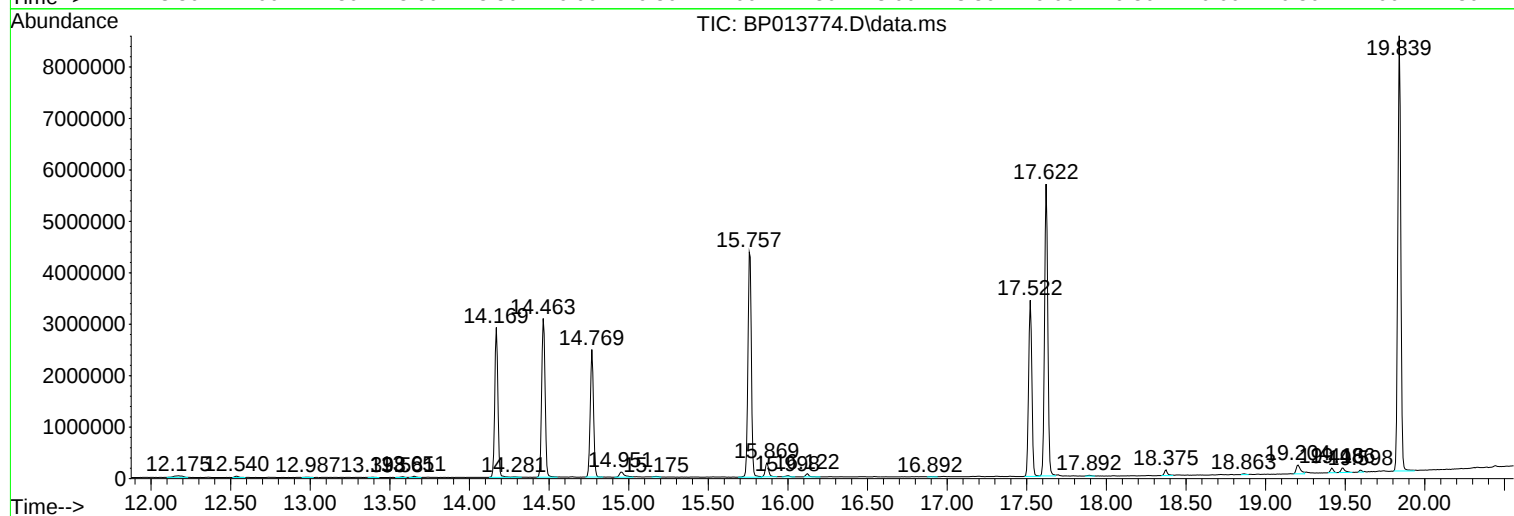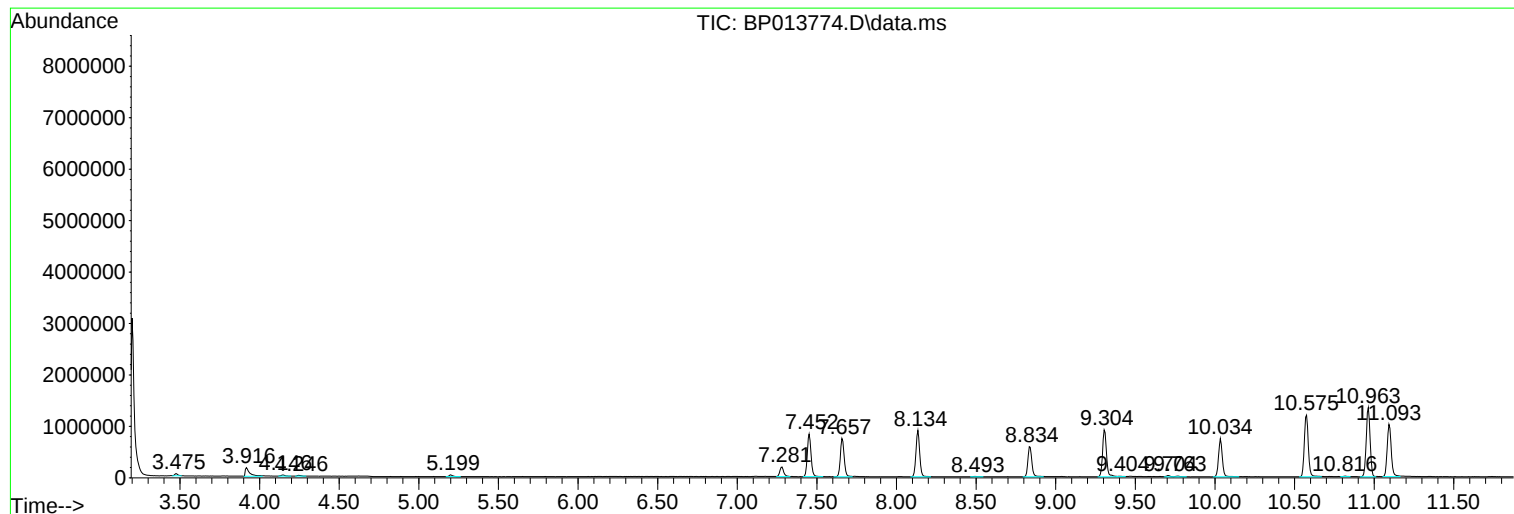

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013774.D
Acq On : 06 Feb 2023 16:24
Operator : CG/JU
Sample : 01381-25
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44P7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013774.D
Acq On : 06 Feb 2023 16:24
Operator : CG/JU
Sample : 01381-25
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44P7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc