

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
 Data File : BP013775.D
 Acq On : 06 Feb 2023 16:58
 Operator : CG/JU
 Sample : 01381-21DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013775.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	38	43	61	rVB	257247	443687	8.90%	1.232%
2	3.928	125	126	135	rBV	25394	52452	1.05%	0.146%
3	4.246	173	180	186	rBV2	12552	26249	0.53%	0.073%
4	5.199	336	342	354	rBV4	10245	21766	0.44%	0.060%
5	5.399	370	376	387	rBV	312503	529080	10.62%	1.470%
6	7.275	688	695	702	rBV	35565	66607	1.34%	0.185%
7	7.446	717	724	736	rVB	186614	316954	6.36%	0.880%
8	7.652	751	759	770	rBV	140868	255052	5.12%	0.708%
9	8.017	814	821	827	rBV	59561	102038	2.05%	0.283%
10	8.128	830	840	844	rBV	719814	1211832	24.32%	3.366%
11	8.487	893	901	909	rBV	506567	864479	17.35%	2.401%
12	8.834	952	960	971	rBV	111282	211647	4.25%	0.588%
13	9.299	1033	1039	1041	rBV	167985	258032	5.18%	0.717%
14	9.340	1041	1046	1059	rVB	1330831	2268006	45.51%	6.299%
15	9.699	1104	1107	1112	rVB6	5843	7953	0.16%	0.022%
16	10.028	1156	1163	1174	rBV	126658	228422	4.58%	0.634%
17	10.481	1233	1240	1246	rBV9	8354	16562	0.33%	0.046%
18	10.569	1246	1255	1264	rBV	215557	407181	8.17%	1.131%
19	10.810	1292	1296	1303	rBV2	21064	37438	0.75%	0.104%
20	10.952	1312	1320	1336	rBV	1087521	1863181	37.39%	5.175%
21	11.093	1336	1344	1357	rBV	110243	238375	4.78%	0.662%
22	11.346	1380	1387	1392	rBV8	5439	10501	0.21%	0.029%
23	12.187	1526	1530	1537	rVB5	8452	16640	0.33%	0.046%
24	12.534	1585	1589	1593	rBV5	4646	7327	0.15%	0.020%
25	13.581	1762	1767	1769	rBV6	4236	7172	0.14%	0.020%
26	13.646	1773	1778	1785	rVB2	28488	47326	0.95%	0.131%
27	14.163	1857	1866	1881	rBV	591814	865844	17.37%	2.405%
28	14.457	1906	1916	1932	rBV	631555	950531	19.07%	2.640%
29	14.763	1961	1968	1977	rBV	2031997	2992321	60.05%	8.311%
30	14.981	1999	2005	2010	rBV9	7335	19402	0.39%	0.054%
31	15.157	2033	2035	2042	rVB8	2973	5332	0.11%	0.015%
32	15.751	2128	2136	2143	rBV	1002548	1417439	28.44%	3.937%
33	15.863	2150	2155	2163	rVB	50025	79591	1.60%	0.221%
34	15.987	2173	2176	2185	rVB	4832	10579	0.21%	0.029%
35	16.116	2194	2198	2204	rVB	16452	23731	0.48%	0.066%
36	17.304	2397	2400	2403	rBV5	4478	5822	0.12%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
 Data File : BP013775.D
 Acq On : 06 Feb 2023 16:58
 Operator : CG/JU
 Sample : 01381-21DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44Q6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M

Title : SVOA CALIBRATION

37	17.516	2428	2436	2446	rBV	2801927	4117600	82.63%	11.437%
38	17.616	2447	2453	2471	rVB	1180753	1779948	35.72%	4.944%
39	18.369	2577	2581	2586	rBV6	21096	33387	0.67%	0.093%
40	18.781	2648	2651	2654	rBV5	12424	14619	0.29%	0.041%
41	19.192	2718	2721	2730	rBV8	25312	54733	1.10%	0.152%
42	19.834	2824	2830	2839	rBV	1796736	2420121	48.56%	6.722%
43	21.592	3124	3129	3139	rBV	3745749	4983453	100.00%	13.842%
44	23.992	3531	3537	3547	rVB	977370	2055126	41.24%	5.708%
45	24.163	3559	3566	3578	rVB2	2137508	4658110	93.47%	12.938%




Sum of corrected areas: 36003648

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013775.D
Acq On : 06 Feb 2023 16:58
Operator : CG/JU
Sample : 01381-21DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

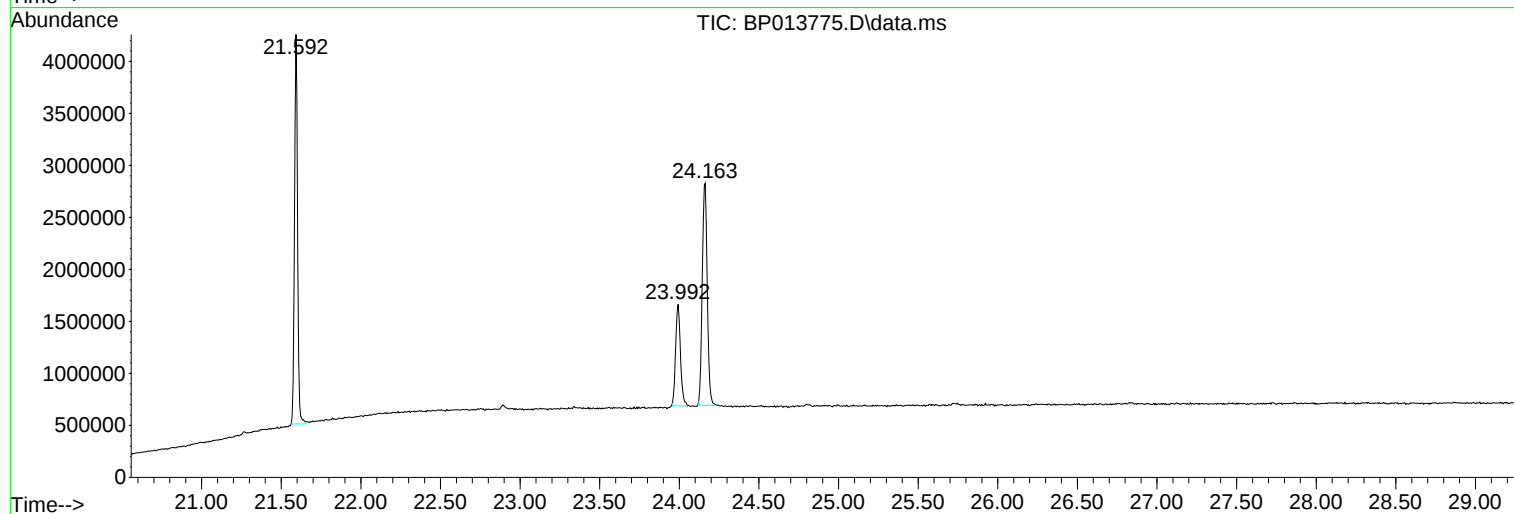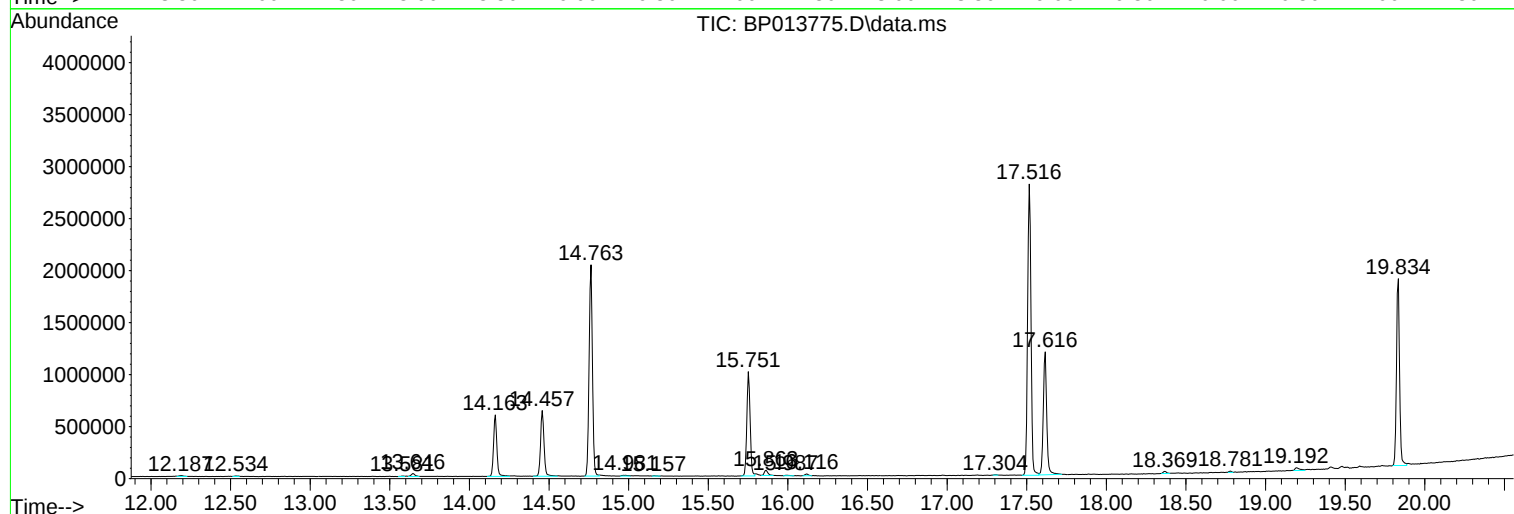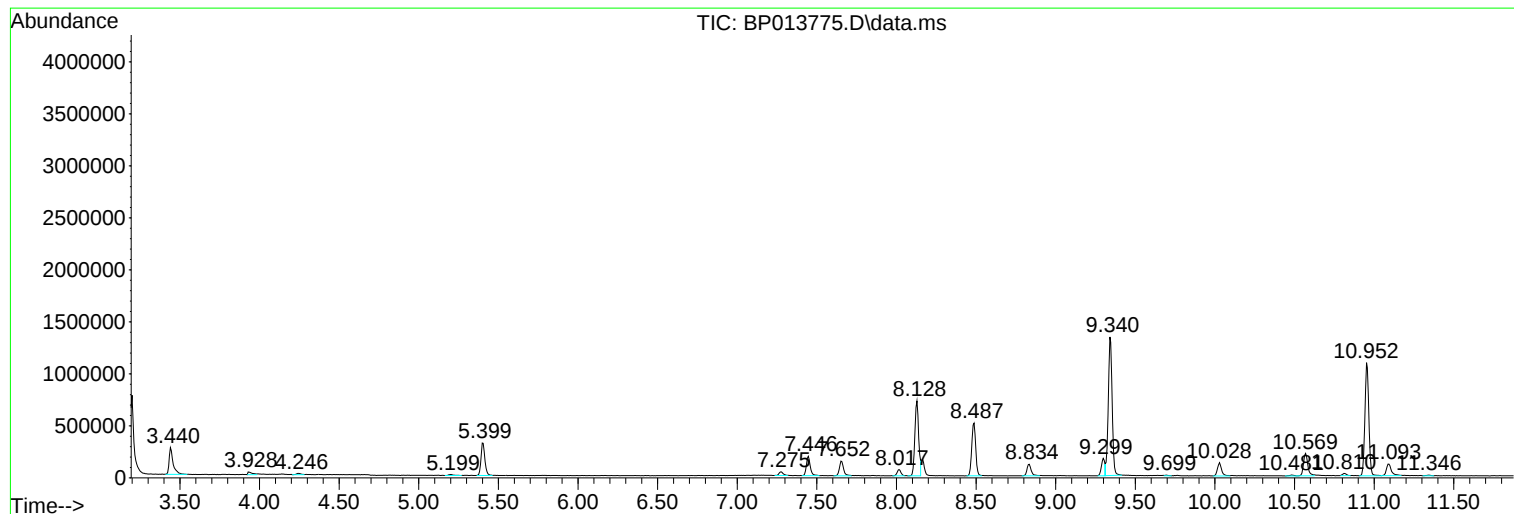

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013775.D
Acq On : 06 Feb 2023 16:58
Operator : CG/JU
Sample : 01381-21DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020623\
Data File : BP013775.D
Acq On : 06 Feb 2023 16:58
Operator : CG/JU
Sample : 01381-21DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44Q6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------