
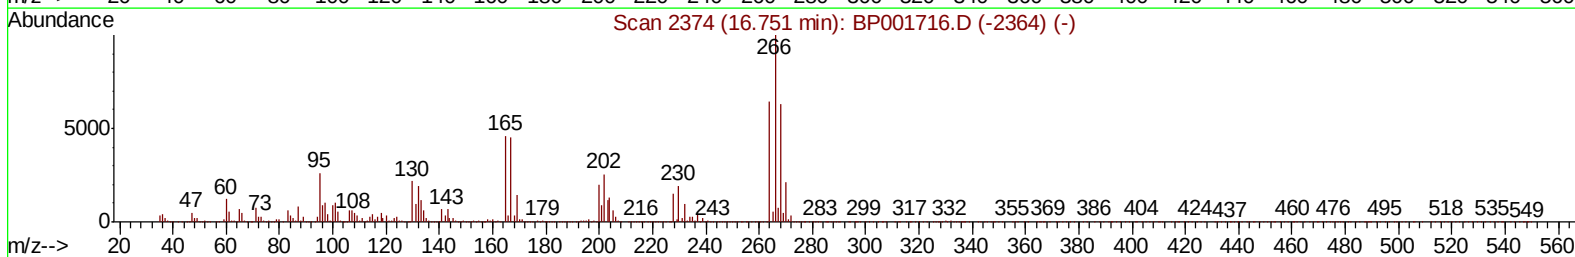
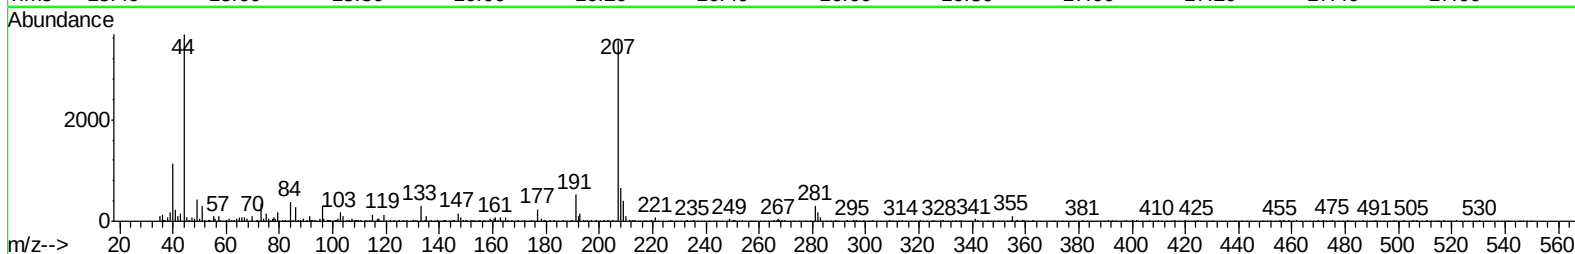


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP020720\
 Data File : BP001722.D
 Acq On : 07 Feb 2020 15:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 02:17:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 15:16:18 2020
 Response via : Initial Calibration

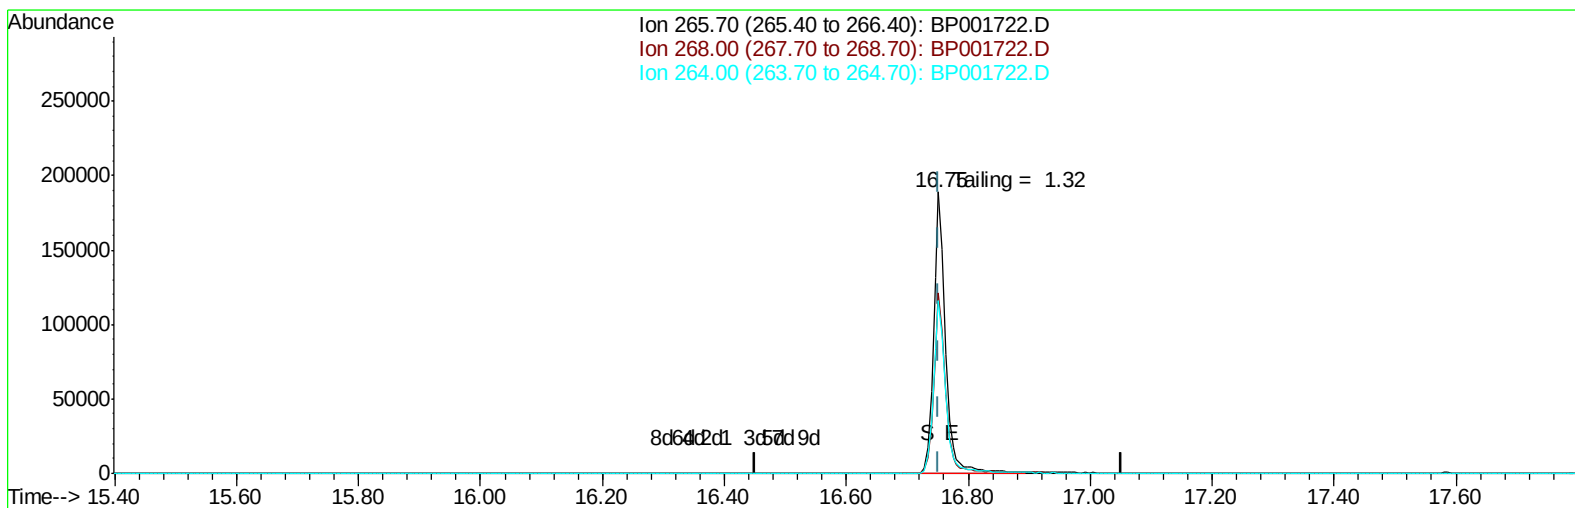

TIC: BP001722.D

(70) Pentachlorophenol (C)




16.404min (-0.347) 23.65ng

response 21

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	140.00#
264.00	64.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP020720\
 Data File : BP001722.D
 Acq On : 07 Feb 2020 15:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 02:17:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 15:16:18 2020
 Response via : Initial Calibration

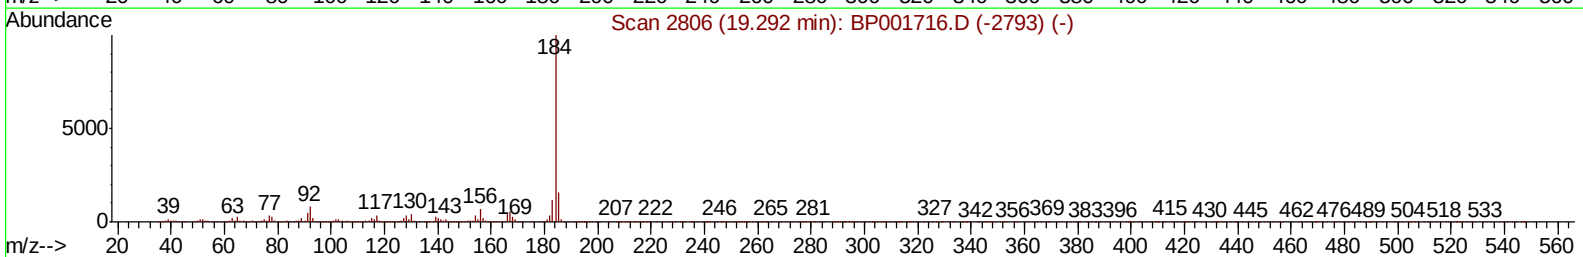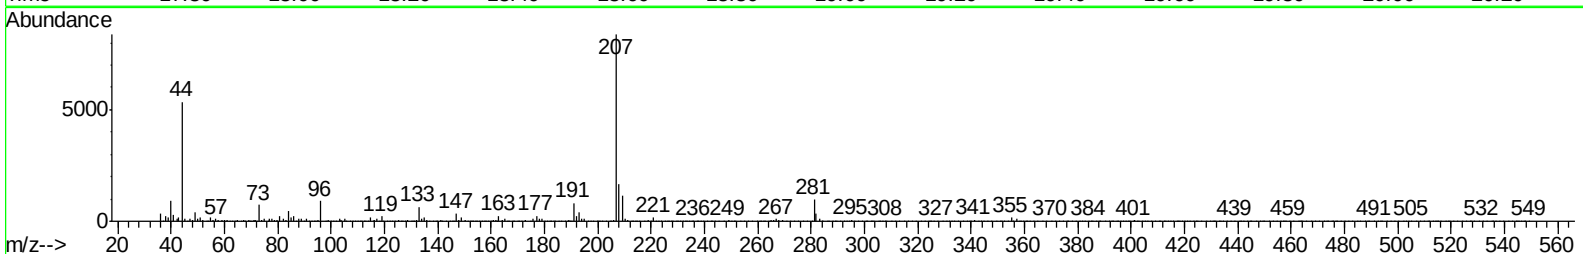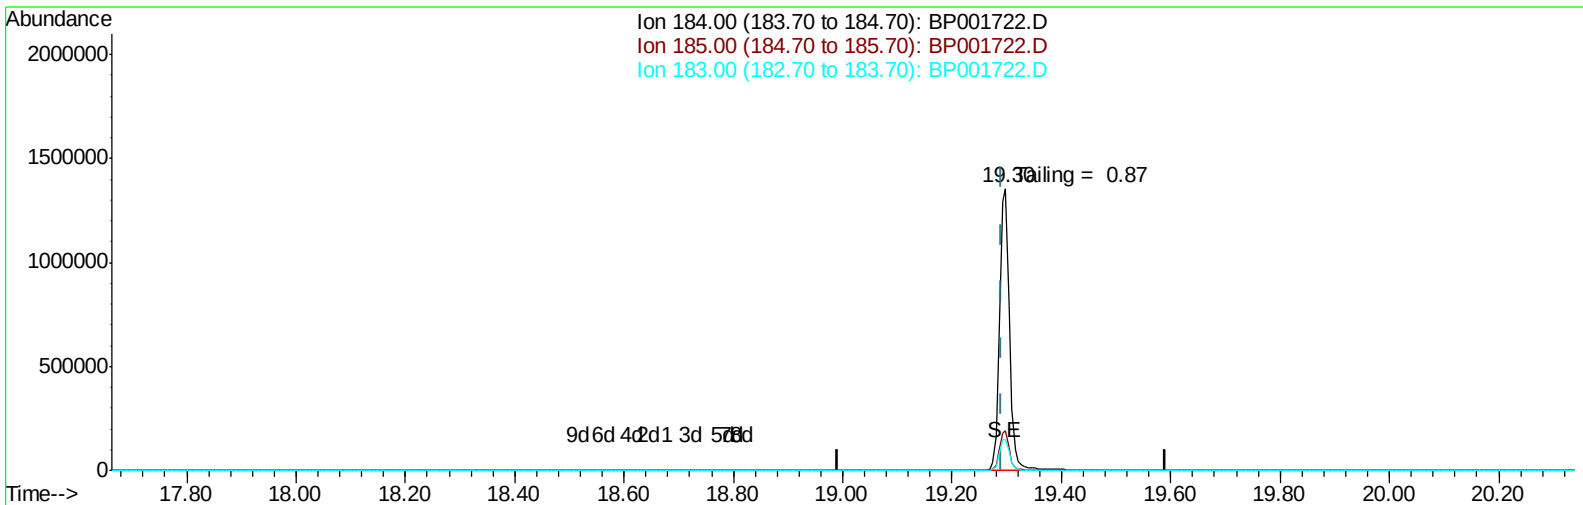

TIC: BP001722.D

(77) Benzidine

18.681min (-0.612) 0.03ng

response 10

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	85.00#
183.00	11.80	50.00#
0.00	0.00	0.00