
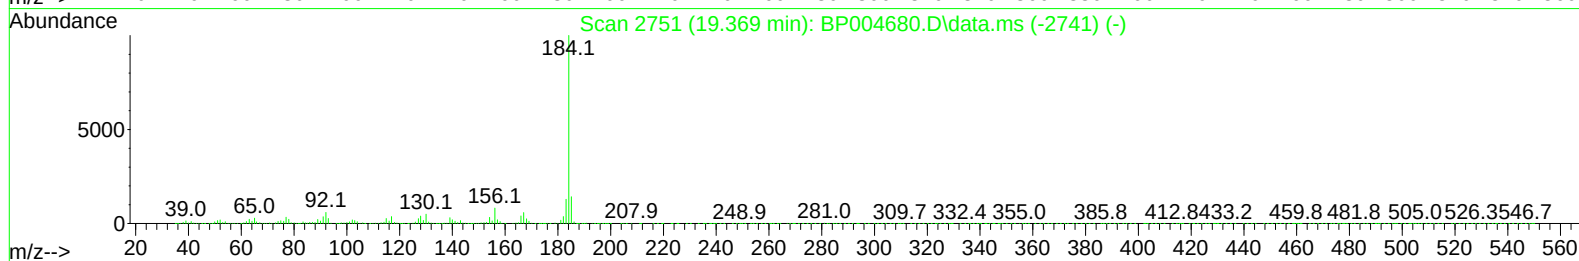
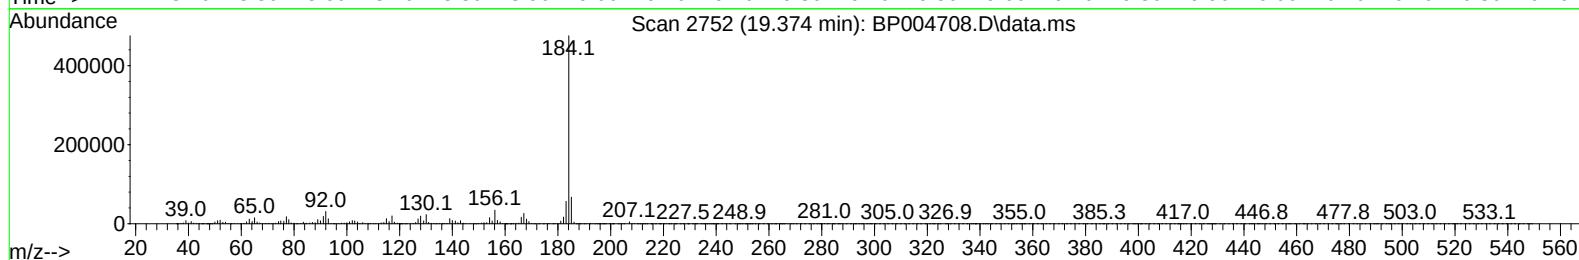


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021121\  
Data File : BP004708.D  
Acq On : 11 Feb 2021 09:06  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 11:17:22 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Feb 05 18:04:48 2021  
Response via : Initial Calibration

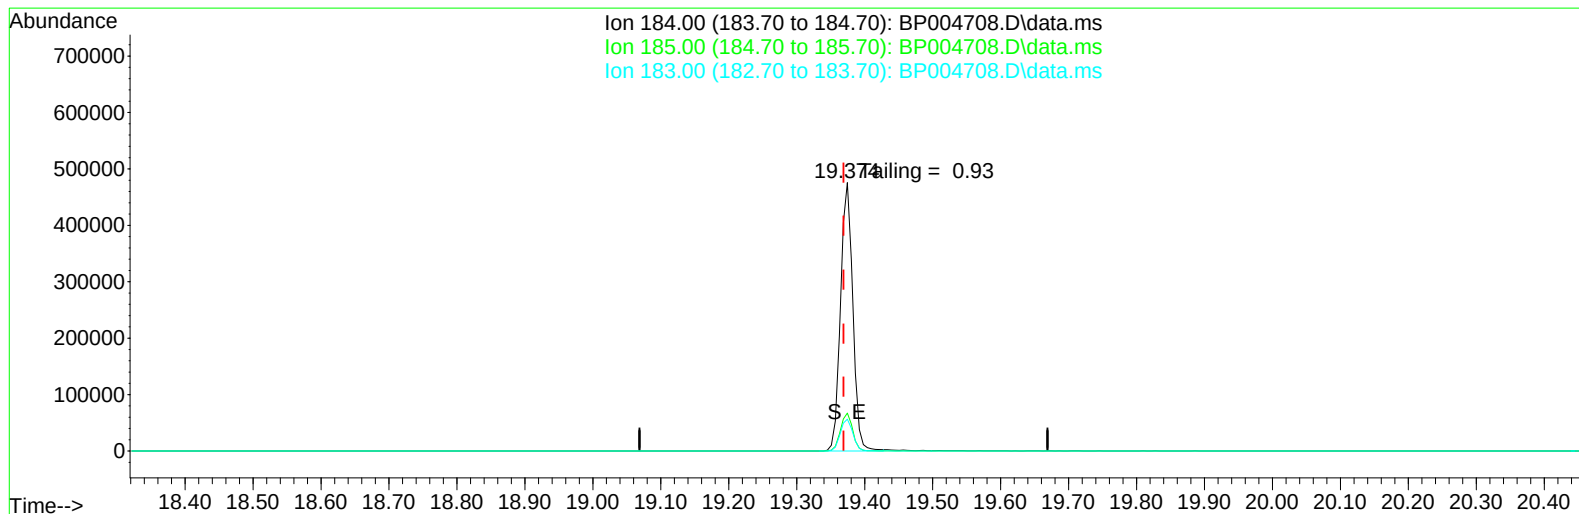

TIC: BP004708.D\data.ms

(77) Benzidine




19.374min (+ 0.005) 6989.26 ng

response 599900

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.15  |
| 183.00 | 12.00  | 11.90  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021121\  
 Data File : BP004708.D  
 Acq On : 11 Feb 2021 09:06  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 11:17:22 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Feb 05 18:04:48 2021  
 Response via : Initial Calibration

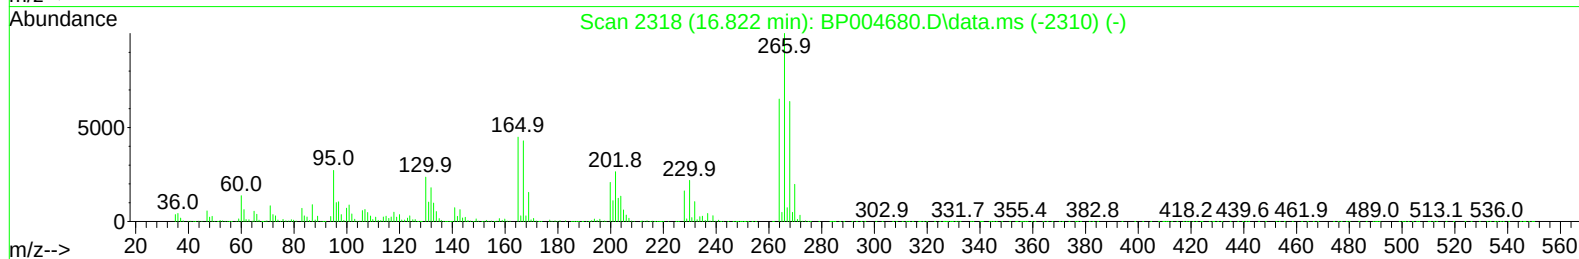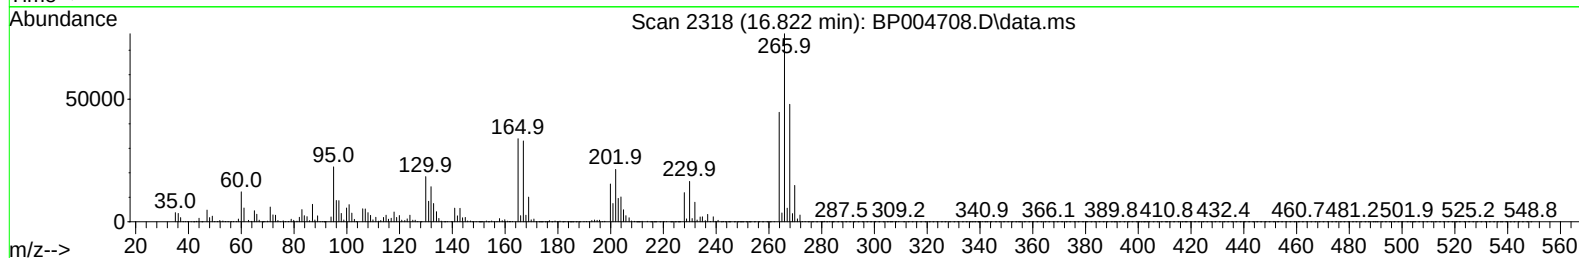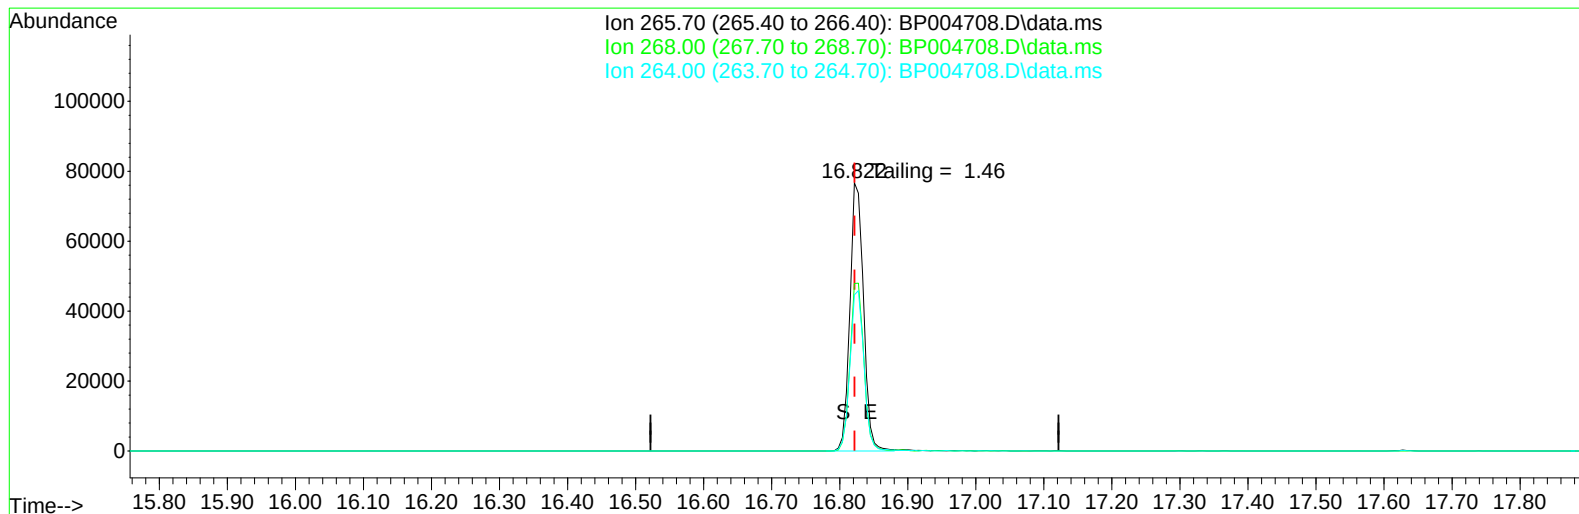

TIC: BP004708.D\data.ms

**(70) Pentachlorophenol (C)**

16.822min (-0.000) 110916.21 ng

response 106229

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.90  | 62.45  |
| 264.00 | 63.30  | 58.18  |
| 0.00   | 0.00   | 0.00   |